

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
 Data File : VV020513.D
 Acq On : 10 Mar 2021 22:13
 Operator : SY/MD
 Sample : M1632-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B57

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M

Title : VOC Analysis

Signal : TIC: VV020513.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	100	rVB	311864	315519	16.48%	2.111%
2	1.568	157	164	179	rBV	237803	270861	14.15%	1.812%
3	2.002	297	299	301	rBV2	614	341	0.02%	0.002%
4	2.108	321	332	369	rVB2	517821	804199	42.00%	5.381%
5	2.439	432	435	442	rVB3	289	298	0.02%	0.002%
6	2.516	451	459	465	rVB4	1383	2263	0.12%	0.015%
7	2.638	494	497	499	rBV	308	159	0.01%	0.001%
8	3.159	653	659	664	rBV2	166	207	0.01%	0.001%
9	3.195	664	670	672	rBV2	650	707	0.04%	0.005%
10	3.796	849	857	861	rVB2	229	293	0.02%	0.002%
11	3.905	878	891	932	rBV	115923	406227	21.22%	2.718%
12	4.352	1012	1030	1064	rBV	300002	760530	39.72%	5.089%
13	4.613	1101	1111	1119	rBV3	3094	5883	0.31%	0.039%
14	4.664	1125	1127	1131	rVB2	275	186	0.01%	0.001%
15	4.738	1147	1150	1153	rVB	466	273	0.01%	0.002%
16	4.777	1153	1162	1165	rBV2	173	277	0.01%	0.002%
17	4.918	1204	1206	1210	rVB	283	172	0.01%	0.001%
18	5.050	1227	1247	1275	rBV2	762624	1914668	100.00%	12.812%
19	5.265	1312	1314	1318	rBV3	344	214	0.01%	0.001%
20	5.362	1341	1344	1346	rBV2	249	162	0.01%	0.001%
21	5.420	1358	1362	1365	rBV3	425	349	0.02%	0.002%
22	5.461	1372	1375	1378	rBV2	235	192	0.01%	0.001%
23	5.490	1381	1384	1387	rBV2	305	273	0.01%	0.002%
24	5.526	1392	1395	1398	rVB2	306	197	0.01%	0.001%
25	5.551	1398	1403	1409	rBV2	278	259	0.01%	0.002%
26	5.619	1411	1424	1451	rBV	567166	1133357	59.19%	7.584%
27	5.908	1502	1514	1535	rBV2	64731	135773	7.09%	0.909%
28	6.011	1544	1546	1551	rVB2	480	305	0.02%	0.002%
29	6.072	1551	1565	1596	rBV	409214	828082	43.25%	5.541%
30	6.326	1640	1644	1646	rBV	275	176	0.01%	0.001%
31	6.506	1697	1700	1704	rBV2	311	222	0.01%	0.001%
32	6.889	1814	1819	1825	rBV2	139	199	0.01%	0.001%
33	6.989	1839	1850	1877	rBV	216298	391973	20.47%	2.623%
34	7.185	1909	1911	1913	rVB	319	151	0.01%	0.001%
35	7.207	1913	1918	1921	rBV2	339	324	0.02%	0.002%
36	7.233	1923	1926	1931	rVB3	290	228	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
 Data File : VV020513.D
 Acq On : 10 Mar 2021 22:13
 Operator : SY/MD
 Sample : M1632-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B57

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
 Title : VOC Analysis

37	7.320	1940	1953	1993	rBV	948861	1624633	84.85%	10.871%
38	7.625	2036	2048	2073	rBV	152876	268013	14.00%	1.793%
39	7.786	2095	2098	2104	rVB3	513	338	0.02%	0.002%
40	7.863	2118	2122	2125	rBV	215	215	0.01%	0.001%
41	7.953	2144	2150	2154	rVB4	612	808	0.04%	0.005%
42	7.985	2154	2160	2167	rBV5	536	591	0.03%	0.004%
43	8.095	2183	2194	2232	rBV2	408911	828626	43.28%	5.545%
44	8.445	2301	2303	2309	rVB3	282	157	0.01%	0.001%
45	8.500	2314	2320	2323	rBV2	277	335	0.02%	0.002%
46	8.603	2351	2352	2356	rBV	296	221	0.01%	0.001%
47	8.622	2356	2358	2361	rVV	472	269	0.01%	0.002%
48	8.641	2361	2364	2371	rVB2	565	565	0.03%	0.004%
49	8.802	2411	2414	2418	rBV2	261	202	0.01%	0.001%
50	8.857	2418	2431	2462	rBV	865984	1410064	73.65%	9.436%
51	9.085	2500	2502	2507	rVB3	234	222	0.01%	0.001%
52	9.156	2522	2524	2531	rVB4	284	248	0.01%	0.002%
53	9.207	2537	2540	2547	rVB2	249	154	0.01%	0.001%
54	9.268	2553	2559	2561	rBV2	180	214	0.01%	0.001%
55	9.391	2591	2597	2602	rBV2	217	252	0.01%	0.002%
56	9.458	2614	2618	2623	rBV2	270	321	0.02%	0.002%
57	9.558	2642	2649	2655	rBV2	260	412	0.02%	0.003%
58	9.648	2674	2677	2680	rVB	283	169	0.01%	0.001%
59	9.667	2680	2683	2688	rBV	258	187	0.01%	0.001%
60	9.709	2691	2696	2698	rVV	218	177	0.01%	0.001%
61	10.056	2801	2804	2812	rVB2	218	226	0.01%	0.002%
62	10.223	2843	2856	2878	rBV	532757	843476	44.05%	5.644%
63	10.391	2900	2908	2909	rBV	693	661	0.03%	0.004%
64	10.558	2956	2960	2963	rBV2	162	156	0.01%	0.001%
65	10.638	2982	2985	2989	rBV2	198	171	0.01%	0.001%
66	10.825	3039	3043	3045	rBV	244	182	0.01%	0.001%
67	10.895	3061	3065	3071	rBV	301	251	0.01%	0.002%
68	10.985	3089	3093	3098	rBV2	225	237	0.01%	0.002%
69	11.175	3147	3152	3157	rBV2	549	675	0.04%	0.005%
70	11.255	3165	3177	3198	rBV	915102	1392312	72.72%	9.317%
71	11.455	3235	3239	3242	rBV2	464	473	0.02%	0.003%
72	11.490	3246	3250	3255	rVB2	437	321	0.02%	0.002%
73	11.571	3273	3275	3278	rVB	411	170	0.01%	0.001%
74	11.632	3278	3294	3317	rBV	1016939	1585076	82.79%	10.607%
75	11.751	3329	3331	3335	rVB4	533	334	0.02%	0.002%
76	11.853	3361	3363	3366	rBV2	318	201	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
 Data File : VV020513.D
 Acq On : 10 Mar 2021 22:13
 Operator : SY/MD
 Sample : M1632-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B57

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M

Title : VOC Analysis

77	11.889	3371	3374	3378	rVB3	456	320	0.02%	0.002%
78	12.136	3446	3451	3454	rBV2	477	415	0.02%	0.003%
79	12.333	3507	3512	3513	rBV2	258	199	0.01%	0.001%
80	12.497	3558	3563	3566	rBV	345	286	0.01%	0.002%
81	12.747	3638	3641	3643	rBV2	345	247	0.01%	0.002%
82	12.847	3669	3672	3674	rVB2	341	177	0.01%	0.001%
83	12.960	3704	3707	3711	rBV2	275	152	0.01%	0.001%
84	13.005	3718	3721	3725	rBV2	322	263	0.01%	0.002%
85	13.053	3733	3736	3740	rBV2	362	274	0.01%	0.002%
86	13.088	3745	3747	3753	rVB3	296	217	0.01%	0.001%
87	13.117	3753	3756	3760	rBV	416	267	0.01%	0.002%
88	13.149	3760	3766	3767	rBV3	292	245	0.01%	0.002%
89	13.197	3779	3781	3787	rBV3	264	238	0.01%	0.002%
90	13.313	3814	3817	3819	rBV2	279	198	0.01%	0.001%
91	13.368	3831	3834	3839	rBV3	397	402	0.02%	0.003%
92	13.455	3858	3861	3862	rBV	281	187	0.01%	0.001%
93	13.506	3874	3877	3879	rBV	265	179	0.01%	0.001%
94	13.734	3945	3948	3950	rBV	295	189	0.01%	0.001%
95	13.821	3973	3975	3979	rVB2	319	177	0.01%	0.001%
96	14.500	4184	4186	4191	rVB2	448	192	0.01%	0.001%
97	14.763	4265	4268	4275	rBV3	378	398	0.02%	0.003%
98	14.824	4285	4287	4289	rBV	366	184	0.01%	0.001%
99	14.924	4316	4318	4321	rBV3	441	271	0.01%	0.002%
100	15.349	4447	4450	4454	rBV4	729	672	0.04%	0.004%




Sum of corrected areas: 14944163

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
Data File : VV020513.D
Acq On : 10 Mar 2021 22:13
Operator : SY/MD
Sample : M1632-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B57

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

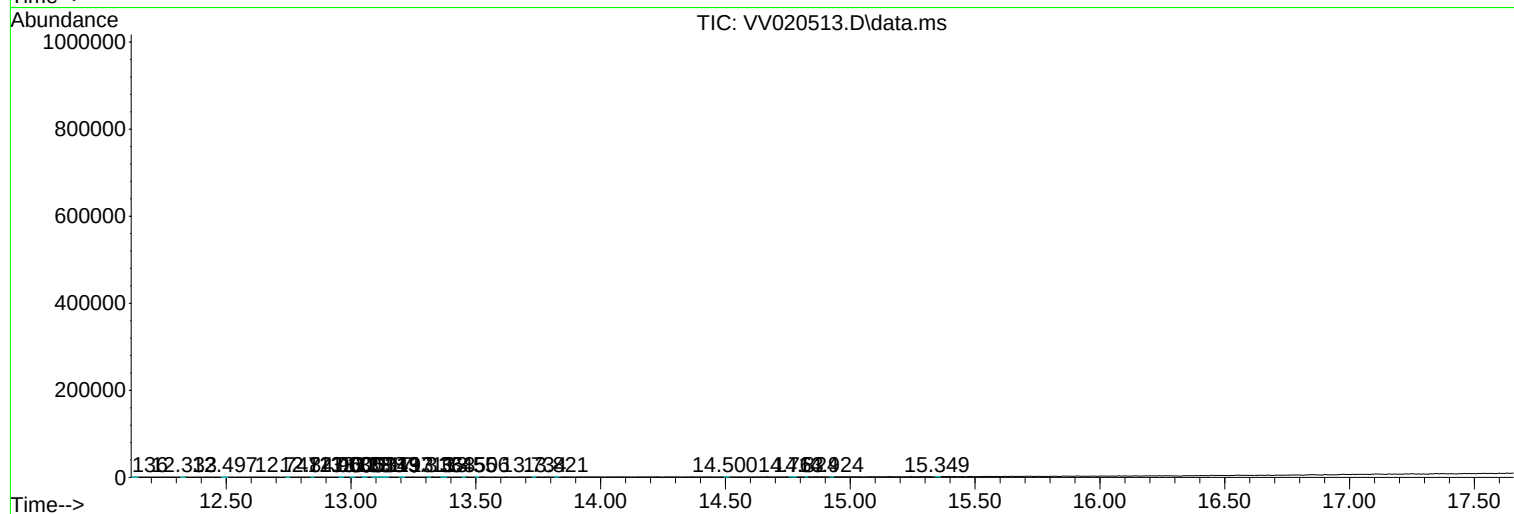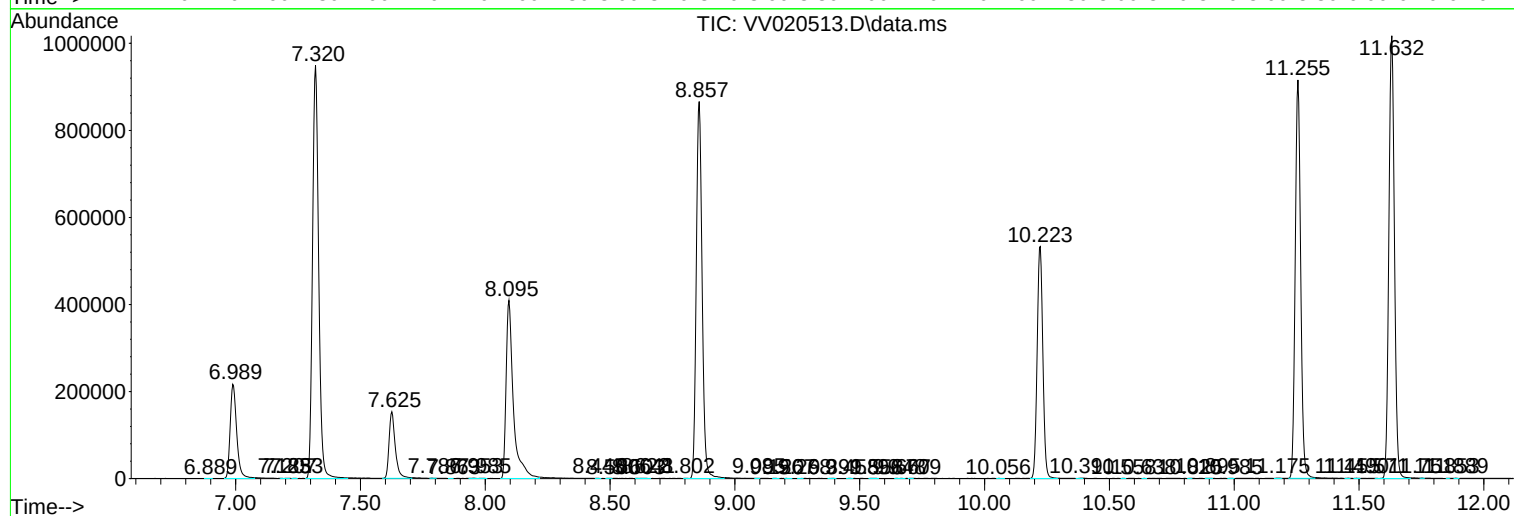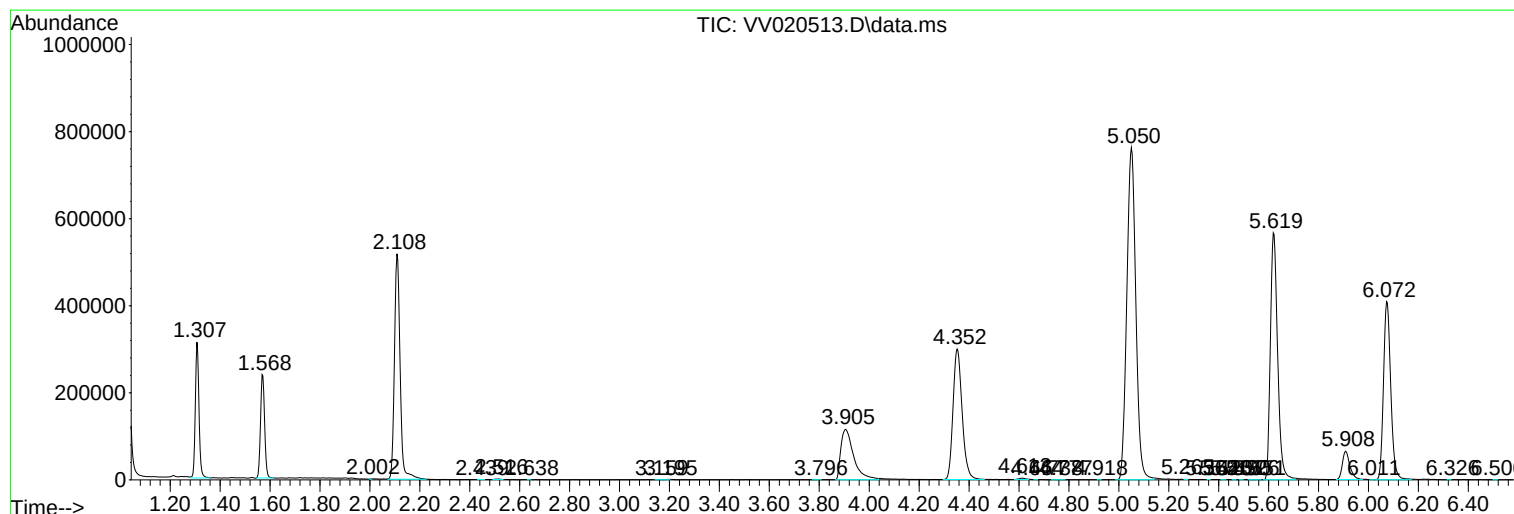

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
Data File : VV020513.D
Acq On : 10 Mar 2021 22:13
Operator : SY/MD
Sample : M1632-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B57

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
Data File : VV020513.D
Acq On : 10 Mar 2021 22:13
Operator : SY/MD
Sample : M1632-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B57

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
