

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
 Data File : VV020514.D
 Acq On : 10 Mar 2021 22:37
 Operator : SY/MD
 Sample : M1632-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B58

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M

Title : VOC Analysis

Signal : TIC: VV020514.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	98	rVB	313307	316415	16.42%	1.969%
2	1.568	156	164	180	rVB	238888	272779	14.16%	1.697%
3	2.108	321	332	372	rVB2	523111	810578	42.07%	5.044%
4	2.298	389	391	395	rVB2	537	350	0.02%	0.002%
5	2.330	395	401	402	rBV	188	195	0.01%	0.001%
6	2.468	441	444	446	rBV3	391	260	0.01%	0.002%
7	2.510	452	457	464	rVB7	1435	1903	0.10%	0.012%
8	2.616	487	490	493	rBV	482	353	0.02%	0.002%
9	2.963	593	598	602	rVV2	179	199	0.01%	0.001%
10	3.053	624	626	632	rBV2	179	176	0.01%	0.001%
11	3.124	645	648	651	rBV2	218	184	0.01%	0.001%
12	3.159	651	659	662	rVV2	236	292	0.02%	0.002%
13	3.185	663	667	668	rVV	294	154	0.01%	0.001%
14	3.208	672	674	679	rVB3	378	302	0.02%	0.002%
15	3.532	772	775	781	rVB2	159	192	0.01%	0.001%
16	3.905	878	891	936	rBV	112088	405010	21.02%	2.520%
17	4.230	987	992	994	rBV3	340	285	0.01%	0.002%
18	4.352	1013	1030	1062	rBV	302746	760994	39.50%	4.735%
19	4.613	1099	1111	1131	rVB2	10021	25324	1.31%	0.158%
20	4.690	1131	1135	1136	rBV2	275	188	0.01%	0.001%
21	4.847	1182	1184	1189	rVB3	212	166	0.01%	0.001%
22	4.883	1189	1195	1196	rBV2	313	306	0.02%	0.002%
23	4.918	1201	1206	1207	rBV	368	253	0.01%	0.002%
24	5.050	1229	1247	1289	rBV2	753768	1926584	100.00%	11.988%
25	5.297	1321	1324	1327	rVV	500	261	0.01%	0.002%
26	5.317	1327	1330	1332	rVB2	288	150	0.01%	0.001%
27	5.346	1337	1339	1343	rVB2	257	164	0.01%	0.001%
28	5.404	1354	1357	1359	rBV2	242	172	0.01%	0.001%
29	5.455	1368	1373	1377	rBV3	369	456	0.02%	0.003%
30	5.619	1412	1424	1456	rBV	572054	1150996	59.74%	7.162%
31	5.841	1491	1493	1497	rVB2	333	153	0.01%	0.001%
32	5.918	1501	1517	1549	rBV3	518135	1072015	55.64%	6.671%
33	6.072	1552	1565	1590	rVV	407042	826514	42.90%	5.143%
34	6.204	1604	1606	1607	rBV	567	216	0.01%	0.001%
35	6.214	1607	1609	1613	rVV3	549	457	0.02%	0.003%
36	6.317	1638	1641	1646	rBV3	368	230	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
 Data File : VV020514.D
 Acq On : 10 Mar 2021 22:37
 Operator : SY/MD
 Sample : M1632-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B58

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M

Title : VOC Analysis

37	6.410	1667	1670	1675	rVB2	272	210	0.01%	0.001%
38	6.805	1789	1793	1795	rBV2	169	166	0.01%	0.001%
39	6.924	1827	1830	1834	rVB2	226	155	0.01%	0.001%
40	6.989	1839	1850	1881	rBV	216834	398940	20.71%	2.482%
41	7.211	1916	1919	1921	rBV2	494	295	0.02%	0.002%
42	7.320	1940	1953	1982	rBV	970207	1655501	85.93%	10.301%
43	7.625	2037	2048	2067	rBV	155761	265710	13.79%	1.653%
44	7.751	2085	2087	2089	rVB	711	297	0.02%	0.002%
45	7.821	2106	2109	2115	rVV3	350	296	0.02%	0.002%
46	7.892	2128	2131	2137	rVB4	374	327	0.02%	0.002%
47	7.947	2140	2148	2157	rVB2	583	1081	0.06%	0.007%
48	7.985	2157	2160	2163	rBV	503	310	0.02%	0.002%
49	8.043	2174	2178	2183	rVB3	208	196	0.01%	0.001%
50	8.095	2183	2194	2228	rBV2	398028	809067	41.99%	5.034%
51	8.519	2324	2326	2329	rBV2	314	204	0.01%	0.001%
52	8.600	2345	2351	2354	rBV3	283	324	0.02%	0.002%
53	8.796	2409	2412	2419	rBV2	284	307	0.02%	0.002%
54	8.857	2419	2431	2461	rBV	887988	1443099	74.90%	8.980%
55	9.098	2503	2506	2509	rVB	519	219	0.01%	0.001%
56	9.162	2522	2526	2531	rVB3	277	252	0.01%	0.002%
57	9.384	2591	2595	2601	rVB2	262	264	0.01%	0.002%
58	9.529	2634	2640	2644	rBV2	262	266	0.01%	0.002%
59	9.889	2749	2752	2754	rBV	246	192	0.01%	0.001%
60	9.969	2774	2777	2782	rBV2	193	158	0.01%	0.001%
61	10.024	2791	2794	2800	rVB2	231	179	0.01%	0.001%
62	10.220	2838	2855	2878	rBV	533430	840530	43.63%	5.230%
63	10.387	2898	2907	2912	rVV3	688	1062	0.06%	0.007%
64	10.407	2912	2913	2915	rVB	553	210	0.01%	0.001%
65	10.529	2946	2951	2954	rVB2	253	242	0.01%	0.002%
66	10.548	2954	2957	2961	rBV	178	191	0.01%	0.001%
67	10.632	2977	2983	2985	rBV2	171	178	0.01%	0.001%
68	10.680	2995	2998	3003	rBV2	227	243	0.01%	0.002%
69	10.870	3052	3057	3059	rVB	251	191	0.01%	0.001%
70	10.976	3083	3090	3095	rBV2	240	377	0.02%	0.002%
71	11.108	3125	3131	3138	rBV2	231	402	0.02%	0.003%
72	11.181	3149	3154	3158	rVB	388	399	0.02%	0.002%
73	11.255	3165	3177	3204	rBV	937454	1440171	74.75%	8.961%
74	11.410	3223	3225	3228	rVB3	564	267	0.01%	0.002%
75	11.493	3248	3251	3253	rBV2	454	213	0.01%	0.001%
76	11.509	3253	3256	3258	rBV	240	150	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
 Data File : VV020514.D
 Acq On : 10 Mar 2021 22:37
 Operator : SY/MD
 Sample : M1632-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B58

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M

Title : VOC Analysis

77	11.548	3266	3268	3276	rVB4	487	525	0.03%	0.003%
78	11.583	3276	3279	3281	rBV2	283	163	0.01%	0.001%
79	11.632	3281	3294	3317	rBV	1040532	1626781	84.44%	10.123%
80	12.156	3454	3457	3460	rBV2	327	245	0.01%	0.002%
81	12.316	3505	3507	3511	rBV2	268	185	0.01%	0.001%
82	12.741	3636	3639	3642	rVB2	350	181	0.01%	0.001%
83	12.805	3656	3659	3663	rBV	165	155	0.01%	0.001%
84	13.014	3722	3724	3729	rVB2	271	227	0.01%	0.001%
85	13.069	3738	3741	3744	rVB3	311	158	0.01%	0.001%
86	13.104	3749	3752	3755	rBV	229	192	0.01%	0.001%
87	13.143	3761	3764	3766	rBV2	200	150	0.01%	0.001%
88	13.197	3779	3781	3783	rBV	407	280	0.01%	0.002%
89	13.262	3798	3801	3804	rBV2	254	194	0.01%	0.001%
90	13.336	3820	3824	3830	rBV	345	305	0.02%	0.002%
91	13.525	3880	3883	3886	rVB2	288	200	0.01%	0.001%
92	13.625	3910	3914	3918	rBV3	262	258	0.01%	0.002%
93	13.648	3918	3921	3923	rBV2	307	205	0.01%	0.001%
94	13.802	3965	3969	3972	rBV2	356	418	0.02%	0.003%
95	14.072	4051	4053	4058	rBV2	302	242	0.01%	0.002%
96	14.117	4065	4067	4071	rVB3	353	250	0.01%	0.002%
97	14.201	4090	4093	4097	rBV	304	295	0.02%	0.002%
98	14.805	4279	4281	4283	rBV3	446	240	0.01%	0.001%
99	15.326	4441	4443	4448	rVB2	614	256	0.01%	0.002%
100	15.882	4613	4616	4618	rBV2	1064	698	0.04%	0.004%


Sum of corrected areas: 16070870

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
Data File : VV020514.D
Acq On : 10 Mar 2021 22:37
Operator : SY/MD
Sample : M1632-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B58

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

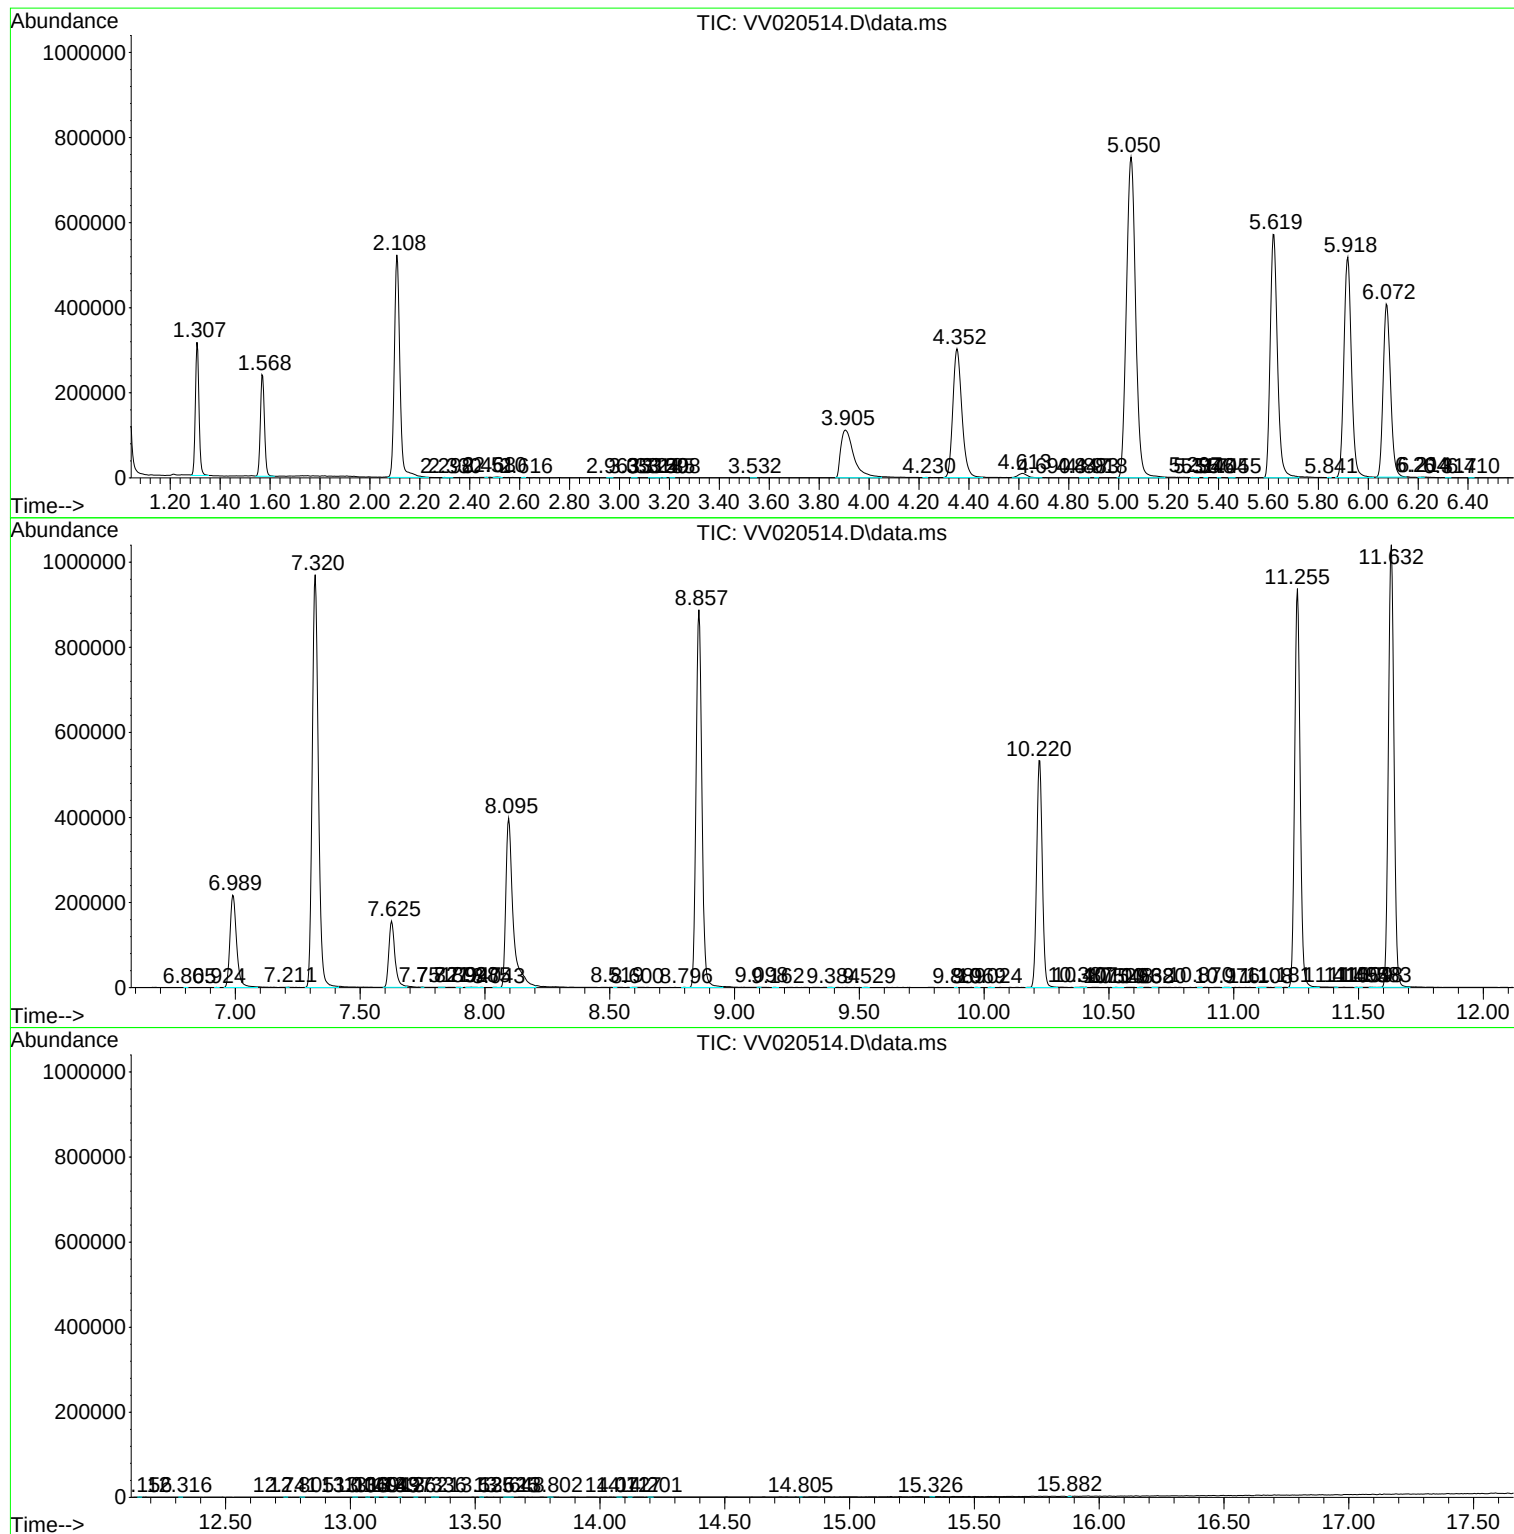

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
Data File : VV020514.D
Acq On : 10 Mar 2021 22:37
Operator : SY/MD
Sample : M1632-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B58

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
Data File : VV020514.D
Acq On : 10 Mar 2021 22:37
Operator : SY/MD
Sample : M1632-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B58

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
