

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
 Data File : VV020516.D
 Acq On : 10 Mar 2021 23:24
 Operator : SY/MD
 Sample : M1632-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B60

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M

Title : VOC Analysis

Signal : TIC: VV020516.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	105	rVB	307275	309614	16.27%	2.099%
2	1.571	156	165	177	rBV	231215	264697	13.91%	1.794%
3	2.028	304	307	308	rBV2	732	345	0.02%	0.002%
4	2.108	321	332	369	rVB	502381	750934	39.46%	5.091%
5	2.291	385	389	395	rVB4	416	515	0.03%	0.003%
6	2.442	432	436	439	rBV2	430	352	0.02%	0.002%
7	2.510	448	457	465	rVB5	1507	2378	0.12%	0.016%
8	2.619	489	491	494	rVB3	411	201	0.01%	0.001%
9	2.793	542	545	548	rBV2	210	161	0.01%	0.001%
10	2.847	560	562	570	rVV2	214	225	0.01%	0.002%
11	2.954	590	595	596	rBV	218	210	0.01%	0.001%
12	2.966	596	599	605	rVB2	370	325	0.02%	0.002%
13	3.532	769	775	779	rBV	210	270	0.01%	0.002%
14	3.622	801	803	808	rVB2	213	214	0.01%	0.001%
15	3.664	808	816	820	rVB2	266	305	0.02%	0.002%
16	3.799	854	858	861	rBV2	252	200	0.01%	0.001%
17	3.902	878	890	943	rBV	97720	343443	18.05%	2.328%
18	4.278	1004	1007	1009	rBV2	362	238	0.01%	0.002%
19	4.352	1013	1030	1065	rVV	296713	755099	39.68%	5.119%
20	4.642	1118	1120	1124	rVB	400	198	0.01%	0.001%
21	4.841	1179	1182	1188	rVB2	411	369	0.02%	0.003%
22	4.873	1188	1192	1195	rBV3	219	203	0.01%	0.001%
23	4.937	1207	1212	1216	rVB2	250	269	0.01%	0.002%
24	4.976	1216	1224	1227	rBV2	196	263	0.01%	0.002%
25	5.050	1227	1247	1272	rBV2	749481	1903086	100.00%	12.901%
26	5.481	1379	1381	1384	rVV3	340	264	0.01%	0.002%
27	5.500	1384	1387	1389	rVV2	454	275	0.01%	0.002%
28	5.622	1411	1425	1455	rBV	566593	1141811	60.00%	7.740%
29	5.828	1485	1489	1490	rBV2	273	175	0.01%	0.001%
30	5.857	1495	1498	1499	rBV2	357	197	0.01%	0.001%
31	5.908	1502	1514	1540	rVB2	59464	122808	6.45%	0.833%
32	6.072	1551	1565	1594	rBV	408942	824297	43.31%	5.588%
33	6.204	1604	1606	1610	rBV3	516	426	0.02%	0.003%
34	6.291	1630	1633	1640	rBV4	369	431	0.02%	0.003%
35	6.342	1643	1649	1651	rBV2	339	299	0.02%	0.002%
36	6.616	1731	1734	1737	rBV	299	195	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
 Data File : VV020516.D
 Acq On : 10 Mar 2021 23:24
 Operator : SY/MD
 Sample : M1632-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B60

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
 Title : VOC Analysis

37	6.658	1743	1747	1750	rBV2	263	202	0.01%	0.001%
38	6.728	1765	1769	1773	rBV2	179	173	0.01%	0.001%
39	6.777	1778	1784	1790	rVB2	164	227	0.01%	0.002%
40	6.915	1824	1827	1831	rVB2	255	177	0.01%	0.001%
41	6.989	1839	1850	1872	rBV	212499	389778	20.48%	2.642%
42	7.156	1899	1902	1908	rVB4	390	378	0.02%	0.003%
43	7.207	1916	1918	1922	rVB2	298	175	0.01%	0.001%
44	7.320	1940	1953	1972	rBV	960509	1624776	85.38%	11.014%
45	7.584	2033	2035	2037	rBV3	332	168	0.01%	0.001%
46	7.625	2037	2048	2074	rVV	150726	263776	13.86%	1.788%
47	7.860	2118	2121	2125	rBV2	368	258	0.01%	0.002%
48	7.931	2140	2143	2145	rBV	254	163	0.01%	0.001%
49	7.944	2145	2147	2151	rVV2	278	213	0.01%	0.001%
50	7.989	2158	2161	2165	rVB2	517	328	0.02%	0.002%
51	8.095	2183	2194	2231	rBV2	377831	778475	40.91%	5.277%
52	8.333	2265	2268	2272	rVB3	413	264	0.01%	0.002%
53	8.448	2301	2304	2307	rVB2	525	321	0.02%	0.002%
54	8.600	2348	2351	2354	rVB2	212	160	0.01%	0.001%
55	8.857	2419	2431	2464	rBV	882480	1423365	74.79%	9.649%
56	9.156	2518	2524	2526	rBV	422	293	0.02%	0.002%
57	9.204	2536	2539	2541	rBV	398	322	0.02%	0.002%
58	9.320	2572	2575	2582	rVB	368	291	0.02%	0.002%
59	9.352	2582	2585	2590	rBV3	370	339	0.02%	0.002%
60	9.577	2651	2655	2658	rBV	246	197	0.01%	0.001%
61	9.693	2688	2691	2695	rBV2	283	219	0.01%	0.001%
62	9.715	2695	2698	2701	rBV	250	194	0.01%	0.001%
63	10.034	2793	2797	2801	rBV	275	241	0.01%	0.002%
64	10.069	2806	2808	2815	rVB2	206	185	0.01%	0.001%
65	10.223	2840	2856	2877	rBV	522384	827348	43.47%	5.609%
66	10.387	2901	2907	2909	rBV3	692	592	0.03%	0.004%
67	10.590	2965	2970	2973	rBV2	233	242	0.01%	0.002%
68	10.641	2982	2986	2989	rBV2	255	221	0.01%	0.001%
69	10.744	3015	3018	3022	rBV	223	185	0.01%	0.001%
70	10.899	3064	3066	3071	rVB2	250	200	0.01%	0.001%
71	10.931	3071	3076	3079	rBV2	230	251	0.01%	0.002%
72	11.050	3109	3113	3117	rVB	275	204	0.01%	0.001%
73	11.104	3126	3130	3137	rBV2	232	323	0.02%	0.002%
74	11.165	3146	3149	3151	rBV2	317	178	0.01%	0.001%
75	11.255	3165	3177	3207	rBV	924996	1408053	73.99%	9.545%
76	11.632	3281	3294	3312	rBV	1027835	1595953	83.86%	10.819%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
 Data File : VV020516.D
 Acq On : 10 Mar 2021 23:24
 Operator : SY/MD
 Sample : M1632-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B60

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M

Title : VOC Analysis

77	11.789	3340	3343	3345	rBV2	441	258	0.01%	0.002%
78	11.899	3375	3377	3386	rVB	273	270	0.01%	0.002%
79	11.944	3387	3391	3393	rBV2	290	194	0.01%	0.001%
80	12.133	3448	3450	3453	rVB2	343	194	0.01%	0.001%
81	12.159	3453	3458	3461	rBV	277	278	0.01%	0.002%
82	12.217	3474	3476	3479	rBV	243	181	0.01%	0.001%
83	12.233	3479	3481	3486	rVB2	327	252	0.01%	0.002%
84	12.313	3502	3506	3508	rBV2	332	238	0.01%	0.002%
85	12.435	3540	3544	3547	rVB	382	289	0.02%	0.002%
86	12.525	3569	3572	3575	rBV2	224	186	0.01%	0.001%
87	12.551	3577	3580	3583	rVV2	428	312	0.02%	0.002%
88	12.603	3594	3596	3601	rVB2	247	202	0.01%	0.001%
89	12.696	3621	3625	3628	rBV	359	334	0.02%	0.002%
90	12.892	3684	3686	3693	rVB3	476	390	0.02%	0.003%
91	12.934	3697	3699	3704	rVB3	292	249	0.01%	0.002%
92	13.040	3728	3732	3737	rBV3	264	249	0.01%	0.002%
93	13.069	3738	3741	3744	rVB2	313	176	0.01%	0.001%
94	13.095	3746	3749	3752	rBV2	222	164	0.01%	0.001%
95	13.169	3770	3772	3774	rBV2	315	164	0.01%	0.001%
96	13.275	3801	3805	3808	rBV2	465	443	0.02%	0.003%
97	13.821	3972	3975	3979	rBV2	366	292	0.02%	0.002%
98	14.580	4209	4211	4220	rVB2	373	387	0.02%	0.003%
99	15.519	4500	4503	4506	rBV3	817	553	0.03%	0.004%
100	15.696	4556	4558	4563	rVB2	773	391	0.02%	0.003%


Sum of corrected areas: 14751346

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
Data File : VV020516.D
Acq On : 10 Mar 2021 23:24
Operator : SY/MD
Sample : M1632-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B60

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

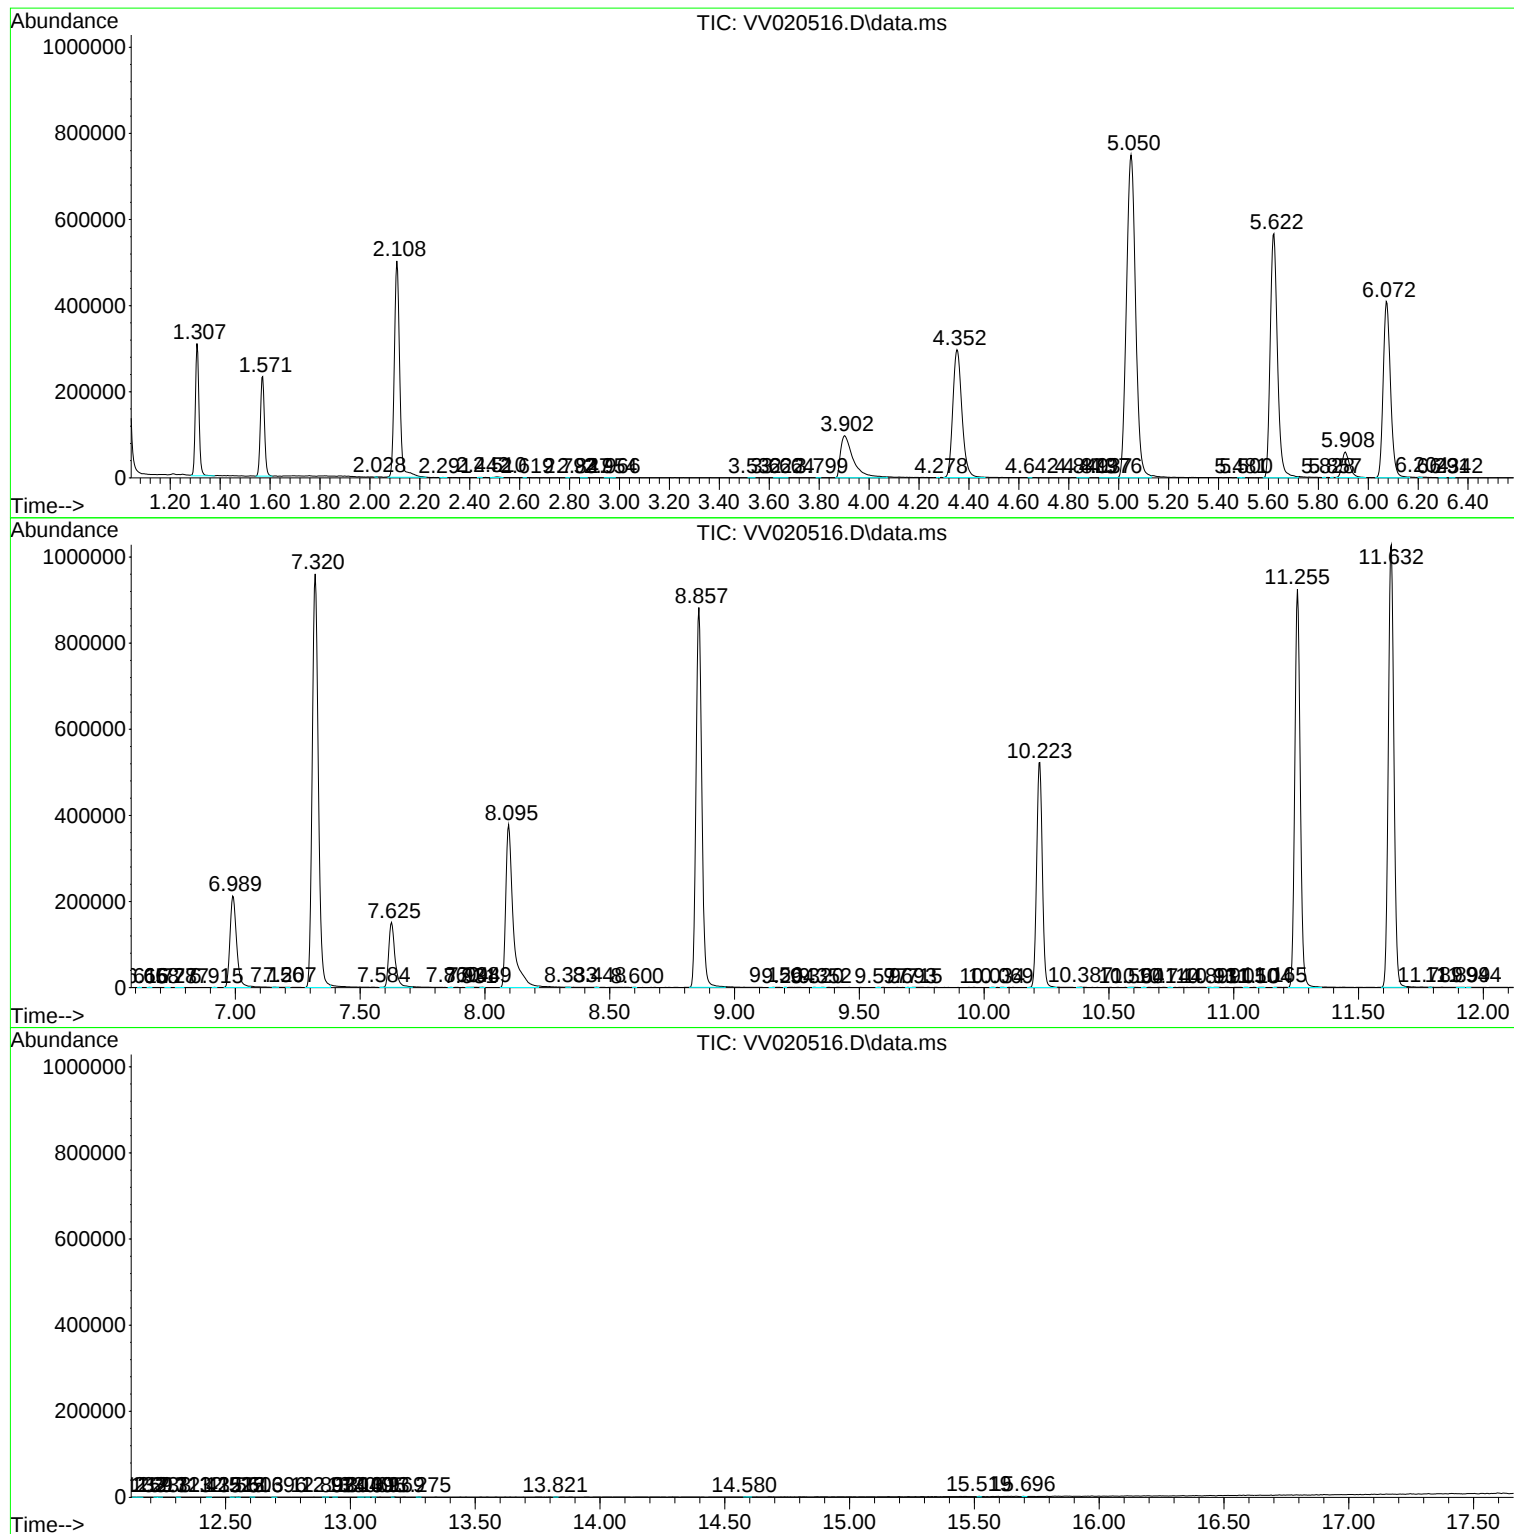

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
Data File : VV020516.D
Acq On : 10 Mar 2021 23:24
Operator : SY/MD
Sample : M1632-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B60

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
Data File : VV020516.D
Acq On : 10 Mar 2021 23:24
Operator : SY/MD
Sample : M1632-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B60

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
