

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
 Data File : VV020518.D
 Acq On : 11 Mar 2021 00:11
 Operator : SY/MD
 Sample : M1632-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B62

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M

Title : VOC Analysis

Signal : TIC: VV020518.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	98	rVB	310900	310354	16.24%	2.025%
2	1.571	157	165	179	rVB	236775	265686	13.91%	1.734%
3	2.111	321	333	371	rVB3	540657	886147	46.38%	5.782%
4	2.294	387	390	393	rVB2	698	498	0.03%	0.003%
5	2.330	398	401	406	rBV3	260	306	0.02%	0.002%
6	2.416	425	428	432	rBV3	309	251	0.01%	0.002%
7	2.510	452	457	458	rBV4	1040	861	0.05%	0.006%
8	2.584	478	480	483	rBV2	240	124	0.01%	0.001%
9	2.760	531	535	537	rVV2	493	307	0.02%	0.002%
10	2.777	537	540	542	rVV	429	222	0.01%	0.001%
11	2.796	542	546	549	rVB2	242	144	0.01%	0.001%
12	2.899	573	578	582	rBV2	333	405	0.02%	0.003%
13	2.924	583	586	592	rBV2	295	246	0.01%	0.002%
14	3.005	607	611	616	rBV2	155	153	0.01%	0.001%
15	3.130	647	650	654	rBV2	139	139	0.01%	0.001%
16	3.195	659	670	686	rVB3	3636	7915	0.41%	0.052%
17	3.265	686	692	694	rBV	167	165	0.01%	0.001%
18	3.674	815	819	822	rVV	277	221	0.01%	0.001%
19	3.912	878	893	927	rBV2	165220	545843	28.57%	3.561%
20	4.352	1013	1030	1062	rBV	301274	761130	39.84%	4.966%
21	4.503	1075	1077	1081	rVB2	423	234	0.01%	0.002%
22	4.616	1096	1112	1130	rVB2	26826	67925	3.56%	0.443%
23	4.699	1136	1138	1142	rBV3	313	227	0.01%	0.001%
24	4.821	1172	1176	1178	rBV3	426	186	0.01%	0.001%
25	5.050	1230	1247	1288	rBV2	749613	1910538	100.00%	12.466%
26	5.352	1339	1341	1346	rVB2	321	236	0.01%	0.002%
27	5.432	1361	1366	1369	rBV3	240	223	0.01%	0.001%
28	5.555	1401	1404	1411	rBV2	260	174	0.01%	0.001%
29	5.622	1411	1425	1448	rBV	570187	1146390	60.00%	7.480%
30	5.911	1501	1515	1544	rBV3	81522	192677	10.08%	1.257%
31	6.075	1551	1566	1588	rBV	404545	819708	42.90%	5.348%
32	6.268	1623	1626	1628	rVB2	327	186	0.01%	0.001%
33	6.284	1628	1631	1632	rBV2	240	137	0.01%	0.001%
34	6.548	1707	1713	1715	rBV2	150	144	0.01%	0.001%
35	6.606	1729	1731	1735	rVB2	313	213	0.01%	0.001%
36	6.632	1735	1739	1742	rBV2	206	178	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW031121\
 Data File : VW020518.D
 Acq On : 11 Mar 2021 00:11
 Operator : SY/MD
 Sample : M1632-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B62

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
 Title : VOC Analysis

37	6.654	1742	1746	1753	rBV	108	139	0.01%	0.001%
38	6.992	1837	1851	1877	rBV	213639	390221	20.42%	2.546%
39	7.198	1913	1915	1917	rBV3	217	123	0.01%	0.001%
40	7.246	1927	1930	1933	rVB	276	201	0.01%	0.001%
41	7.320	1941	1953	1985	rBV	950450	1625778	85.10%	10.608%
42	7.548	2023	2024	2028	rBV2	299	172	0.01%	0.001%
43	7.625	2038	2048	2068	rBV	151777	260526	13.64%	1.700%
44	7.818	2105	2108	2112	rVB3	398	332	0.02%	0.002%
45	7.854	2116	2119	2125	rVB5	398	369	0.02%	0.002%
46	7.944	2139	2147	2148	rBV2	482	534	0.03%	0.003%
47	8.095	2183	2194	2234	rBV2	409689	822762	43.06%	5.368%
48	8.452	2302	2305	2309	rVB3	355	264	0.01%	0.002%
49	8.477	2309	2313	2316	rBV2	219	190	0.01%	0.001%
50	8.519	2320	2326	2330	rVB3	279	213	0.01%	0.001%
51	8.677	2370	2375	2376	rBV	339	210	0.01%	0.001%
52	8.754	2395	2399	2402	rBV2	368	267	0.01%	0.002%
53	8.857	2419	2431	2462	rBV	892282	1435707	75.15%	9.368%
54	9.066	2495	2496	2499	rVB	268	128	0.01%	0.001%
55	9.107	2507	2509	2515	rVB2	499	398	0.02%	0.003%
56	9.358	2585	2587	2596	rVB2	231	206	0.01%	0.001%
57	9.497	2627	2630	2632	rBV	174	122	0.01%	0.001%
58	9.683	2684	2688	2690	rBV	235	204	0.01%	0.001%
59	9.796	2718	2723	2724	rBV	280	221	0.01%	0.001%
60	10.030	2791	2796	2799	rBV2	220	217	0.01%	0.001%
61	10.050	2799	2802	2805	rBV2	157	136	0.01%	0.001%
62	10.223	2843	2856	2877	rBV	538580	844343	44.19%	5.509%
63	10.387	2900	2907	2917	rBV2	805	1069	0.06%	0.007%
64	10.612	2974	2977	2980	rBV2	195	139	0.01%	0.001%
65	10.757	3018	3022	3026	rVB2	219	208	0.01%	0.001%
66	10.815	3033	3040	3045	rBV2	226	321	0.02%	0.002%
67	11.017	3100	3103	3107	rBV2	275	254	0.01%	0.002%
68	11.178	3150	3153	3157	rBV2	388	273	0.01%	0.002%
69	11.255	3164	3177	3204	rBV	935096	1422493	74.46%	9.281%
70	11.448	3235	3237	3240	rVB	298	170	0.01%	0.001%
71	11.468	3240	3243	3248	rVB2	571	493	0.03%	0.003%
72	11.496	3249	3252	3257	rBV2	396	273	0.01%	0.002%
73	11.519	3257	3259	3262	rBV2	227	147	0.01%	0.001%
74	11.632	3280	3294	3316	rBV	1016718	1590192	83.23%	10.376%
75	11.828	3351	3355	3356	rBV	259	164	0.01%	0.001%
76	11.902	3375	3378	3382	rBV2	203	124	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
 Data File : VV020518.D
 Acq On : 11 Mar 2021 00:11
 Operator : SY/MD
 Sample : M1632-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B62

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
 Title : VOC Analysis

77	11.982	3401	3403	3408	rVB2	371	294	0.02%	0.002%
78	12.098	3436	3439	3440	rBV	262	141	0.01%	0.001%
79	12.123	3445	3447	3451	rVB2	235	140	0.01%	0.001%
80	12.365	3519	3522	3527	rVB	288	218	0.01%	0.001%
81	12.390	3527	3530	3533	rBV	234	155	0.01%	0.001%
82	12.484	3556	3559	3561	rBV	231	138	0.01%	0.001%
83	12.718	3629	3632	3639	rBV2	195	275	0.01%	0.002%
84	12.754	3639	3643	3646	rVV2	211	201	0.01%	0.001%
85	12.850	3669	3673	3676	rBV3	378	345	0.02%	0.002%
86	12.889	3683	3685	3689	rVB2	225	134	0.01%	0.001%
87	13.107	3750	3753	3755	rVB2	305	153	0.01%	0.001%
88	13.123	3755	3758	3759	rBV	302	157	0.01%	0.001%
89	13.255	3793	3799	3801	rBV2	528	592	0.03%	0.004%
90	13.426	3849	3852	3859	rBV2	273	302	0.02%	0.002%
91	13.525	3881	3883	3888	rBV2	293	177	0.01%	0.001%
92	13.712	3938	3941	3943	rBV2	199	141	0.01%	0.001%
93	13.808	3969	3971	3973	rBV	235	128	0.01%	0.001%
94	13.969	4019	4021	4024	rBV2	284	214	0.01%	0.001%
95	14.217	4095	4098	4101	rBV3	287	212	0.01%	0.001%
96	14.818	4282	4285	4286	rBV	442	244	0.01%	0.002%
97	15.062	4359	4361	4362	rBV2	446	126	0.01%	0.001%
98	15.200	4402	4404	4407	rBV2	478	328	0.02%	0.002%
99	15.246	4415	4418	4422	rBV2	682	381	0.02%	0.002%
100	15.577	4519	4521	4524	rBV	898	411	0.02%	0.003%




Sum of corrected areas: 15326403

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
Data File : VV020518.D
Acq On : 11 Mar 2021 00:11
Operator : SY/MD
Sample : M1632-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B62

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

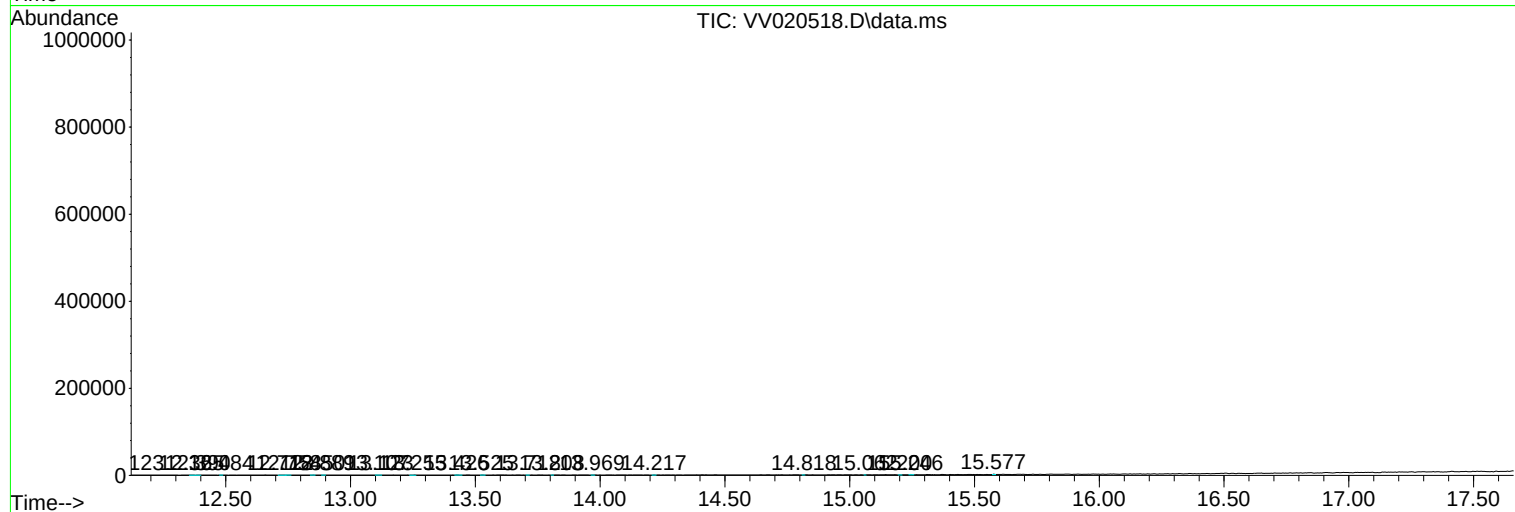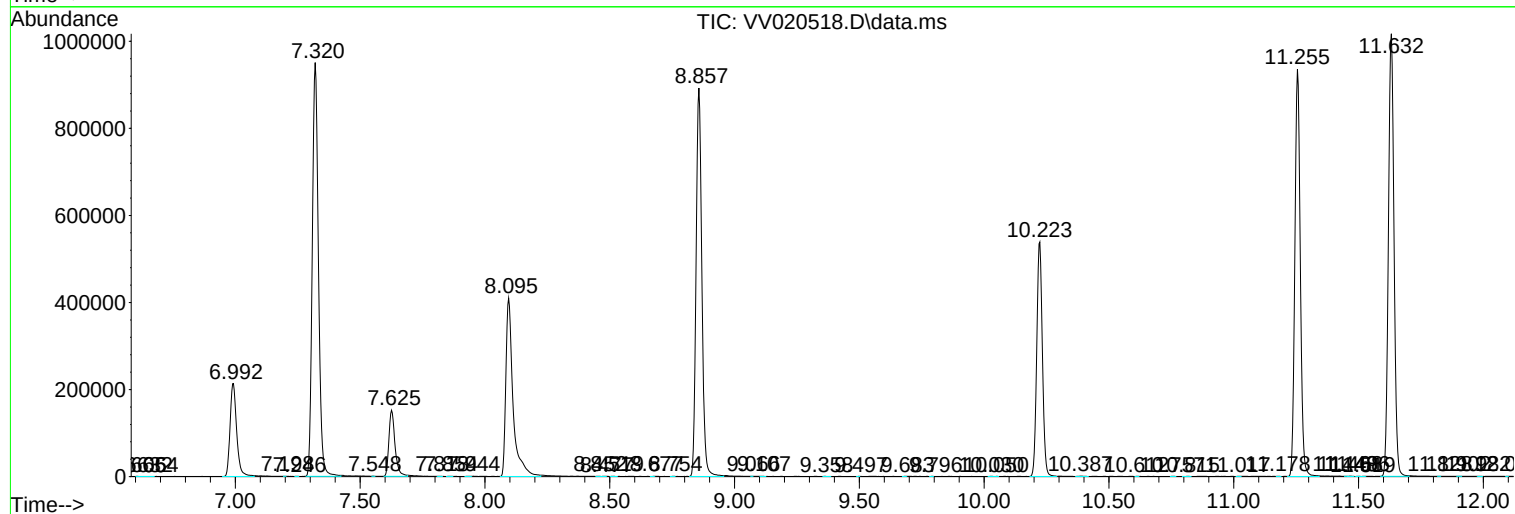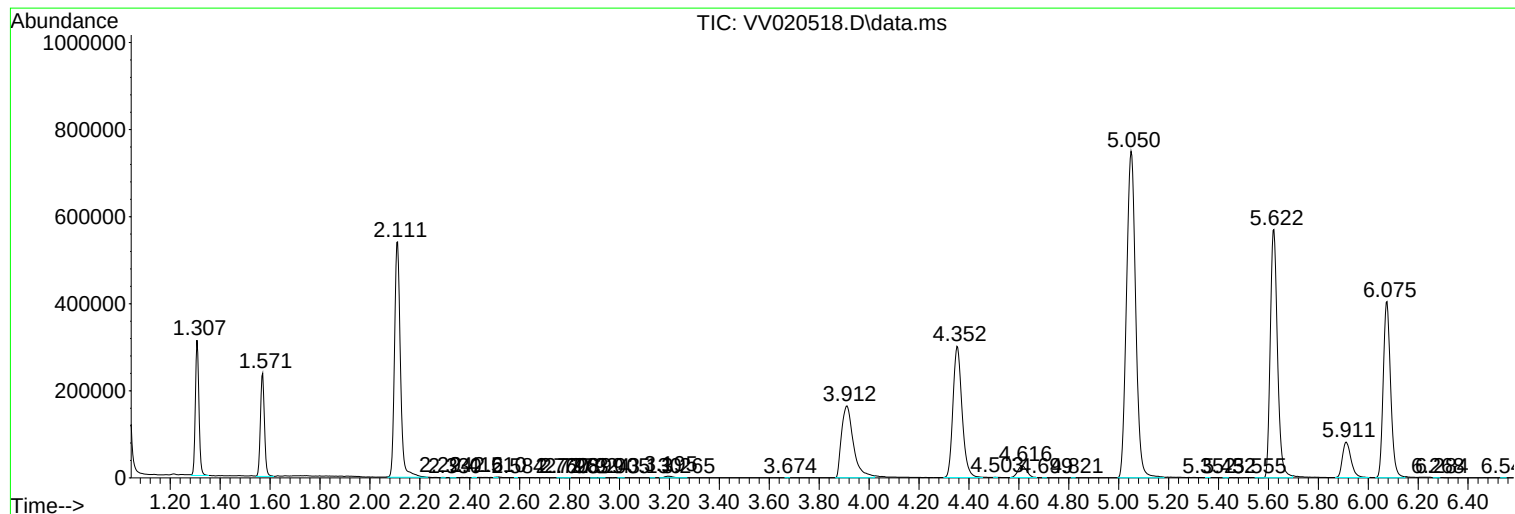

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
Data File : VV020518.D
Acq On : 11 Mar 2021 00:11
Operator : SY/MD
Sample : M1632-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B62

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
Data File : VV020518.D
Acq On : 11 Mar 2021 00:11
Operator : SY/MD
Sample : M1632-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B62

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
