

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
 Data File : VV020519.D
 Acq On : 11 Mar 2021 00:35
 Operator : SY/MD
 Sample : M1632-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B63

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M

Title : VOC Analysis

Signal : TIC: VV020519.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	103	rVB	298969	301450	16.15%	2.079%
2	1.571	157	165	183	rVB	224727	257721	13.81%	1.777%
3	2.034	307	309	313	rBV3	557	430	0.02%	0.003%
4	2.108	322	332	378	rVB	481152	730048	39.11%	5.034%
5	2.291	386	389	395	rBV4	405	436	0.02%	0.003%
6	2.497	451	453	455	rBV3	438	280	0.02%	0.002%
7	2.577	476	478	481	rVB2	276	155	0.01%	0.001%
8	2.738	525	528	531	rBV	274	248	0.01%	0.002%
9	2.825	553	555	561	rVB	390	285	0.02%	0.002%
10	2.857	561	565	570	rBV2	173	206	0.01%	0.001%
11	2.928	582	587	590	rVB	221	217	0.01%	0.001%
12	2.953	590	595	598	rBV	310	305	0.02%	0.002%
13	3.124	641	648	651	rBV2	180	198	0.01%	0.001%
14	3.294	697	701	705	rVB2	280	250	0.01%	0.002%
15	3.326	705	711	713	rBV2	262	203	0.01%	0.001%
16	3.365	717	723	730	rBV2	176	243	0.01%	0.002%
17	3.632	802	806	809	rBV2	237	222	0.01%	0.002%
18	3.683	816	822	824	rBV2	217	219	0.01%	0.002%
19	3.902	879	890	930	rBV	92172	325113	17.42%	2.242%
20	4.352	1013	1030	1063	rBV2	288315	732880	39.26%	5.053%
21	4.584	1100	1102	1107	rBV3	374	268	0.01%	0.002%
22	4.674	1126	1130	1132	rBV	363	273	0.01%	0.002%
23	4.696	1135	1137	1142	rVB	358	290	0.02%	0.002%
24	4.757	1153	1156	1159	rBV	217	155	0.01%	0.001%
25	4.831	1177	1179	1184	rVB2	292	188	0.01%	0.001%
26	5.050	1229	1247	1286	rBV2	736709	1866563	100.00%	12.871%
27	5.384	1346	1351	1353	rBV2	263	228	0.01%	0.002%
28	5.413	1356	1360	1362	rVB3	426	287	0.02%	0.002%
29	5.429	1362	1365	1367	rBV2	388	241	0.01%	0.002%
30	5.481	1376	1381	1383	rBV	441	342	0.02%	0.002%
31	5.619	1412	1424	1456	rBV	564247	1131875	60.64%	7.805%
32	5.912	1503	1515	1537	rBV3	66351	145600	7.80%	1.004%
33	6.072	1550	1565	1596	rBV	397031	803121	43.03%	5.538%
34	6.198	1602	1604	1605	rBV2	371	168	0.01%	0.001%
35	6.281	1628	1630	1633	rVB2	365	184	0.01%	0.001%
36	6.317	1638	1641	1645	rVB2	225	209	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW031121\
 Data File : VW020519.D
 Acq On : 11 Mar 2021 00:35
 Operator : SY/MD
 Sample : M1632-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B63

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
 Title : VOC Analysis

37	6.600	1726	1729	1732	rBV2	197	155	0.01%	0.001%
38	6.693	1752	1758	1760	rBV	163	155	0.01%	0.001%
39	6.940	1830	1835	1839	rBV	204	254	0.01%	0.002%
40	6.989	1839	1850	1881	rBV	207990	376884	20.19%	2.599%
41	7.169	1904	1906	1914	rVB4	424	372	0.02%	0.003%
42	7.320	1941	1953	1986	rBV	933291	1598987	85.66%	11.026%
43	7.625	2038	2048	2078	rVV	145978	254467	13.63%	1.755%
44	7.857	2117	2120	2123	rBV2	234	185	0.01%	0.001%
45	7.889	2126	2130	2133	rVV2	398	323	0.02%	0.002%
46	7.934	2139	2144	2145	rVV3	272	220	0.01%	0.002%
47	7.944	2145	2147	2156	rVV3	523	511	0.03%	0.004%
48	7.985	2159	2160	2164	rBV2	327	154	0.01%	0.001%
49	8.095	2183	2194	2235	rBV2	363936	749271	40.14%	5.167%
50	8.468	2307	2310	2315	rVB3	255	194	0.01%	0.001%
51	8.500	2315	2320	2323	rBV2	224	267	0.01%	0.002%
52	8.693	2377	2380	2385	rBV2	209	171	0.01%	0.001%
53	8.738	2388	2394	2397	rBV2	195	268	0.01%	0.002%
54	8.792	2406	2411	2414	rBV2	223	237	0.01%	0.002%
55	8.857	2418	2431	2460	rBV	884407	1411231	75.61%	9.731%
56	9.140	2517	2519	2523	rVB	367	192	0.01%	0.001%
57	9.178	2528	2531	2535	rBV2	263	195	0.01%	0.001%
58	9.461	2616	2619	2623	rVB2	224	152	0.01%	0.001%
59	9.564	2644	2651	2652	rBV2	283	272	0.01%	0.002%
60	9.760	2708	2712	2715	rBV2	224	190	0.01%	0.001%
61	9.847	2736	2739	2743	rVB	317	265	0.01%	0.002%
62	9.873	2743	2747	2749	rBV2	309	272	0.01%	0.002%
63	9.963	2769	2775	2777	rBV2	198	211	0.01%	0.001%
64	10.223	2837	2856	2879	rBV	503150	799593	42.84%	5.513%
65	10.355	2894	2897	2902	rVB2	219	208	0.01%	0.001%
66	10.381	2902	2905	2911	rBV2	437	545	0.03%	0.004%
67	10.458	2925	2929	2932	rBV2	233	246	0.01%	0.002%
68	10.509	2940	2945	2949	rBV	332	344	0.02%	0.002%
69	10.603	2966	2974	2979	rBV2	403	671	0.04%	0.005%
70	10.709	3003	3007	3010	rBV3	475	467	0.03%	0.003%
71	11.034	3106	3108	3113	rVB2	275	152	0.01%	0.001%
72	11.207	3159	3162	3165	rBV	274	207	0.01%	0.001%
73	11.255	3165	3177	3205	rBV	905955	1388414	74.38%	9.574%
74	11.535	3260	3264	3266	rBV3	239	234	0.01%	0.002%
75	11.632	3280	3294	3317	rBV	989219	1558115	83.48%	10.744%
76	11.947	3386	3392	3395	rBV	243	293	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
 Data File : VV020519.D
 Acq On : 11 Mar 2021 00:35
 Operator : SY/MD
 Sample : M1632-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B63

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
 Title : VOC Analysis

77	12.005	3404	3410	3419	rBV7	2992	4017	0.22%	0.028%
78	12.249	3480	3486	3494	rVB3	1195	1799	0.10%	0.012%
79	12.345	3513	3516	3519	rBV	207	162	0.01%	0.001%
80	12.365	3520	3522	3527	rVB2	406	301	0.02%	0.002%
81	12.429	3539	3542	3546	rBV2	240	186	0.01%	0.001%
82	12.644	3606	3609	3612	rBV	299	204	0.01%	0.001%
83	12.837	3666	3669	3673	rBV2	159	163	0.01%	0.001%
84	13.017	3722	3725	3727	rBV2	352	185	0.01%	0.001%
85	13.114	3747	3755	3758	rBV2	402	508	0.03%	0.004%
86	13.246	3793	3796	3801	rVB2	385	222	0.01%	0.002%
87	13.320	3816	3819	3823	rBV2	202	203	0.01%	0.001%
88	13.342	3823	3826	3831	rVB3	329	345	0.02%	0.002%
89	13.439	3853	3856	3860	rBV3	273	252	0.01%	0.002%
90	13.467	3860	3865	3870	rVB2	336	404	0.02%	0.003%
91	13.898	3996	3999	4004	rBB2	328	262	0.01%	0.002%
92	14.069	4050	4052	4057	rVB2	432	226	0.01%	0.002%
93	14.146	4073	4076	4084	rVB3	506	626	0.03%	0.004%
94	14.413	4149	4159	4170	rVB6	26988	43042	2.31%	0.297%
95	14.606	4216	4219	4226	rVB4	1205	1264	0.07%	0.009%
96	14.734	4257	4259	4261	rBV	546	187	0.01%	0.001%
97	15.307	4435	4437	4438	rBV	662	328	0.02%	0.002%
98	15.451	4480	4482	4484	rBV2	674	336	0.02%	0.002%
99	15.545	4509	4511	4512	rBV	446	210	0.01%	0.001%
100	15.644	4540	4542	4545	rBV2	670	408	0.02%	0.003%


Sum of corrected areas: 14502485

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
Data File : VV020519.D
Acq On : 11 Mar 2021 00:35
Operator : SY/MD
Sample : M1632-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B63

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

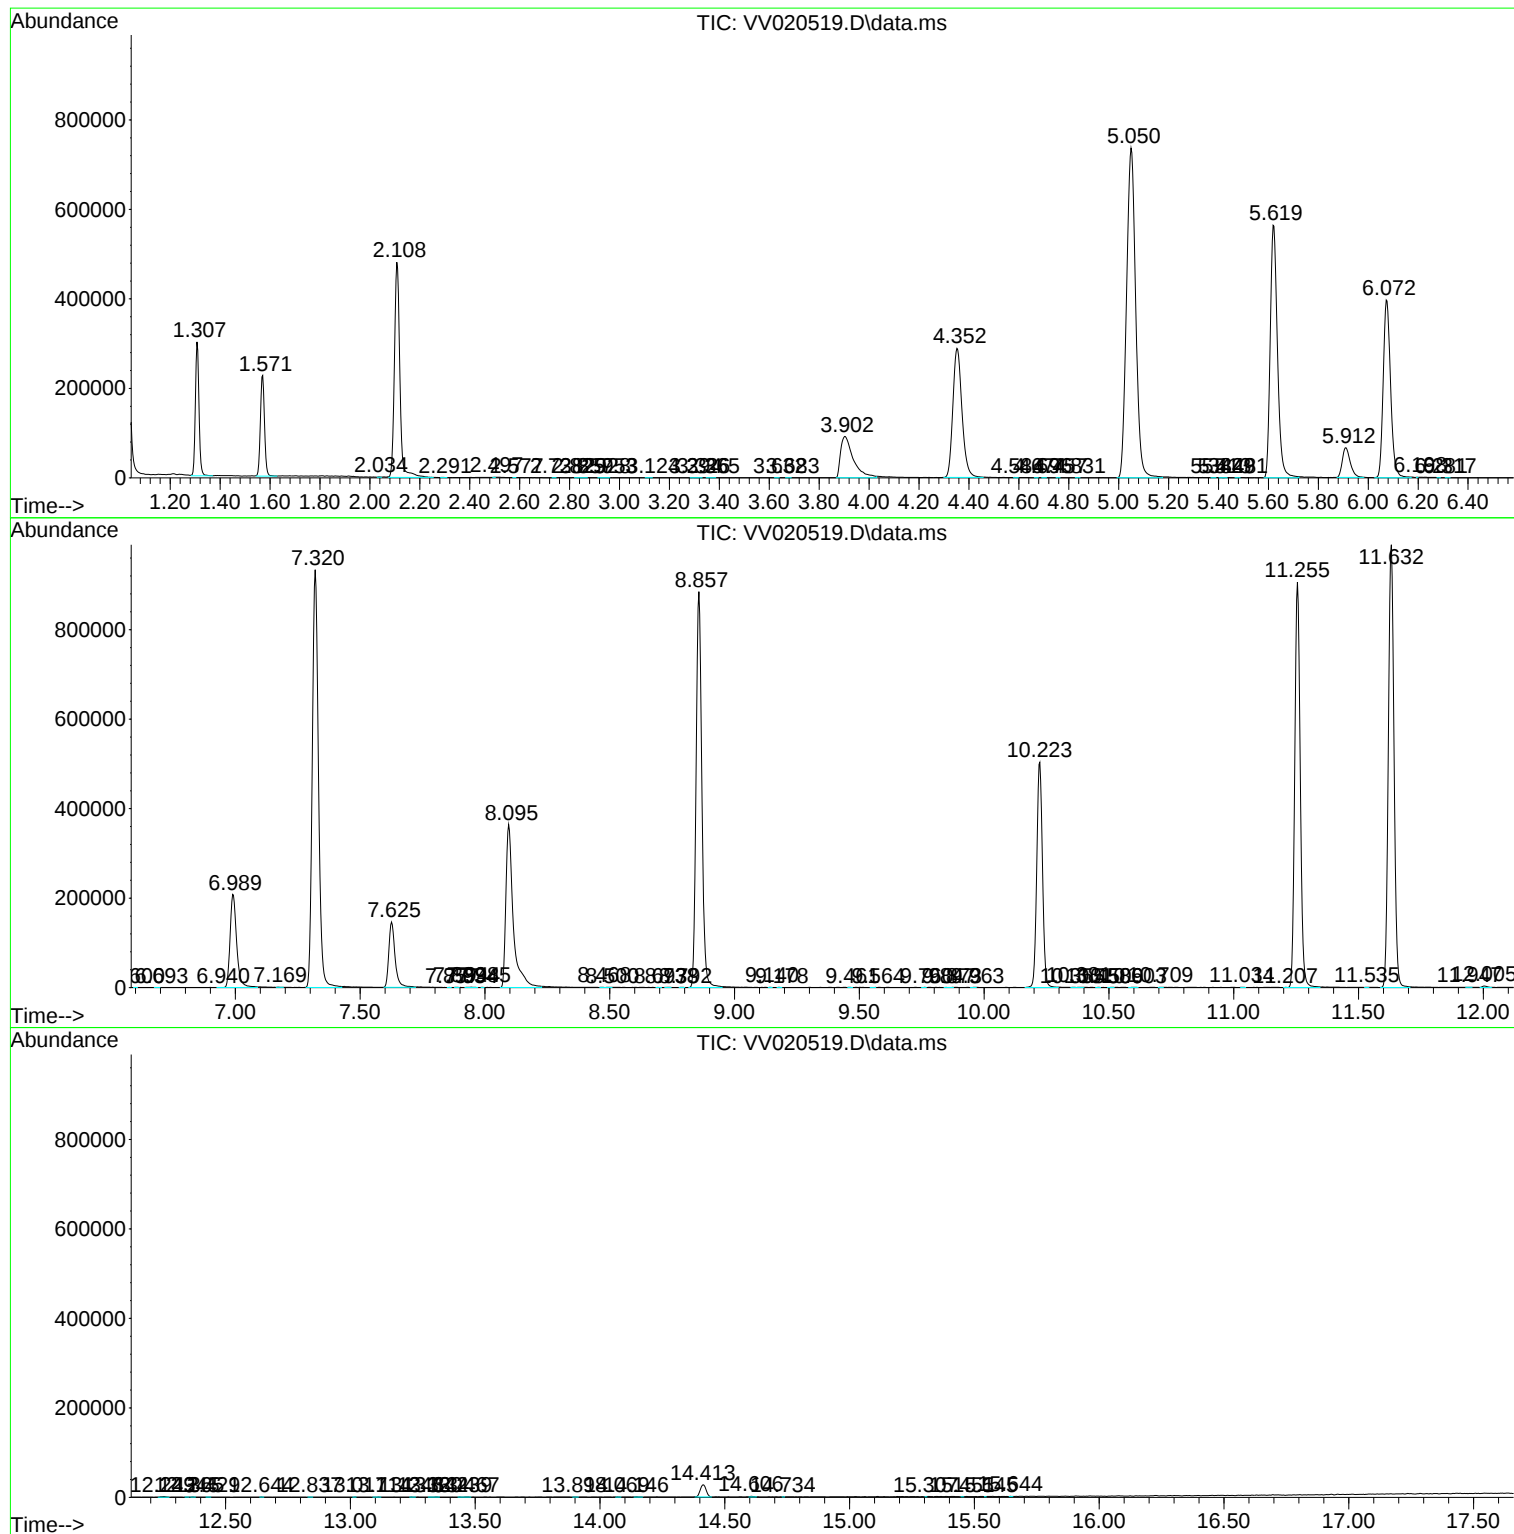

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
Data File : VV020519.D
Acq On : 11 Mar 2021 00:35
Operator : SY/MD
Sample : M1632-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B63

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
Data File : VV020519.D
Acq On : 11 Mar 2021 00:35
Operator : SY/MD
Sample : M1632-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B63

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
