

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
 Data File : VV020520.D
 Acq On : 11 Mar 2021 00:58
 Operator : SY/MD
 Sample : M1632-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B64

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M

Title : VOC Analysis

Signal : TIC: VV020520.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	102	rVB	309552	311478	16.29%	2.113%
2	1.568	157	164	177	rVB	232042	264679	13.85%	1.795%
3	2.108	320	332	378	rVB	504118	759939	39.75%	5.154%
4	2.291	386	389	391	rBV2	365	223	0.01%	0.002%
5	2.320	396	398	401	rBV3	347	229	0.01%	0.002%
6	2.423	427	430	432	rVB2	414	224	0.01%	0.002%
7	2.471	443	445	449	rBV	343	274	0.01%	0.002%
8	2.516	453	459	462	rVV4	810	861	0.05%	0.006%
9	2.667	501	506	510	rVB4	351	323	0.02%	0.002%
10	2.722	519	523	525	rVB	295	172	0.01%	0.001%
11	2.809	545	550	553	rBV	192	163	0.01%	0.001%
12	3.073	629	632	635	rBV2	248	168	0.01%	0.001%
13	3.146	651	655	658	rBV2	210	164	0.01%	0.001%
14	3.294	695	701	705	rBV2	238	240	0.01%	0.002%
15	3.343	712	716	721	rVB2	164	200	0.01%	0.001%
16	3.394	728	732	735	rVB2	203	157	0.01%	0.001%
17	3.471	753	756	759	rBV	195	155	0.01%	0.001%
18	3.513	766	769	771	rBV	235	157	0.01%	0.001%
19	3.552	777	781	787	rVB	257	278	0.01%	0.002%
20	3.638	803	808	818	rVB2	276	362	0.02%	0.002%
21	3.738	836	839	843	rVB2	217	211	0.01%	0.001%
22	3.799	855	858	861	rBV2	293	196	0.01%	0.001%
23	3.902	873	890	937	rBV2	97815	347988	18.20%	2.360%
24	4.352	1010	1030	1061	rBV	301663	756899	39.59%	5.134%
25	4.638	1115	1119	1120	rVV	335	195	0.01%	0.001%
26	4.658	1120	1125	1129	rVV3	281	329	0.02%	0.002%
27	4.677	1129	1131	1135	rVV2	331	279	0.01%	0.002%
28	4.712	1139	1142	1146	rVB2	313	183	0.01%	0.001%
29	4.757	1151	1156	1161	rVB3	385	315	0.02%	0.002%
30	5.050	1228	1247	1286	rBV2	757462	1911611	100.00%	12.966%
31	5.346	1333	1339	1343	rBV4	477	625	0.03%	0.004%
32	5.381	1348	1350	1357	rVB3	232	170	0.01%	0.001%
33	5.568	1403	1408	1411	rBV2	234	317	0.02%	0.002%
34	5.619	1412	1424	1449	rBV	562462	1129593	59.09%	7.662%
35	5.822	1485	1487	1490	rBV2	356	212	0.01%	0.001%
36	5.908	1502	1514	1538	rBV2	58228	121793	6.37%	0.826%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
 Data File : VV020520.D
 Acq On : 11 Mar 2021 00:58
 Operator : SY/MD
 Sample : M1632-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B64

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
 Title : VOC Analysis

37	6.072	1552	1565	1595	rBV	406742	818627	42.82%	5.552%
38	6.217	1607	1610	1614	rVB6	1066	761	0.04%	0.005%
39	6.391	1662	1664	1669	rVB2	635	395	0.02%	0.003%
40	6.433	1674	1677	1682	rVB	254	214	0.01%	0.001%
41	6.571	1714	1720	1723	rBV	157	170	0.01%	0.001%
42	6.667	1744	1750	1752	rVV2	153	169	0.01%	0.001%
43	6.683	1752	1755	1764	rVB2	316	327	0.02%	0.002%
44	6.822	1794	1798	1803	rVB2	220	207	0.01%	0.001%
45	6.989	1839	1850	1878	rBV	211079	388036	20.30%	2.632%
46	7.150	1898	1900	1903	rBV2	321	174	0.01%	0.001%
47	7.214	1917	1920	1922	rBV	360	202	0.01%	0.001%
48	7.262	1930	1935	1940	rBV2	355	301	0.02%	0.002%
49	7.320	1940	1953	1976	rBV	956018	1639539	85.77%	11.120%
50	7.625	2038	2048	2072	rBV	150518	261092	13.66%	1.771%
51	7.924	2137	2141	2144	rBV2	466	432	0.02%	0.003%
52	7.986	2157	2160	2167	rBV4	413	429	0.02%	0.003%
53	8.095	2183	2194	2237	rBV2	376558	781658	40.89%	5.302%
54	8.323	2264	2265	2270	rVB4	506	325	0.02%	0.002%
55	8.349	2270	2273	2277	rBV3	582	391	0.02%	0.003%
56	8.529	2323	2329	2334	rVB2	412	464	0.02%	0.003%
57	8.558	2334	2338	2341	rBV2	250	184	0.01%	0.001%
58	8.857	2418	2431	2467	rBV	878854	1414040	73.97%	9.591%
59	9.027	2482	2484	2488	rVB2	624	339	0.02%	0.002%
60	9.075	2497	2499	2504	rBV2	217	201	0.01%	0.001%
61	9.124	2510	2514	2518	rBV2	406	273	0.01%	0.002%
62	9.156	2522	2524	2527	rBV	293	176	0.01%	0.001%
63	9.198	2534	2537	2540	rBV	330	223	0.01%	0.002%
64	9.272	2557	2560	2563	rBV2	347	230	0.01%	0.002%
65	9.407	2598	2602	2608	rBV2	414	365	0.02%	0.002%
66	9.535	2638	2642	2645	rBV	224	178	0.01%	0.001%
67	9.841	2733	2737	2740	rBV2	276	251	0.01%	0.002%
68	9.892	2750	2753	2756	rBV2	242	159	0.01%	0.001%
69	10.053	2799	2803	2806	rBV	193	168	0.01%	0.001%
70	10.220	2839	2855	2872	rBV	529187	822908	43.05%	5.581%
71	10.339	2888	2892	2894	rBV3	241	194	0.01%	0.001%
72	10.391	2901	2908	2912	rBV3	897	1112	0.06%	0.008%
73	10.436	2919	2922	2925	rVB	284	178	0.01%	0.001%
74	10.603	2970	2974	2976	rBV	297	255	0.01%	0.002%
75	10.796	3029	3034	3038	rVB2	298	358	0.02%	0.002%
76	10.825	3038	3043	3047	rBV2	229	297	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
 Data File : VV020520.D
 Acq On : 11 Mar 2021 00:58
 Operator : SY/MD
 Sample : M1632-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B64

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M

Title : VOC Analysis

77	10.847	3047	3050	3055	rVV2	195	201	0.01%	0.001%
78	10.992	3089	3095	3098	rBV	235	189	0.01%	0.001%
79	11.079	3118	3122	3126	rBV2	214	190	0.01%	0.001%
80	11.127	3133	3137	3139	rBV	258	222	0.01%	0.002%
81	11.146	3140	3143	3146	rVV2	185	162	0.01%	0.001%
82	11.207	3160	3162	3165	rVB	304	164	0.01%	0.001%
83	11.255	3165	3177	3208	rBV	899784	1396535	73.06%	9.472%
84	11.362	3208	3210	3213	rBV3	637	406	0.02%	0.003%
85	11.448	3234	3237	3239	rBV2	397	321	0.02%	0.002%
86	11.526	3259	3261	3265	rVB2	427	227	0.01%	0.002%
87	11.555	3265	3270	3273	rBV4	311	324	0.02%	0.002%
88	11.632	3280	3294	3318	rBV	1018388	1594552	83.41%	10.815%
89	11.802	3345	3347	3350	rVB3	357	167	0.01%	0.001%
90	11.915	3379	3382	3385	rVB3	377	234	0.01%	0.002%
91	12.535	3572	3575	3579	rVB	229	161	0.01%	0.001%
92	12.616	3597	3600	3605	rBV3	273	281	0.01%	0.002%
93	12.664	3610	3615	3618	rBV2	264	228	0.01%	0.002%
94	12.937	3697	3700	3705	rBV2	255	176	0.01%	0.001%
95	13.008	3720	3722	3727	rVB2	353	245	0.01%	0.002%
96	13.037	3727	3731	3732	rBV2	337	221	0.01%	0.001%
97	13.220	3785	3788	3791	rBV3	305	278	0.01%	0.002%
98	13.632	3912	3916	3917	rBV	325	225	0.01%	0.002%
99	13.828	3974	3977	3980	rBV2	368	198	0.01%	0.001%
100	14.371	4143	4146	4153	rVB2	489	242	0.01%	0.002%


Sum of corrected areas: 14743513

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
Data File : VV020520.D
Acq On : 11 Mar 2021 00:58
Operator : SY/MD
Sample : M1632-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B64

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

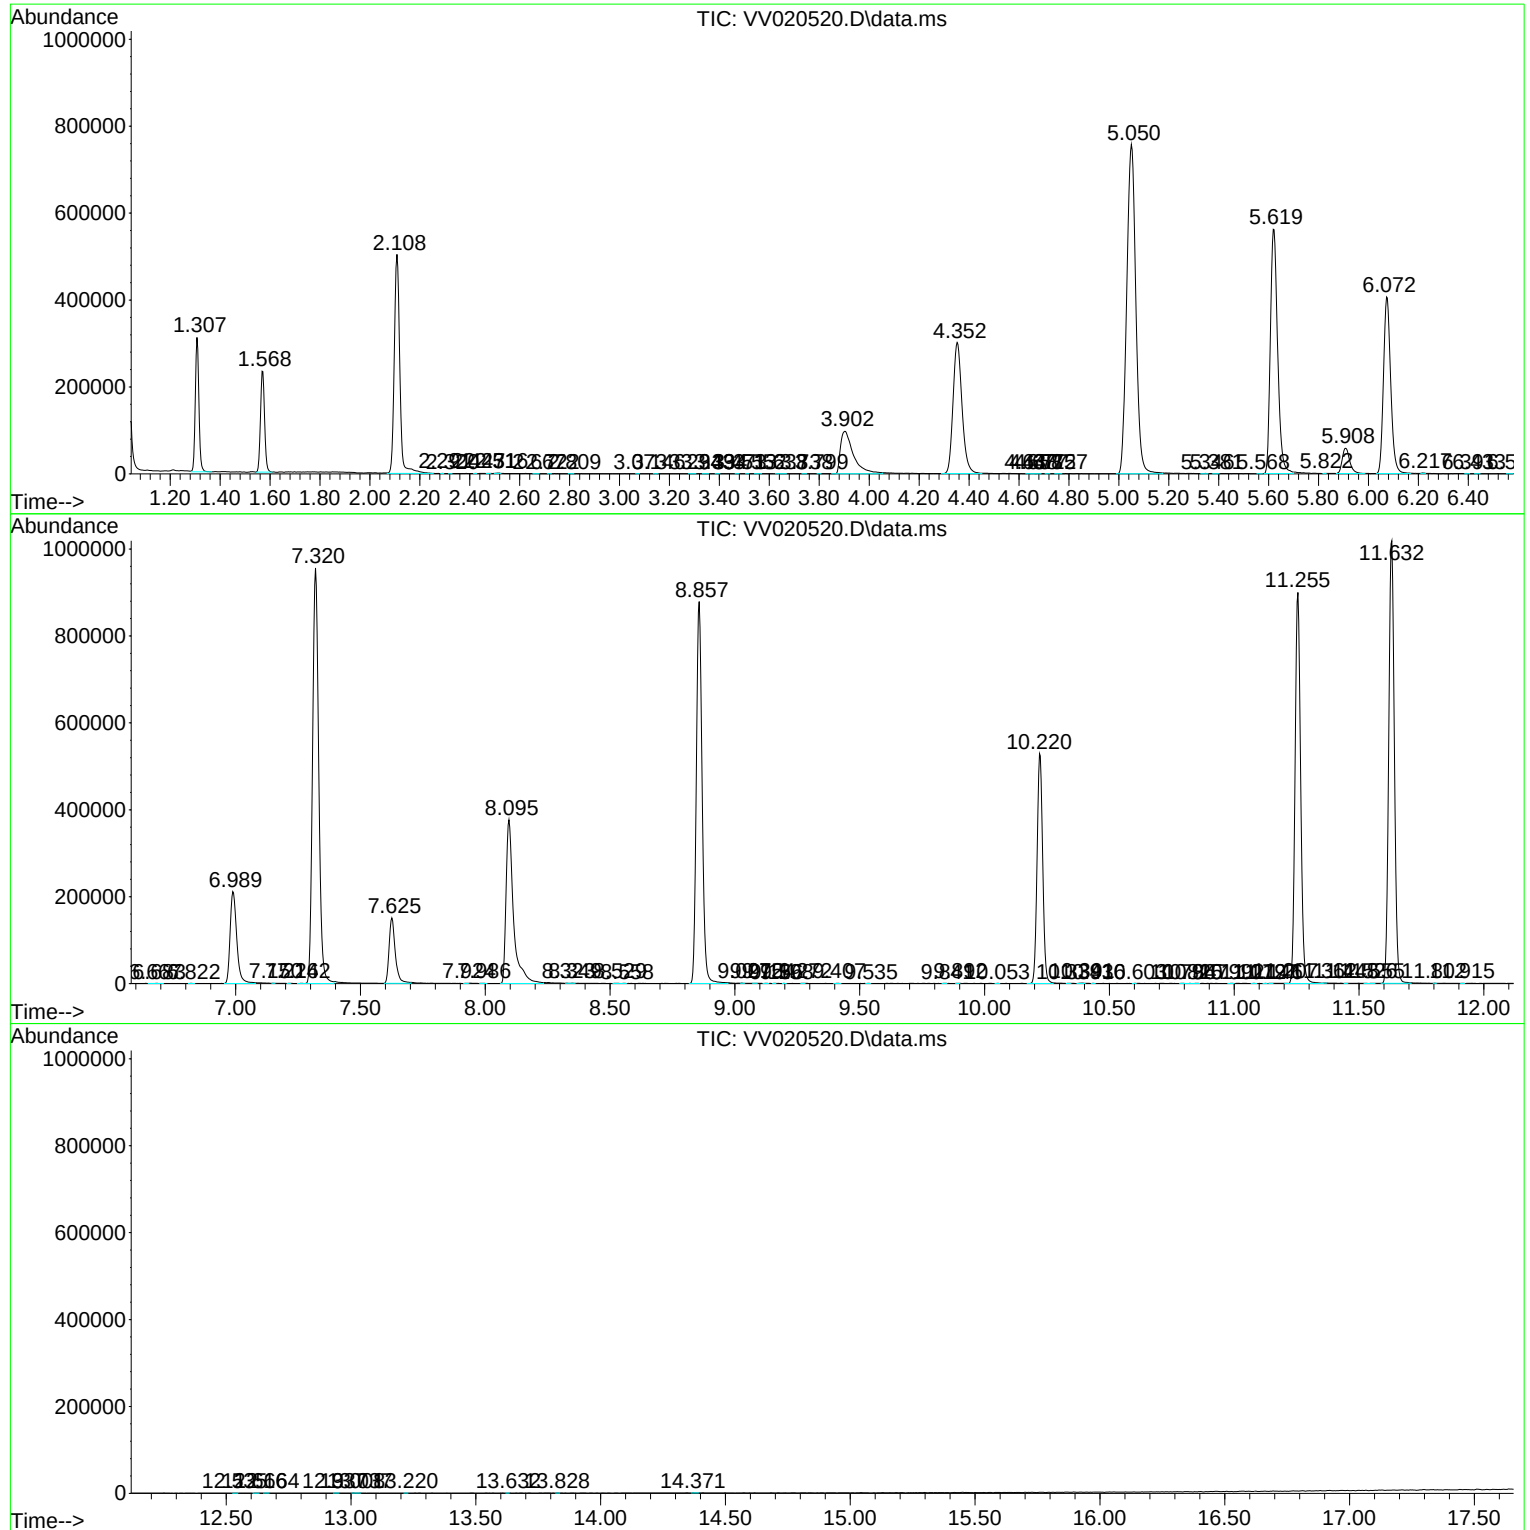

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
Data File : VV020520.D
Acq On : 11 Mar 2021 00:58
Operator : SY/MD
Sample : M1632-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B64

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
Data File : VV020520.D
Acq On : 11 Mar 2021 00:58
Operator : SY/MD
Sample : M1632-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B64

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc