

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
 Data File : VV020521.D
 Acq On : 11 Mar 2021 01:22
 Operator : SY/MD
 Sample : M1632-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B65

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
 Title : VOC Analysis

Signal : TIC: VV020521.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	103	rVB	312521	315010	16.28%	2.102%
2	1.571	157	165	179	rBV	233758	267122	13.81%	1.782%
3	2.108	320	332	347	rBV	503265	734636	37.97%	4.902%
4	2.394	418	421	423	rBV	276	165	0.01%	0.001%
5	2.413	425	427	430	rVB2	300	171	0.01%	0.001%
6	2.510	452	457	461	rVV5	1149	1260	0.07%	0.008%
7	2.542	464	467	469	rBV2	382	184	0.01%	0.001%
8	2.558	470	472	477	rVB3	385	299	0.02%	0.002%
9	2.584	477	480	481	rBV2	270	166	0.01%	0.001%
10	2.658	500	503	509	rVB2	225	198	0.01%	0.001%
11	2.838	554	559	562	rBV2	235	261	0.01%	0.002%
12	2.950	590	594	597	rVB	290	206	0.01%	0.001%
13	3.060	624	628	630	rBV	212	170	0.01%	0.001%
14	3.127	645	649	654	rVV2	163	171	0.01%	0.001%
15	3.253	686	688	691	rBV	231	186	0.01%	0.001%
16	3.307	702	705	708	rBV2	228	175	0.01%	0.001%
17	3.426	736	742	746	rBV2	213	321	0.02%	0.002%
18	3.494	756	763	765	rBV	328	392	0.02%	0.003%
19	3.548	775	780	783	rBV2	216	255	0.01%	0.002%
20	3.597	791	795	799	rBV	230	187	0.01%	0.001%
21	3.677	817	820	823	rBV2	249	207	0.01%	0.001%
22	3.786	850	854	858	rBV	247	219	0.01%	0.001%
23	3.902	876	890	938	rBV	99241	354861	18.34%	2.368%
24	4.227	989	991	997	rBV2	338	268	0.01%	0.002%
25	4.352	1009	1030	1069	rBV	305357	770430	39.82%	5.141%
26	4.580	1098	1101	1107	rBV3	341	287	0.01%	0.002%
27	4.606	1107	1109	1111	rVV	297	196	0.01%	0.001%
28	4.622	1111	1114	1120	rVV4	639	550	0.03%	0.004%
29	4.671	1123	1129	1136	rBV2	426	671	0.03%	0.004%
30	4.728	1142	1147	1150	rBV2	292	254	0.01%	0.002%
31	5.050	1229	1247	1275	rBV2	768916	1934660	100.00%	12.909%
32	5.326	1330	1333	1336	rBV	330	229	0.01%	0.002%
33	5.474	1377	1379	1383	rBV	297	210	0.01%	0.001%
34	5.542	1397	1400	1404	rBV2	232	245	0.01%	0.002%
35	5.564	1405	1407	1412	rVB2	294	229	0.01%	0.002%
36	5.622	1412	1425	1451	rBV	565809	1135211	58.68%	7.575%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
 Data File : VV020521.D
 Acq On : 11 Mar 2021 01:22
 Operator : SY/MD
 Sample : M1632-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B65

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
 Title : VOC Analysis

37	5.912	1502	1515	1538	rBV3	89877	213631	11.04%	1.425%
38	6.072	1551	1565	1589	rBV	411316	831512	42.98%	5.548%
39	6.214	1606	1609	1612	rBV4	701	534	0.03%	0.004%
40	6.246	1617	1619	1622	rVB2	382	150	0.01%	0.001%
41	6.275	1627	1628	1632	rBV	239	164	0.01%	0.001%
42	6.336	1644	1647	1652	rVB3	429	349	0.02%	0.002%
43	6.397	1662	1666	1668	rBV	248	159	0.01%	0.001%
44	6.494	1691	1696	1700	rBV2	209	238	0.01%	0.002%
45	6.622	1731	1736	1739	rBV2	251	215	0.01%	0.001%
46	6.741	1768	1773	1779	rVB2	179	201	0.01%	0.001%
47	6.818	1791	1797	1802	rVV2	281	324	0.02%	0.002%
48	6.892	1817	1820	1825	rVB2	159	149	0.01%	0.001%
49	6.928	1827	1831	1835	rBV2	147	165	0.01%	0.001%
50	6.989	1839	1850	1878	rBV	212587	394269	20.38%	2.631%
51	7.236	1925	1927	1931	rVB	373	208	0.01%	0.001%
52	7.259	1931	1934	1941	rBV2	204	229	0.01%	0.002%
53	7.320	1941	1953	1982	rBV	968625	1664273	86.02%	11.105%
54	7.625	2037	2048	2072	rBV	151922	264954	13.70%	1.768%
55	7.783	2093	2097	2098	rBV2	301	209	0.01%	0.001%
56	7.809	2102	2105	2106	rBV2	418	178	0.01%	0.001%
57	7.831	2110	2112	2116	rVB2	393	328	0.02%	0.002%
58	7.928	2138	2142	2145	rBV	360	329	0.02%	0.002%
59	7.986	2156	2160	2164	rVB5	665	642	0.03%	0.004%
60	8.027	2170	2173	2176	rBV	459	270	0.01%	0.002%
61	8.095	2183	2194	2242	rBV2	388723	801084	41.41%	5.345%
62	8.407	2289	2291	2294	rVB2	372	151	0.01%	0.001%
63	8.477	2309	2313	2316	rVB2	307	218	0.01%	0.001%
64	8.584	2343	2346	2349	rBV	223	164	0.01%	0.001%
65	8.654	2364	2368	2370	rBV2	189	169	0.01%	0.001%
66	8.857	2419	2431	2463	rBV	874270	1421058	73.45%	9.482%
67	9.085	2499	2502	2507	rVB	316	186	0.01%	0.001%
68	9.153	2520	2523	2527	rBV2	266	249	0.01%	0.002%
69	9.268	2552	2559	2561	rBV	400	376	0.02%	0.003%
70	9.349	2582	2584	2589	rVV	235	198	0.01%	0.001%
71	9.458	2615	2618	2622	rVB2	224	188	0.01%	0.001%
72	9.551	2643	2647	2650	rBV	176	161	0.01%	0.001%
73	9.995	2781	2785	2790	rBV2	256	357	0.02%	0.002%
74	10.220	2843	2855	2880	rBV	537999	839143	43.37%	5.599%
75	10.307	2880	2882	2886	rVB2	344	186	0.01%	0.001%
76	10.355	2895	2897	2900	rVB	479	213	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
 Data File : VV020521.D
 Acq On : 11 Mar 2021 01:22
 Operator : SY/MD
 Sample : M1632-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B65

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M

Title : VOC Analysis

77	10.391	2900	2908	2911	rBV3	769	958	0.05%	0.006%
78	10.455	2925	2928	2933	rVB2	262	194	0.01%	0.001%
79	11.165	3146	3149	3152	rBV	407	313	0.02%	0.002%
80	11.201	3157	3160	3162	rBV2	260	201	0.01%	0.001%
81	11.255	3165	3177	3200	rBV	903307	1403057	72.52%	9.362%
82	11.336	3200	3202	3206	rVB2	678	434	0.02%	0.003%
83	11.455	3235	3239	3241	rBV2	410	385	0.02%	0.003%
84	11.632	3281	3294	3316	rBV	1041030	1618528	83.66%	10.799%
85	11.767	3333	3336	3338	rVB2	557	315	0.02%	0.002%
86	11.789	3338	3343	3348	rVB2	635	654	0.03%	0.004%
87	12.001	3406	3409	3415	rBV2	179	207	0.01%	0.001%
88	12.239	3478	3483	3486	rBV2	380	382	0.02%	0.003%
89	12.664	3611	3615	3616	rBV	369	220	0.01%	0.001%
90	12.690	3621	3623	3626	rBV	289	175	0.01%	0.001%
91	12.895	3682	3687	3690	rBV3	306	317	0.02%	0.002%
92	13.040	3728	3732	3736	rVB3	349	257	0.01%	0.002%
93	13.079	3742	3744	3746	rBV2	307	161	0.01%	0.001%
94	13.146	3762	3765	3768	rBV2	366	284	0.01%	0.002%
95	13.410	3842	3847	3849	rBV	313	300	0.02%	0.002%
96	13.493	3871	3873	3877	rVB2	374	273	0.01%	0.002%
97	13.538	3885	3887	3895	rVB3	397	427	0.02%	0.003%
98	14.091	4056	4059	4063	rBV2	452	282	0.01%	0.002%
99	14.860	4296	4298	4304	rBV2	358	307	0.02%	0.002%
100	15.693	4554	4557	4558	rBV3	1177	555	0.03%	0.004%




Sum of corrected areas: 14987229

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
Data File : VV020521.D
Acq On : 11 Mar 2021 01:22
Operator : SY/MD
Sample : M1632-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B65

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

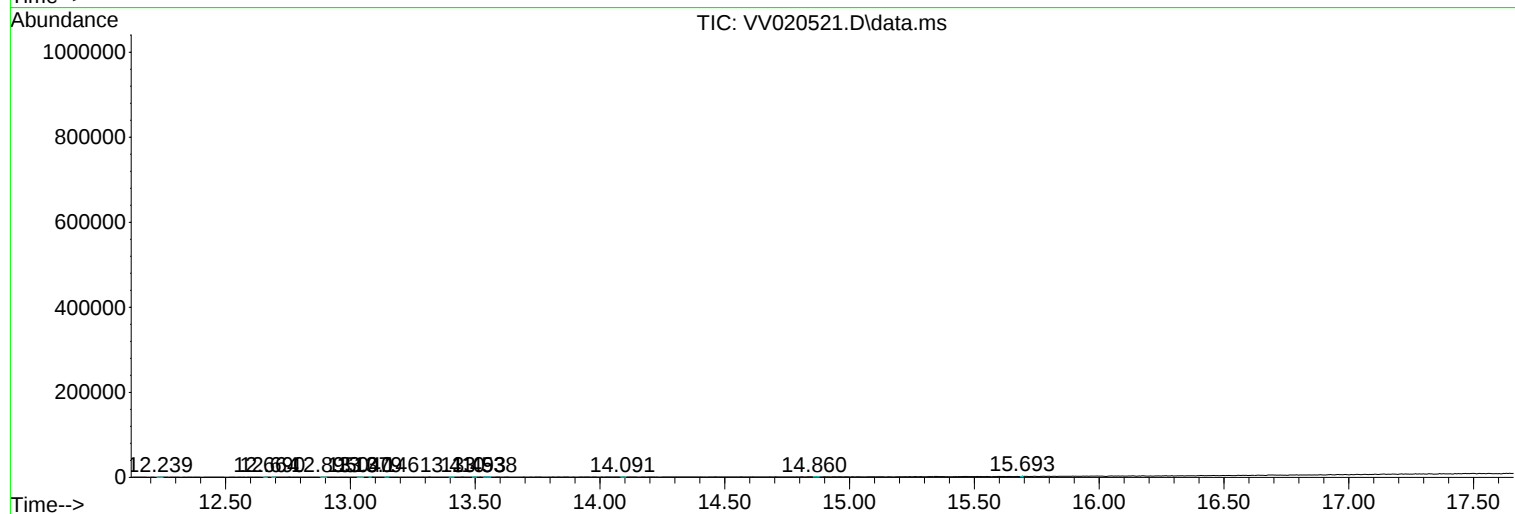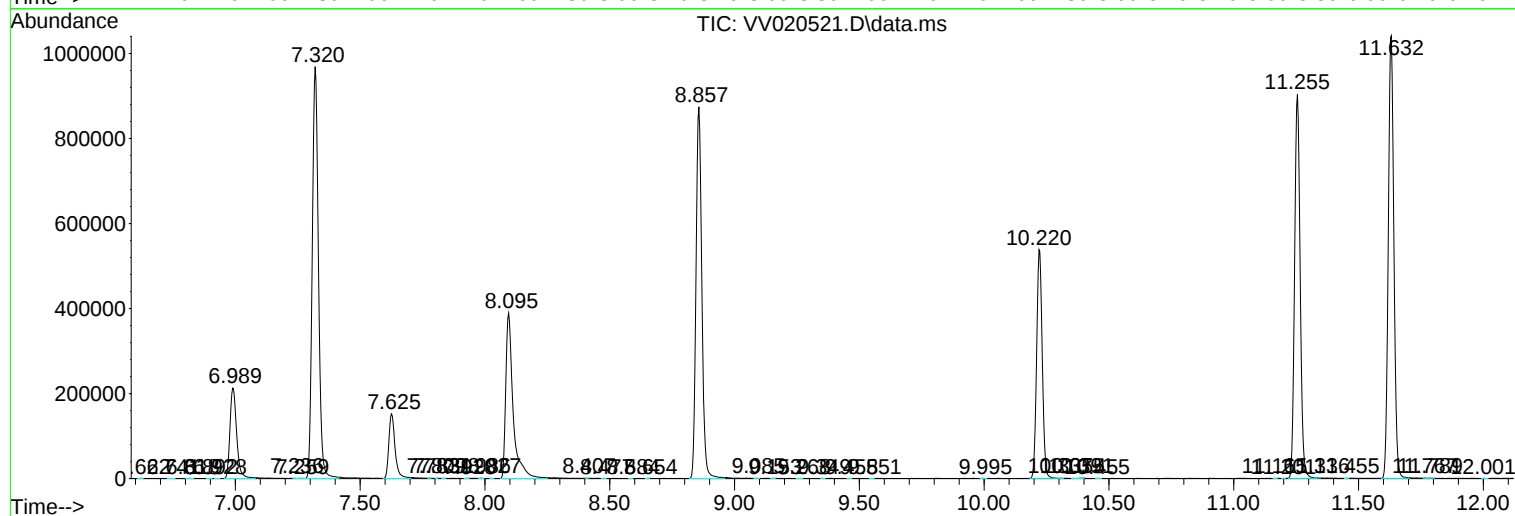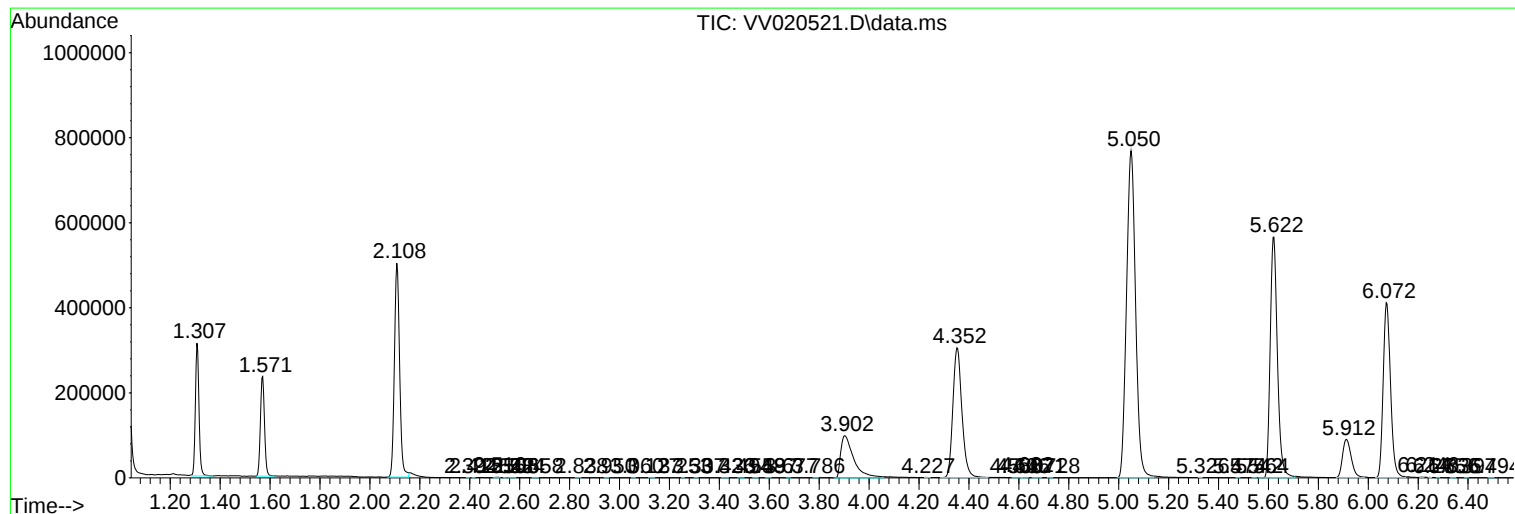

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
Data File : VV020521.D
Acq On : 11 Mar 2021 01:22
Operator : SY/MD
Sample : M1632-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B65

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
Data File : VV020521.D
Acq On : 11 Mar 2021 01:22
Operator : SY/MD
Sample : M1632-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B65

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
