
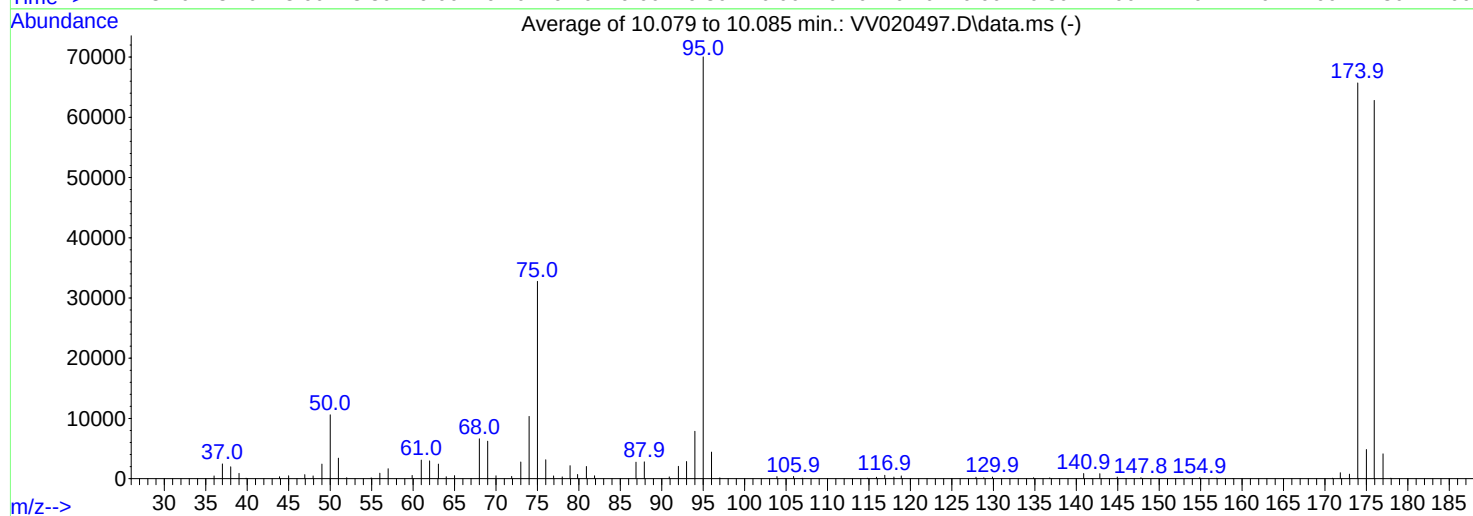


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031121\
 Data File : VV020497.D
 Acq On : 10 Mar 2021 15:07
 Operator : SY/MD
 Sample : BFB97
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB97

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
 Title : VOC Analysis
 Last Update : Thu Mar 11 03:02:24 2021

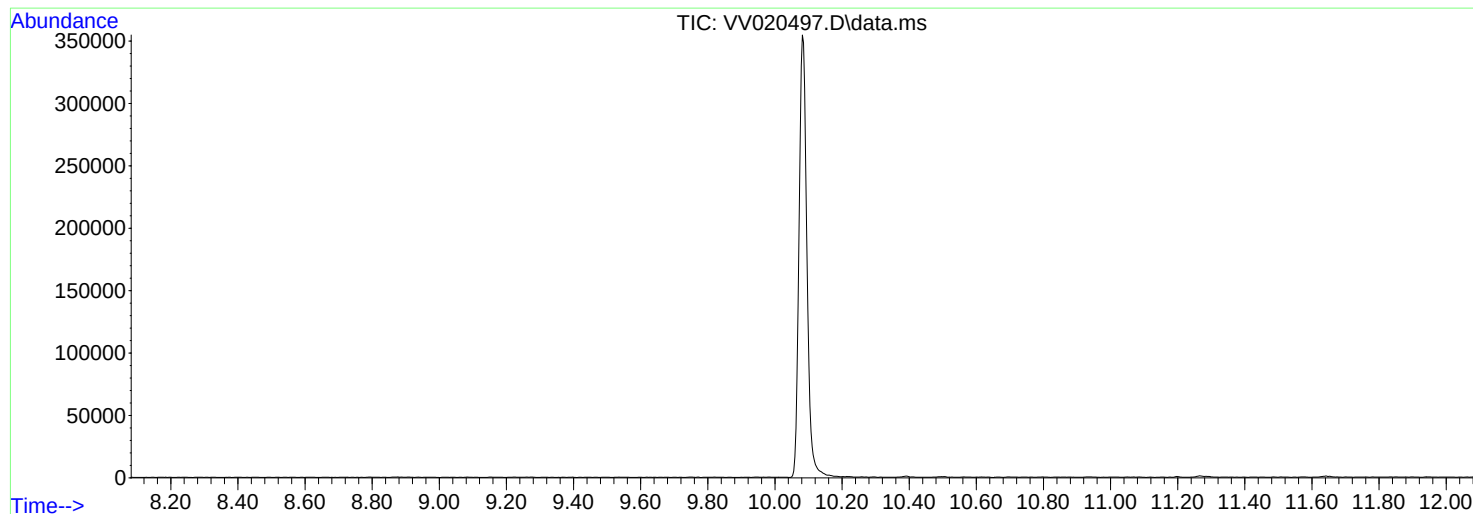

AutoFind: Scans 2811, 2812, 2813; Background Corrected with Scan 2800

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.1	10594	PASS
75	95	30	80	46.8	32752	PASS
95	95	100	100	100.0	70043	PASS
96	95	5	9	6.3	4416	PASS
173	174	0.00	2	1.1	752	PASS
174	95	50	120	93.8	65696	PASS
175	174	5	9	7.4	4829	PASS
176	174	95	101	95.6	62800	PASS
177	176	5	9	6.6	4118	PASS

m/z	Abundance
36.00	410.0
37.00	2421.0
38.00	1898.0
39.00	855.0
39.90	187.0
44.00	644.0
45.00	539.0
46.90	691.0
47.90	471.0
49.00	2202.0
50.00	10286.0
51.00	3316.0
52.00	191.0
54.90	148.0
56.00	865.0
57.00	1545.0
59.90	527.0
61.00	3004.0
62.00	2916.0
63.00	2175.0
64.00	307.0
65.00	480.0
67.00	110.0
68.00	6452.0
69.00	6115.0
70.00	522.0
71.90	373.0
73.00	2729.0
74.00	10345.0
75.00	31912.0
76.00	2947.0
76.90	477.0
78.00	232.0
78.90	2139.0
79.80	644.0
80.90	1989.0
81.90	483.0
86.90	2475.0
87.90	2628.0
90.90	298.0
92.00	2139.0
93.00	2609.0
94.00	7817.0
95.00	67544.0
96.00	4257.0
97.00	112.0
103.90	339.0
104.90	108.0
105.90	374.0
107.00	127.0
115.90	277.0
116.90	490.0
118.10	242.0
118.90	447.0
127.90	228.0
128.90	141.0
129.80	268.0
134.80	163.0
136.80	136.0
140.90	798.0
141.80	114.0
142.80	748.0
145.00	284.0
147.80	172.0
154.90	141.0
156.90	117.0
171.80	877.0
173.00	612.0
173.90	61424.0
175.00	4534.0
175.90	59568.0
177.00	3916.0

Instrument :
MSVOA_V
ClientSampleId :
BFB97

m/z	Abundance
36.00	463.0
37.00	2538.0
38.00	2058.0
39.00	907.0
39.90	208.0
44.00	620.0
45.00	503.0
46.90	667.0
47.90	461.0
49.00	2493.0
50.00	10830.0
51.00	3580.0
52.00	153.0
54.90	144.0
56.00	978.0
57.00	1700.0
59.90	571.0
61.00	3175.0
62.00	3046.0
63.00	2492.0
64.00	322.0
65.00	540.0
68.00	6889.0
69.00	6418.0
70.00	473.0
71.90	367.0
73.00	2820.0
74.00	10562.0
75.00	33680.0
76.00	3269.0
77.00	480.0
78.00	240.0
79.00	2179.0
79.80	702.0
80.90	2110.0
81.90	515.0
86.90	2831.0
87.90	2896.0
90.90	288.0
92.00	2087.0
93.00	2908.0
94.00	8062.0
95.00	72208.0
96.00	4525.0
97.00	154.0
103.90	364.0
105.90	379.0
106.90	105.0
114.80	112.0
115.90	246.0
116.90	575.0
118.00	268.0
118.90	461.0
127.90	244.0
128.90	154.0
129.90	266.0
134.90	160.0
136.80	138.0
140.90	862.0
142.90	856.0
145.00	269.0
147.80	180.0
154.90	204.0
157.20	130.0
171.00	120.0
171.90	1018.0
173.00	792.0
174.00	67864.0
175.00	5018.0
175.90	64568.0
177.00	4251.0
177.90	128.0

Instrument :
MSVOA_V
ClientSampleId :
BFB97

m/z	Abundance
36.00	492.0
37.00	2392.0
38.00	1930.0
39.00	863.0
39.80	197.0
43.90	587.0
45.00	396.0
47.00	649.0
48.00	405.0
49.00	2573.0
50.00	10665.0
51.00	3315.0
52.00	116.0
55.00	127.0
56.00	877.0
57.00	1711.0
59.90	524.0
61.00	3078.0
62.00	2874.0
63.10	2558.0
64.00	294.0
65.00	531.0
68.00	6478.0
69.00	6144.0
70.00	447.0
71.90	370.0
73.00	2735.0
74.00	10144.0
75.00	32664.0
76.00	3224.0
77.00	393.0
77.80	209.0
78.10	213.0
79.00	2132.0
79.90	693.0
80.90	1983.0
81.90	488.0
86.90	2940.0
87.90	2867.0
90.90	283.0
92.00	1947.0
93.00	3032.0
94.00	7703.0
95.00	70376.0
96.00	4465.0
97.00	165.0
103.90	345.0
105.90	340.0
114.80	151.0
115.90	213.0
116.90	592.0
117.90	258.0
118.90	475.0
127.90	258.0
128.80	157.0
130.00	255.0
134.90	130.0
136.80	126.0
140.90	874.0
142.90	867.0
144.90	231.0
146.00	106.0
147.80	154.0
154.90	247.0
157.00	158.0
158.90	102.0
170.80	120.0
171.90	1084.0
172.90	853.0
174.00	67800.0
175.00	4934.0
176.00	64264.0
177.00	4187.0
178.00	102.0

Instrument :
MSVOA_V
ClientSampleId :
BFB97

m/z	Abundance
39.90	102.0
43.90	300.0

Instrument :
MSVOA_V
ClientSampleId :
BFB97