

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031124\
 Data File : VV034535.D
 Acq On : 11 Mar 2024 11:55
 Operator : SY/MD
 Sample : P1637-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Mar 12 01:31:04 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Mar 12 01:30:00 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	320770	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	300369	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	142466	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	97716	35.140	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	70.280%		
7) Chloroethane-d5	1.529	69	88343	40.779	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	81.560%		
11) 1,1-Dichloroethene-d2	2.056	65	46312	36.826	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	73.660%		
21) 2-Butanone-d5	3.777	46	183142	98.485	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	98.490%		
24) Chloroform-d	4.246	84	214175	43.561	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	87.120%		
26) 1,2-Dichloroethane-d4	4.937	65	149196	46.436	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.880%		
32) Benzene-d6	4.957	84	395103	43.585	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	87.160%		
36) 1,2-Dichloropropane-d6	5.985	67	128352	46.395	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	92.780%		
41) Toluene-d8	7.239	98	335436	40.889	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	81.780%		
43) trans-1,3-Dichloroprop...	7.551	79	57893	41.672	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	83.340%		
47) 2-Hexanone-d5	8.021	63	133131	96.368	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	96.370%		
56) 1,1,2,2-Tetrachloroeth...	10.149	84	177439	48.737	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	97.480%		
66) 1,2-Dichlorobenzene-d4	11.558	152	134090	46.047	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	92.100%		
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	6.915	75	4004	1.012	ug/L	# 74


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031124\
Data File : VV034535.D
Acq On : 11 Mar 2024 11:55
Operator : SY/MD
Sample : P1637-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Mar 12 01:31:04 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Mar 12 01:30:00 2024
Response via : Initial Calibration

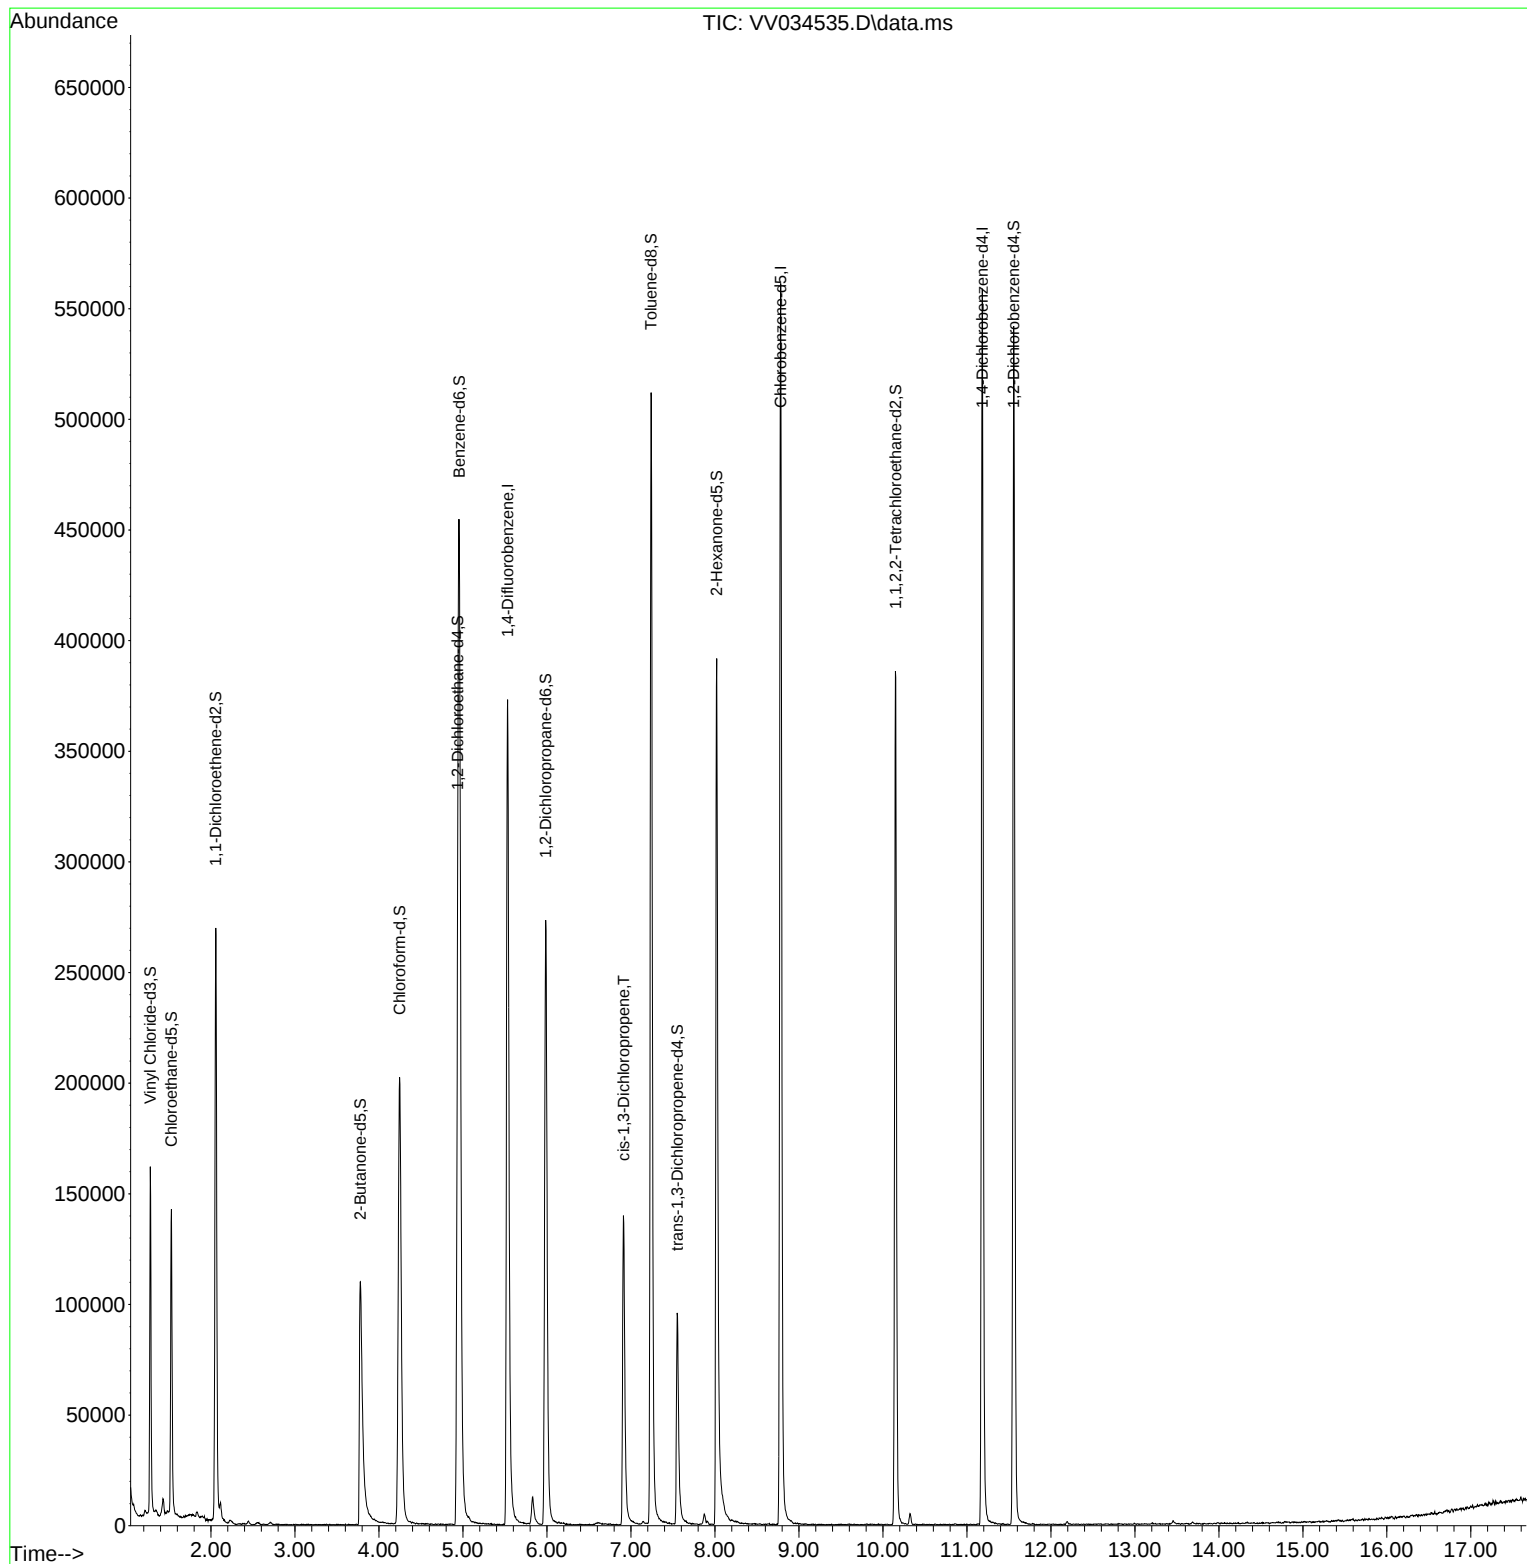

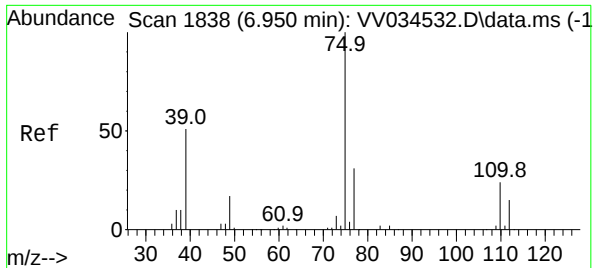

#39
 cis-1,3-Dichloropropene
 Concen: 1.012 ug/L
 RT: 6.915 min Scan# 11
 Delta R.T. -0.035 min
 Lab File: VV034535.D
 Acq: 11 Mar 2024 11:55

Instrument :
 MSVOA_V
 ClientSampleId :

Tgt Ion: 75 Resp: 4004
 Ion Ratio Lower Upper
 75 100
 77 44.0 20.9 38.9#

