

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031124\
 Data File : VV034533.D
 Acq On : 11 Mar 2024 10:56
 Operator : SY/MD
 Sample : VV0311WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK239

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M

Title : VOC Analysis

Signal : TIC: VV034533.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	94	rVB	157599	172845	13.72%	1.771%
2	1.529	145	152	177	rVB	146090	178726	14.18%	1.831%
3	2.060	306	317	342	rBV	278689	410591	32.59%	4.207%
4	2.201	360	361	363	rBV2	491	150	0.01%	0.002%
5	2.365	410	412	414	rBV	244	108	0.01%	0.001%
6	2.449	431	438	448	rVB6	2276	3763	0.30%	0.039%
7	2.519	458	460	462	rBV	203	87	0.01%	0.001%
8	2.548	467	469	471	rBV	245	110	0.01%	0.001%
9	2.703	512	517	523	rVB4	496	543	0.04%	0.006%
10	2.757	531	534	537	rBV2	221	155	0.01%	0.002%
11	2.818	548	553	556	rBV	430	336	0.03%	0.003%
12	2.863	566	567	570	rVB2	280	89	0.01%	0.001%
13	2.937	587	590	593	rBV	203	149	0.01%	0.002%
14	2.970	597	600	601	rBV	218	148	0.01%	0.002%
15	3.053	624	626	628	rBV2	227	124	0.01%	0.001%
16	3.159	657	659	663	rBV	231	162	0.01%	0.002%
17	3.397	729	733	735	rBV	175	128	0.01%	0.001%
18	3.535	773	776	778	rBV2	115	83	0.01%	0.001%
19	3.696	825	826	827	rVB	183	35	0.00%	0.000%
20	3.715	827	832	841	rBV2	259	268	0.02%	0.003%
21	3.780	843	852	891	rBV	121695	325621	25.84%	3.336%
22	4.246	981	997	1025	rBV2	203041	524764	41.65%	5.377%
23	4.670	1126	1129	1130	rBV	214	99	0.01%	0.001%
24	4.748	1150	1153	1157	rBV	267	209	0.02%	0.002%
25	4.789	1163	1166	1167	rBV2	277	160	0.01%	0.002%
26	4.899	1198	1200	1201	rBV	200	104	0.01%	0.001%
27	4.953	1201	1217	1253	rVV2	472034	1259990	100.00%	12.910%
28	5.278	1316	1318	1320	rBV2	381	189	0.02%	0.002%
29	5.336	1333	1336	1342	rBV2	574	618	0.05%	0.006%
30	5.449	1369	1371	1376	rBV2	281	180	0.01%	0.002%
31	5.468	1376	1377	1381	rVB2	216	133	0.01%	0.001%
32	5.532	1386	1397	1428	rBV	371954	774513	61.47%	7.935%
33	5.828	1479	1489	1511	rBV2	17510	39882	3.17%	0.409%
34	5.985	1525	1538	1567	rBV	283786	585459	46.47%	5.998%
35	6.243	1617	1618	1619	rBV	219	76	0.01%	0.001%
36	6.262	1622	1624	1628	rVB3	430	236	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031124\
 Data File : VV034533.D
 Acq On : 11 Mar 2024 10:56
 Operator : SY/MD
 Sample : VV0311WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK239

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	6.484	1689	1693	1698	rBV2	268	285	0.02%	0.003%
38	6.574	1716	1721	1723	rBV2	569	459	0.04%	0.005%
39	6.844	1802	1805	1808	rVB2	249	154	0.01%	0.002%
40	6.866	1810	1812	1814	rBV2	215	138	0.01%	0.001%
41	6.911	1816	1826	1858	rBV	146256	278225	22.08%	2.851%
42	7.239	1918	1928	1968	rBV	515281	924310	73.36%	9.470%
43	7.551	2016	2025	2049	rBV	97402	181685	14.42%	1.861%
44	7.760	2088	2090	2092	rBV	296	123	0.01%	0.001%
45	7.815	2104	2107	2111	rBV2	228	154	0.01%	0.002%
46	7.860	2118	2121	2122	rBV	384	225	0.02%	0.002%
47	7.956	2145	2151	2152	rBV2	363	277	0.02%	0.003%
48	8.021	2162	2171	2206	rBV	424080	765660	60.77%	7.845%
49	8.384	2281	2284	2287	rBV3	519	337	0.03%	0.003%
50	8.600	2349	2351	2353	rBV	290	162	0.01%	0.002%
51	8.783	2397	2408	2439	rBV	558605	923518	73.30%	9.462%
52	9.059	2493	2494	2495	rVB	272	52	0.00%	0.001%
53	9.069	2495	2497	2500	rBV	300	173	0.01%	0.002%
54	9.095	2501	2505	2507	rBV	331	257	0.02%	0.003%
55	9.201	2536	2538	2541	rVB3	331	198	0.02%	0.002%
56	9.220	2541	2544	2547	rBV2	186	141	0.01%	0.001%
57	9.381	2593	2594	2598	rBV2	227	108	0.01%	0.001%
58	9.468	2618	2621	2624	rBV2	204	156	0.01%	0.002%
59	9.487	2625	2627	2628	rBV2	209	68	0.01%	0.001%
60	9.542	2642	2644	2645	rBV	165	70	0.01%	0.001%
61	9.551	2645	2647	2651	rVB2	189	132	0.01%	0.001%
62	9.870	2742	2746	2747	rBV2	370	252	0.02%	0.003%
63	9.976	2776	2779	2782	rBV	307	171	0.01%	0.002%
64	10.149	2820	2833	2858	rBV	395827	623788	49.51%	6.391%
65	10.458	2926	2929	2931	rBV	224	140	0.01%	0.001%
66	10.702	2999	3005	3007	rBV2	267	291	0.02%	0.003%
67	10.828	3040	3044	3048	rBV2	305	377	0.03%	0.004%
68	10.886	3061	3062	3064	rVB	284	106	0.01%	0.001%
69	11.130	3132	3138	3144	rBV3	1068	1081	0.09%	0.011%
70	11.181	3144	3154	3178	rBV	551828	874271	69.39%	8.958%
71	11.361	3209	3210	3211	rBV	333	127	0.01%	0.001%
72	11.400	3219	3222	3225	rBV2	310	177	0.01%	0.002%
73	11.558	3258	3271	3298	rBV	552558	882735	70.06%	9.044%
74	12.053	3423	3425	3426	rBV	220	101	0.01%	0.001%
75	12.117	3444	3445	3446	rBV	138	42	0.00%	0.000%
76	12.590	3588	3592	3598	rBV2	693	721	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031124\
Data File : VV034533.D
Acq On : 11 Mar 2024 10:56
Operator : SY/MD
Sample : VV0311WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK239

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Title : VOC Analysis

77	12.898	3686	3688	3690	rBV	269	137	0.01%	0.001%
78	12.963	3706	3708	3713	rBV3	283	187	0.01%	0.002%
79	13.210	3778	3785	3796	rBV3	2300	2908	0.23%	0.030%
80	13.448	3852	3859	3868	rBV	7022	10756	0.85%	0.110%
81	13.686	3926	3933	3940	rBV4	2968	3874	0.31%	0.040%




Sum of corrected areas: 9760142

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031124\
Data File : VV034533.D
Acq On : 11 Mar 2024 10:56
Operator : SY/MD
Sample : VV0311WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK239

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

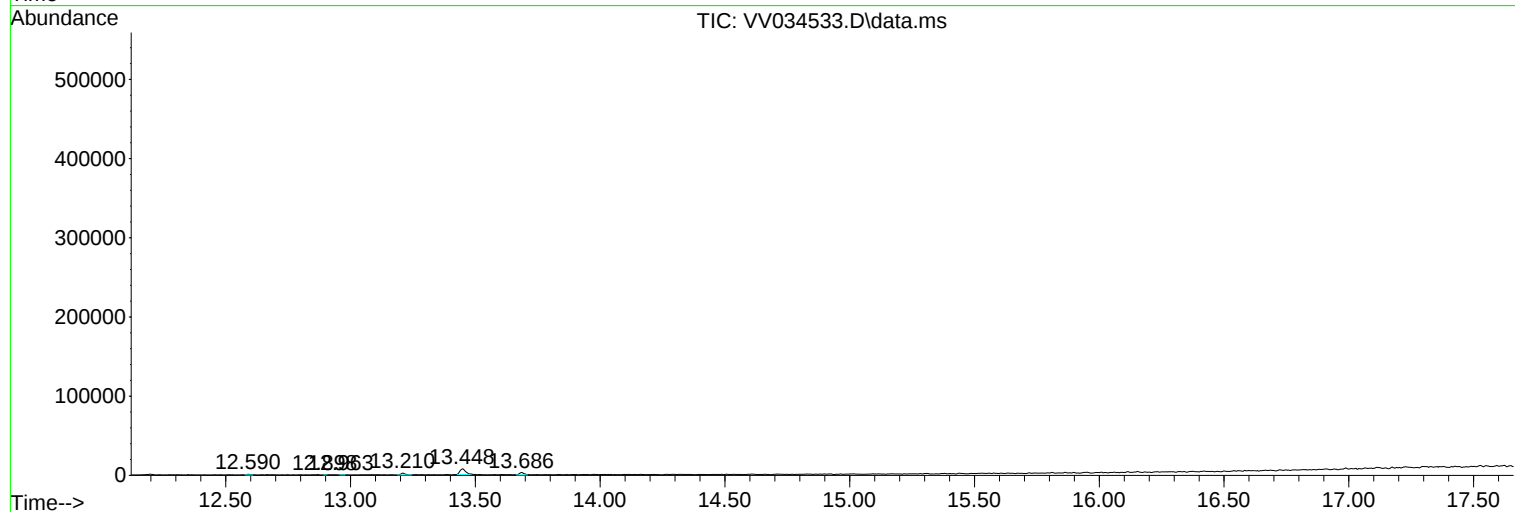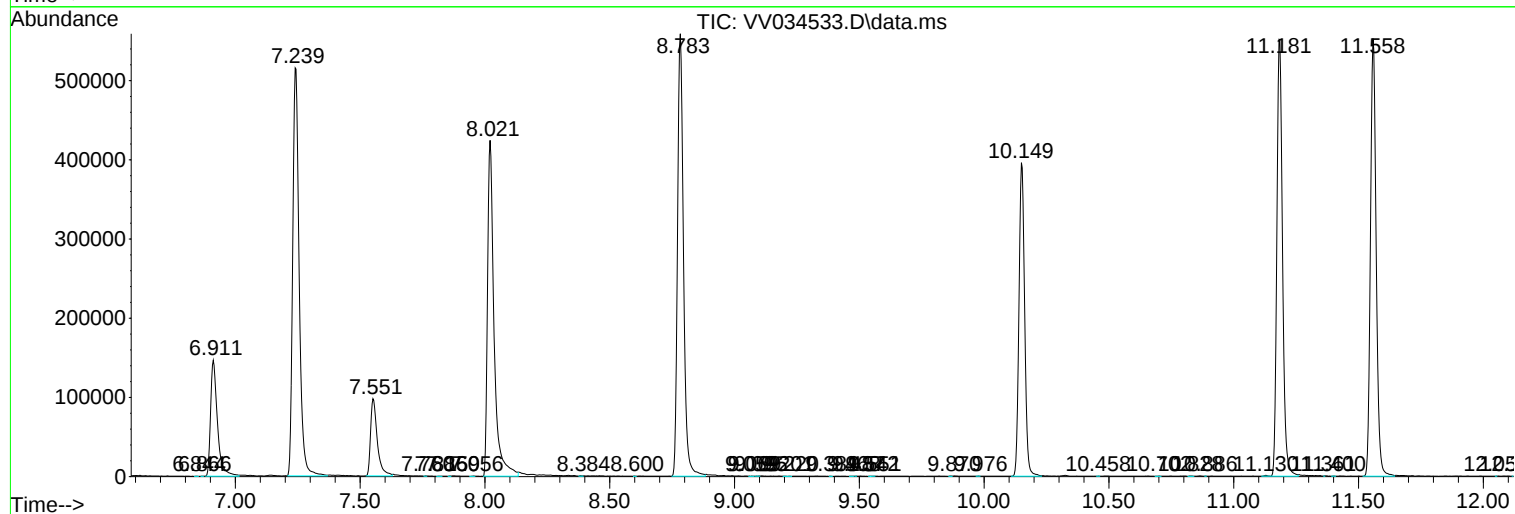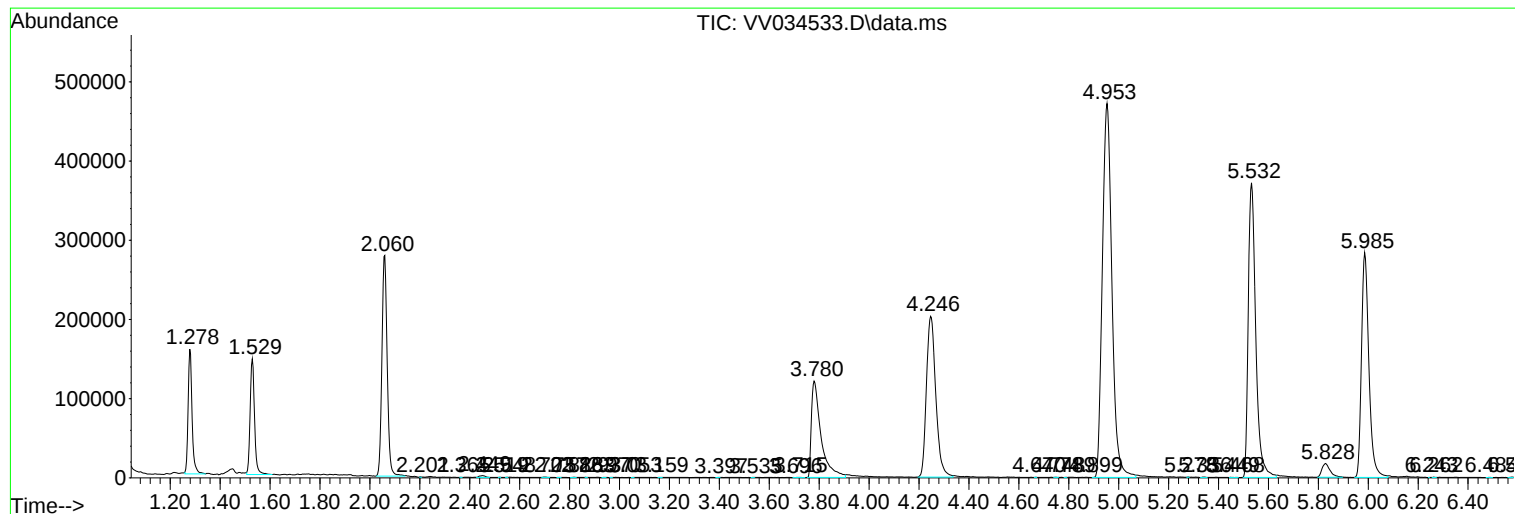

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031124\
Data File : VV034533.D
Acq On : 11 Mar 2024 10:56
Operator : SY/MD
Sample : VV0311WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK239

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031124\
Data File : VV034533.D
Acq On : 11 Mar 2024 10:56
Operator : SY/MD
Sample : VV0311WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK239

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc