

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031124\
 Data File : VV034536.D
 Acq On : 11 Mar 2024 12:19
 Operator : SY/MD
 Sample : P1637-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCNR3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034536.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	90	rVB	152908	154294	2.72%	1.037%
2	1.529	145	152	170	rVB	134995	166406	2.93%	1.119%
3	2.056	306	316	329	rBV	254456	371653	6.54%	2.499%
4	2.641	497	498	501	rBV	187	119	0.00%	0.001%
5	2.696	510	515	517	rBV4	976	895	0.02%	0.006%
6	3.053	624	626	630	rBV	182	104	0.00%	0.001%
7	3.175	660	664	666	rBV	115	99	0.00%	0.001%
8	3.223	676	679	680	rBV	150	85	0.00%	0.001%
9	3.497	759	764	767	rBV2	364	359	0.01%	0.002%
10	3.561	782	784	787	rVB2	138	67	0.00%	0.000%
11	3.587	787	792	796	rBV2	212	234	0.00%	0.002%
12	3.667	814	817	819	rBV	158	116	0.00%	0.001%
13	3.699	825	827	829	rBV	278	154	0.00%	0.001%
14	3.780	844	852	888	rBV	113768	313972	5.53%	2.111%
15	4.146	962	966	971	rBV4	563	634	0.01%	0.004%
16	4.246	980	997	1030	rBV	192513	494620	8.71%	3.325%
17	4.564	1094	1096	1101	rVB2	583	328	0.01%	0.002%
18	4.680	1128	1132	1134	rBV	304	243	0.00%	0.002%
19	4.738	1147	1150	1151	rBV	197	106	0.00%	0.001%
20	4.773	1159	1161	1163	rBV	266	130	0.00%	0.001%
21	4.953	1201	1217	1256	rBV2	434245	1161135	20.44%	7.807%
22	5.320	1329	1331	1335	rVB2	715	356	0.01%	0.002%
23	5.336	1335	1336	1337	rBV	342	100	0.00%	0.001%
24	5.407	1356	1358	1359	rBV	231	121	0.00%	0.001%
25	5.445	1368	1370	1374	rVB3	307	175	0.00%	0.001%
26	5.493	1384	1385	1386	rBV3	170	60	0.00%	0.000%
27	5.532	1386	1397	1432	rVV	358552	745974	13.13%	5.015%
28	5.834	1479	1491	1509	rBV7	17600	43443	0.76%	0.292%
29	5.921	1516	1518	1520	rVB3	190	54	0.00%	0.000%
30	5.985	1526	1538	1566	rBV	256311	536943	9.45%	3.610%
31	6.265	1623	1625	1629	rVB2	228	157	0.00%	0.001%
32	6.288	1630	1632	1635	rVB	283	131	0.00%	0.001%
33	6.313	1638	1640	1643	rVB2	389	220	0.00%	0.001%
34	6.419	1672	1673	1676	rVB	184	48	0.00%	0.000%
35	6.436	1676	1678	1679	rBV	259	87	0.00%	0.001%
36	6.747	1773	1775	1780	rBV2	324	226	0.00%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031124\
 Data File : VV034536.D
 Acq On : 11 Mar 2024 12:19
 Operator : SY/MD
 Sample : P1637-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCNR3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	6.799	1787	1791	1796	rBV2	225	267	0.00%	0.002%
38	6.911	1816	1826	1854	rBV	134026	253227	4.46%	1.703%
39	7.136	1890	1896	1897	rBV2	1166	960	0.02%	0.006%
40	7.243	1917	1929	1954	rBV	485641	856824	15.08%	5.761%
41	7.551	2017	2025	2053	rBV	89565	166128	2.92%	1.117%
42	7.799	2098	2102	2103	rBV	435	219	0.00%	0.001%
43	7.902	2120	2134	2162	rBV	3409727	5680580	100.00%	38.192%
44	8.021	2163	2171	2213	rVB	400692	723236	12.73%	4.863%
45	8.548	2332	2335	2338	rVB2	304	169	0.00%	0.001%
46	8.564	2338	2340	2341	rBV2	379	166	0.00%	0.001%
47	8.612	2351	2355	2358	rBV2	354	347	0.01%	0.002%
48	8.641	2361	2364	2366	rVB	197	88	0.00%	0.001%
49	8.657	2366	2369	2374	rBV2	283	248	0.00%	0.002%
50	8.783	2397	2408	2444	rBV	547776	899623	15.84%	6.048%
51	9.053	2490	2492	2494	rBV	189	85	0.00%	0.001%
52	9.088	2500	2503	2505	rBV2	310	194	0.00%	0.001%
53	9.127	2513	2515	2519	rVB2	322	145	0.00%	0.001%
54	9.152	2519	2523	2525	rBV	260	154	0.00%	0.001%
55	9.172	2525	2529	2532	rBV2	251	221	0.00%	0.001%
56	9.204	2537	2539	2543	rVB2	196	89	0.00%	0.001%
57	9.291	2563	2566	2567	rBV	261	95	0.00%	0.001%
58	9.879	2745	2749	2752	rBV	342	317	0.01%	0.002%
59	9.953	2769	2772	2775	rBV2	269	194	0.00%	0.001%
60	10.024	2790	2794	2795	rBV	227	109	0.00%	0.001%
61	10.075	2803	2810	2812	rBV2	163	221	0.00%	0.001%
62	10.152	2821	2834	2859	rBV	370700	588914	10.37%	3.959%
63	10.326	2877	2888	2900	rVB6	2176	3867	0.07%	0.026%
64	10.413	2912	2915	2918	rBV2	190	131	0.00%	0.001%
65	10.612	2975	2977	2978	rBV2	254	100	0.00%	0.001%
66	10.622	2978	2980	2985	rVB2	490	265	0.00%	0.002%
67	10.931	3075	3076	3077	rBV2	170	54	0.00%	0.000%
68	11.117	3130	3134	3135	rBV2	281	212	0.00%	0.001%
69	11.185	3144	3155	3179	rBV	556622	862779	15.19%	5.801%
70	11.432	3229	3232	3236	rVB3	348	229	0.00%	0.002%
71	11.516	3256	3258	3260	rBV	233	95	0.00%	0.001%
72	11.558	3260	3271	3293	rBV	527728	837792	14.75%	5.633%
73	12.471	3552	3555	3559	rBV2	449	295	0.01%	0.002%
74	12.609	3597	3598	3603	rVB2	204	146	0.00%	0.001%
75	12.747	3640	3641	3643	rBV	265	100	0.00%	0.001%
76	12.783	3650	3652	3655	rVB	437	201	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031124\
Data File : VV034536.D
Acq On : 11 Mar 2024 12:19
Operator : SY/MD
Sample : P1637-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCNR3

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Title : VOC Analysis

77	12.799	3655	3657	3660	rBV2	260	188	0.00%	0.001%
78	13.207	3781	3784	3786	rBV2	507	258	0.00%	0.002%
79	13.262	3798	3801	3804	rBV2	371	244	0.00%	0.002%




Sum of corrected areas: 14873624

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031124\
Data File : VV034536.D
Acq On : 11 Mar 2024 12:19
Operator : SY/MD
Sample : P1637-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCNR3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

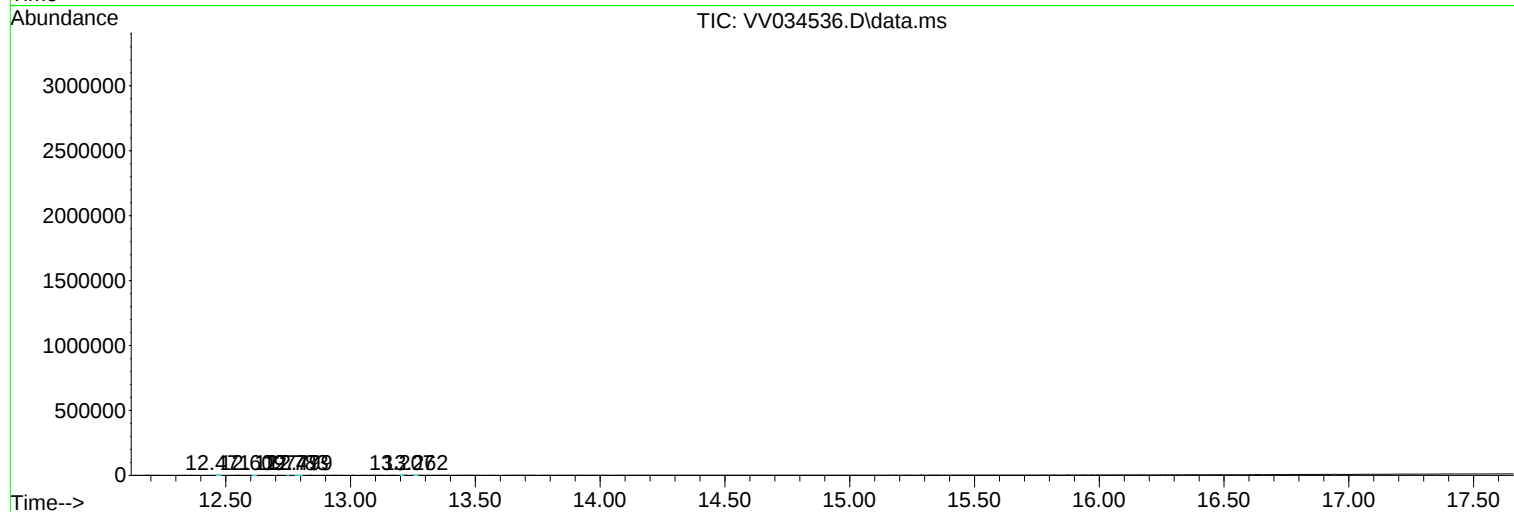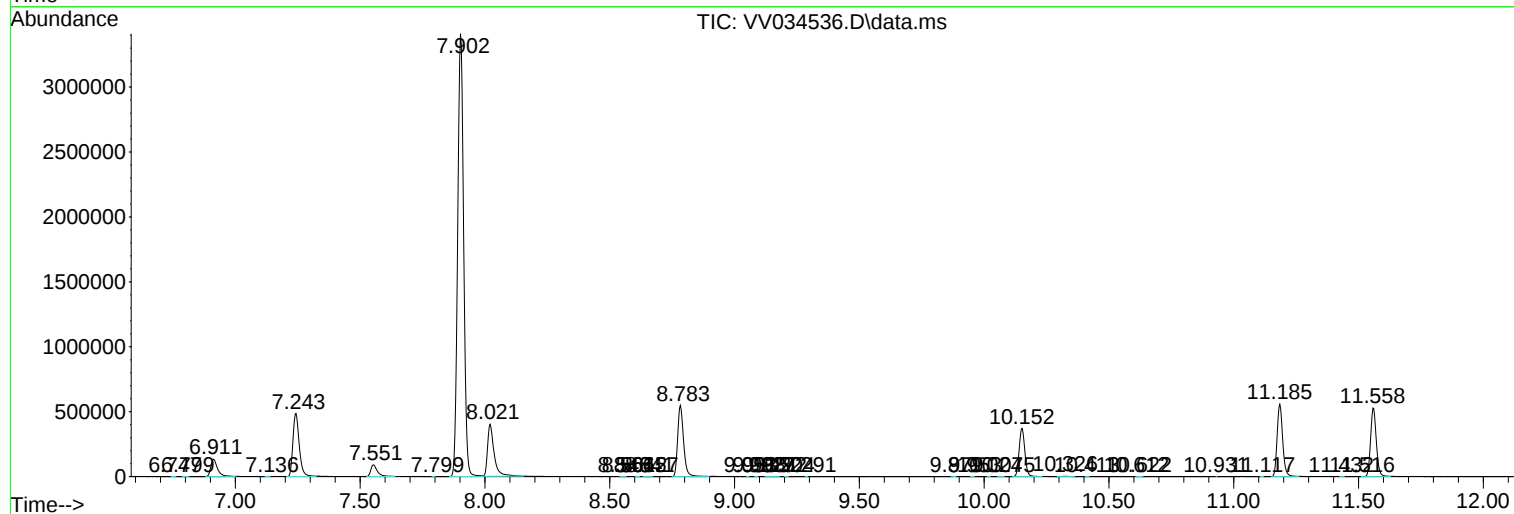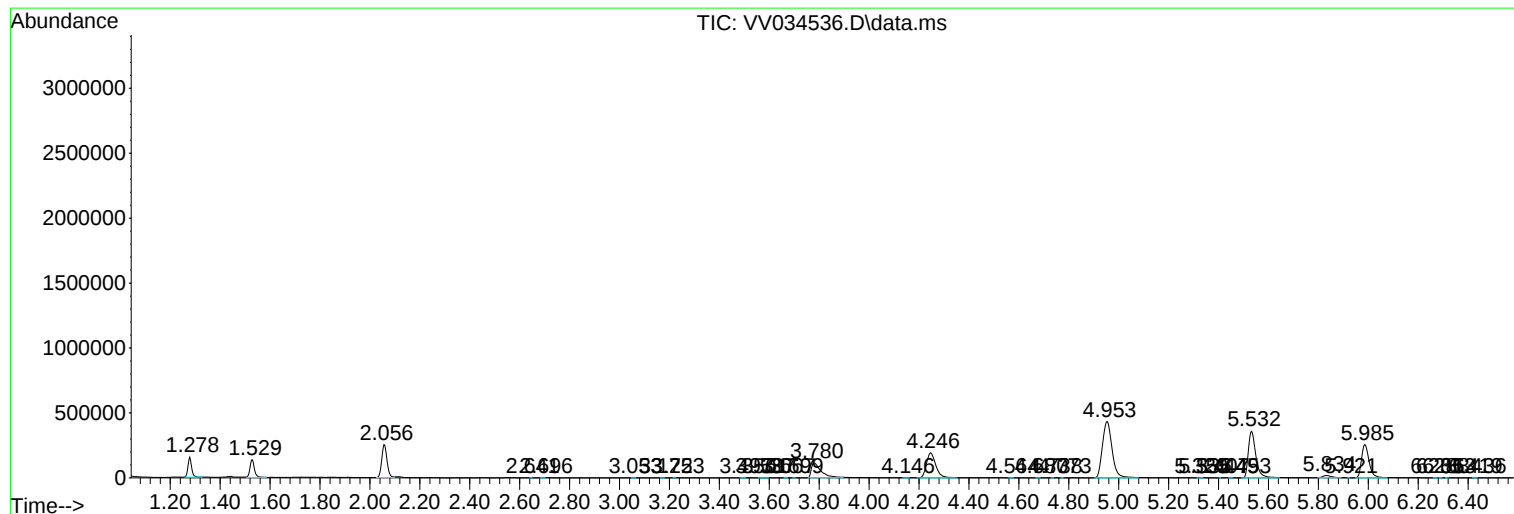

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031124\
Data File : VV034536.D
Acq On : 11 Mar 2024 12:19
Operator : SY/MD
Sample : P1637-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCNR3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031124\
Data File : VV034536.D
Acq On : 11 Mar 2024 12:19
Operator : SY/MD
Sample : P1637-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCNR3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc