

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031124\
 Data File : VV034537.D
 Acq On : 11 Mar 2024 12:43
 Operator : SY/MD
 Sample : P1637-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCNR4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034537.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	89	rVV	136991	142661	12.68%	1.594%
2	1.349	92	96	104	rVB	9936	10313	0.92%	0.115%
3	1.526	144	151	167	rVB	126240	153474	13.64%	1.715%
4	2.056	306	316	327	rBV	238445	347321	30.86%	3.881%
5	2.224	359	368	385	rVB3	5038	11435	1.02%	0.128%
6	2.291	385	389	395	rVB2	504	437	0.04%	0.005%
7	2.449	432	438	445	rBV3	1270	1622	0.14%	0.018%
8	2.558	462	472	485	rBV3	2292	4574	0.41%	0.051%
9	2.851	560	563	564	rBV	292	188	0.02%	0.002%
10	2.989	604	606	616	rVB	363	322	0.03%	0.004%
11	3.288	694	699	703	rBV2	190	223	0.02%	0.002%
12	3.330	708	712	715	rBV	311	296	0.03%	0.003%
13	3.506	763	767	769	rBV	273	208	0.02%	0.002%
14	3.780	844	852	889	rBV	107939	287417	25.54%	3.212%
15	4.130	959	961	962	rBV	283	145	0.01%	0.002%
16	4.246	981	997	1033	rBV	184995	476009	42.30%	5.319%
17	4.558	1091	1094	1096	rVB2	321	168	0.01%	0.002%
18	4.571	1096	1098	1106	rVB3	297	310	0.03%	0.003%
19	4.748	1149	1153	1154	rBV3	286	189	0.02%	0.002%
20	4.863	1185	1189	1193	rBV2	226	223	0.02%	0.002%
21	4.953	1200	1217	1250	rBV2	416900	1125304	100.00%	12.575%
22	5.439	1365	1368	1370	rBV	331	196	0.02%	0.002%
23	5.452	1370	1372	1374	rVB	347	147	0.01%	0.002%
24	5.474	1376	1379	1383	rBV2	268	194	0.02%	0.002%
25	5.532	1385	1397	1430	rBV	361176	746347	66.32%	8.340%
26	5.738	1458	1461	1465	rVB2	346	252	0.02%	0.003%
27	5.828	1479	1489	1506	rBV5	12012	26785	2.38%	0.299%
28	5.985	1525	1538	1578	rBV	255383	527716	46.90%	5.897%
29	6.162	1589	1593	1596	rBV4	439	394	0.04%	0.004%
30	6.297	1632	1635	1638	rVV2	332	307	0.03%	0.003%
31	6.313	1638	1640	1642	rVB	367	159	0.01%	0.002%
32	6.358	1652	1654	1657	rVB3	265	145	0.01%	0.002%
33	6.583	1720	1724	1728	rBV2	957	1122	0.10%	0.013%
34	6.635	1738	1740	1743	rBV3	322	158	0.01%	0.002%
35	6.657	1743	1747	1751	rVV3	426	425	0.04%	0.005%
36	6.911	1816	1826	1850	rBV	130463	249192	22.14%	2.785%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031124\
 Data File : VV034537.D
 Acq On : 11 Mar 2024 12:43
 Operator : SY/MD
 Sample : P1637-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCNR4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	7.063	1870	1873	1878	rVB4	555	598	0.05%	0.007%
38	7.243	1917	1929	1957	rBV	465938	819992	72.87%	9.163%
39	7.503	2006	2010	2012	rVV	283	218	0.02%	0.002%
40	7.555	2016	2026	2050	rBV	87598	165070	14.67%	1.845%
41	7.741	2082	2084	2086	rVB2	313	145	0.01%	0.002%
42	7.789	2097	2099	2103	rVB3	396	233	0.02%	0.003%
43	7.818	2103	2108	2112	rBV	318	290	0.03%	0.003%
44	7.841	2112	2115	2116	rBV2	285	166	0.01%	0.002%
45	7.873	2116	2125	2131	rBV3	5663	9846	0.87%	0.110%
46	8.021	2161	2171	2207	rBV	357068	664060	59.01%	7.421%
47	8.371	2277	2280	2283	rVB3	406	240	0.02%	0.003%
48	8.387	2283	2285	2291	rVB3	429	388	0.03%	0.004%
49	8.419	2291	2295	2296	rBV	321	199	0.02%	0.002%
50	8.484	2312	2315	2318	rBV3	367	280	0.02%	0.003%
51	8.538	2329	2332	2336	rBV2	354	257	0.02%	0.003%
52	8.648	2364	2366	2369	rBV	237	195	0.02%	0.002%
53	8.783	2397	2408	2439	rBV	543419	898744	79.87%	10.043%
54	9.088	2500	2503	2504	rBV	414	243	0.02%	0.003%
55	9.191	2529	2535	2540	rBV2	199	245	0.02%	0.003%
56	9.484	2624	2626	2628	rVV2	375	189	0.02%	0.002%
57	9.558	2642	2649	2654	rVB2	288	326	0.03%	0.004%
58	9.625	2663	2670	2674	rBV2	287	330	0.03%	0.004%
59	9.808	2724	2727	2731	rVB	238	176	0.02%	0.002%
60	9.895	2751	2754	2756	rVB	256	152	0.01%	0.002%
61	10.005	2785	2788	2790	rBV	269	148	0.01%	0.002%
62	10.149	2819	2833	2856	rBV	360833	574463	51.05%	6.420%
63	10.326	2878	2888	2900	rVB3	7359	11916	1.06%	0.133%
64	10.487	2935	2938	2941	rVV	280	177	0.02%	0.002%
65	10.718	3008	3010	3017	rVB2	214	219	0.02%	0.002%
66	10.895	3061	3065	3072	rBV3	352	406	0.04%	0.005%
67	11.001	3094	3098	3101	rBV2	268	272	0.02%	0.003%
68	11.120	3133	3135	3137	rBV2	353	186	0.02%	0.002%
69	11.185	3144	3155	3182	rBV	541616	860780	76.49%	9.619%
70	11.349	3202	3206	3210	rVB3	718	554	0.05%	0.006%
71	11.558	3259	3271	3295	rBV	510410	808983	71.89%	9.040%
72	11.824	3352	3354	3358	rBV3	287	233	0.02%	0.003%
73	12.197	3459	3470	3477	rBV2	2032	3153	0.28%	0.035%
74	12.268	3489	3492	3495	rBV2	288	220	0.02%	0.002%
75	12.439	3542	3545	3548	rVB	430	212	0.02%	0.002%
76	12.487	3556	3560	3563	rBV	382	269	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031124\
 Data File : VV034537.D
 Acq On : 11 Mar 2024 12:43
 Operator : SY/MD
 Sample : P1637-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCNR4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	12.522	3569	3571	3578	rVB2	287	191	0.02%	0.002%
78	12.718	3629	3632	3636	rVV2	370	249	0.02%	0.003%
79	12.873	3677	3680	3683	rBV	373	217	0.02%	0.002%
80	13.062	3736	3739	3742	rVB3	266	177	0.02%	0.002%
81	13.168	3768	3772	3775	rBB3	466	346	0.03%	0.004%
82	13.220	3784	3788	3790	rBV2	254	193	0.02%	0.002%
83	13.303	3810	3814	3816	rBV2	386	316	0.03%	0.004%
84	13.455	3856	3861	3865	rBV3	748	867	0.08%	0.010%
85	13.676	3924	3930	3931	rBV3	582	435	0.04%	0.005%
86	13.738	3946	3949	3951	rBV2	334	223	0.02%	0.002%
87	13.773	3958	3960	3965	rBV2	332	266	0.02%	0.003%
88	13.914	3999	4004	4007	rBV3	355	371	0.03%	0.004%
89	14.139	4071	4074	4076	rBV	341	179	0.02%	0.002%
90	14.168	4081	4083	4086	rBV2	288	180	0.02%	0.002%
91	14.332	4132	4134	4137	rVB2	518	295	0.03%	0.003%
92	14.400	4152	4155	4158	rBV2	571	403	0.04%	0.005%
93	14.426	4159	4163	4165	rBV2	462	328	0.03%	0.004%
94	14.657	4230	4235	4237	rBV4	620	524	0.05%	0.006%
95	14.715	4250	4253	4256	rBV3	459	392	0.03%	0.004%
96	14.731	4256	4258	4261	rVV2	443	279	0.02%	0.003%
97	14.795	4276	4278	4282	rVB	550	227	0.02%	0.003%
98	15.008	4342	4344	4345	rBV	585	217	0.02%	0.002%
99	15.033	4350	4352	4353	rBV2	568	271	0.02%	0.003%
100	15.133	4381	4383	4385	rBV3	518	284	0.03%	0.003%


Sum of corrected areas: 8948581

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031124\
Data File : VV034537.D
Acq On : 11 Mar 2024 12:43
Operator : SY/MD
Sample : P1637-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCNR4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

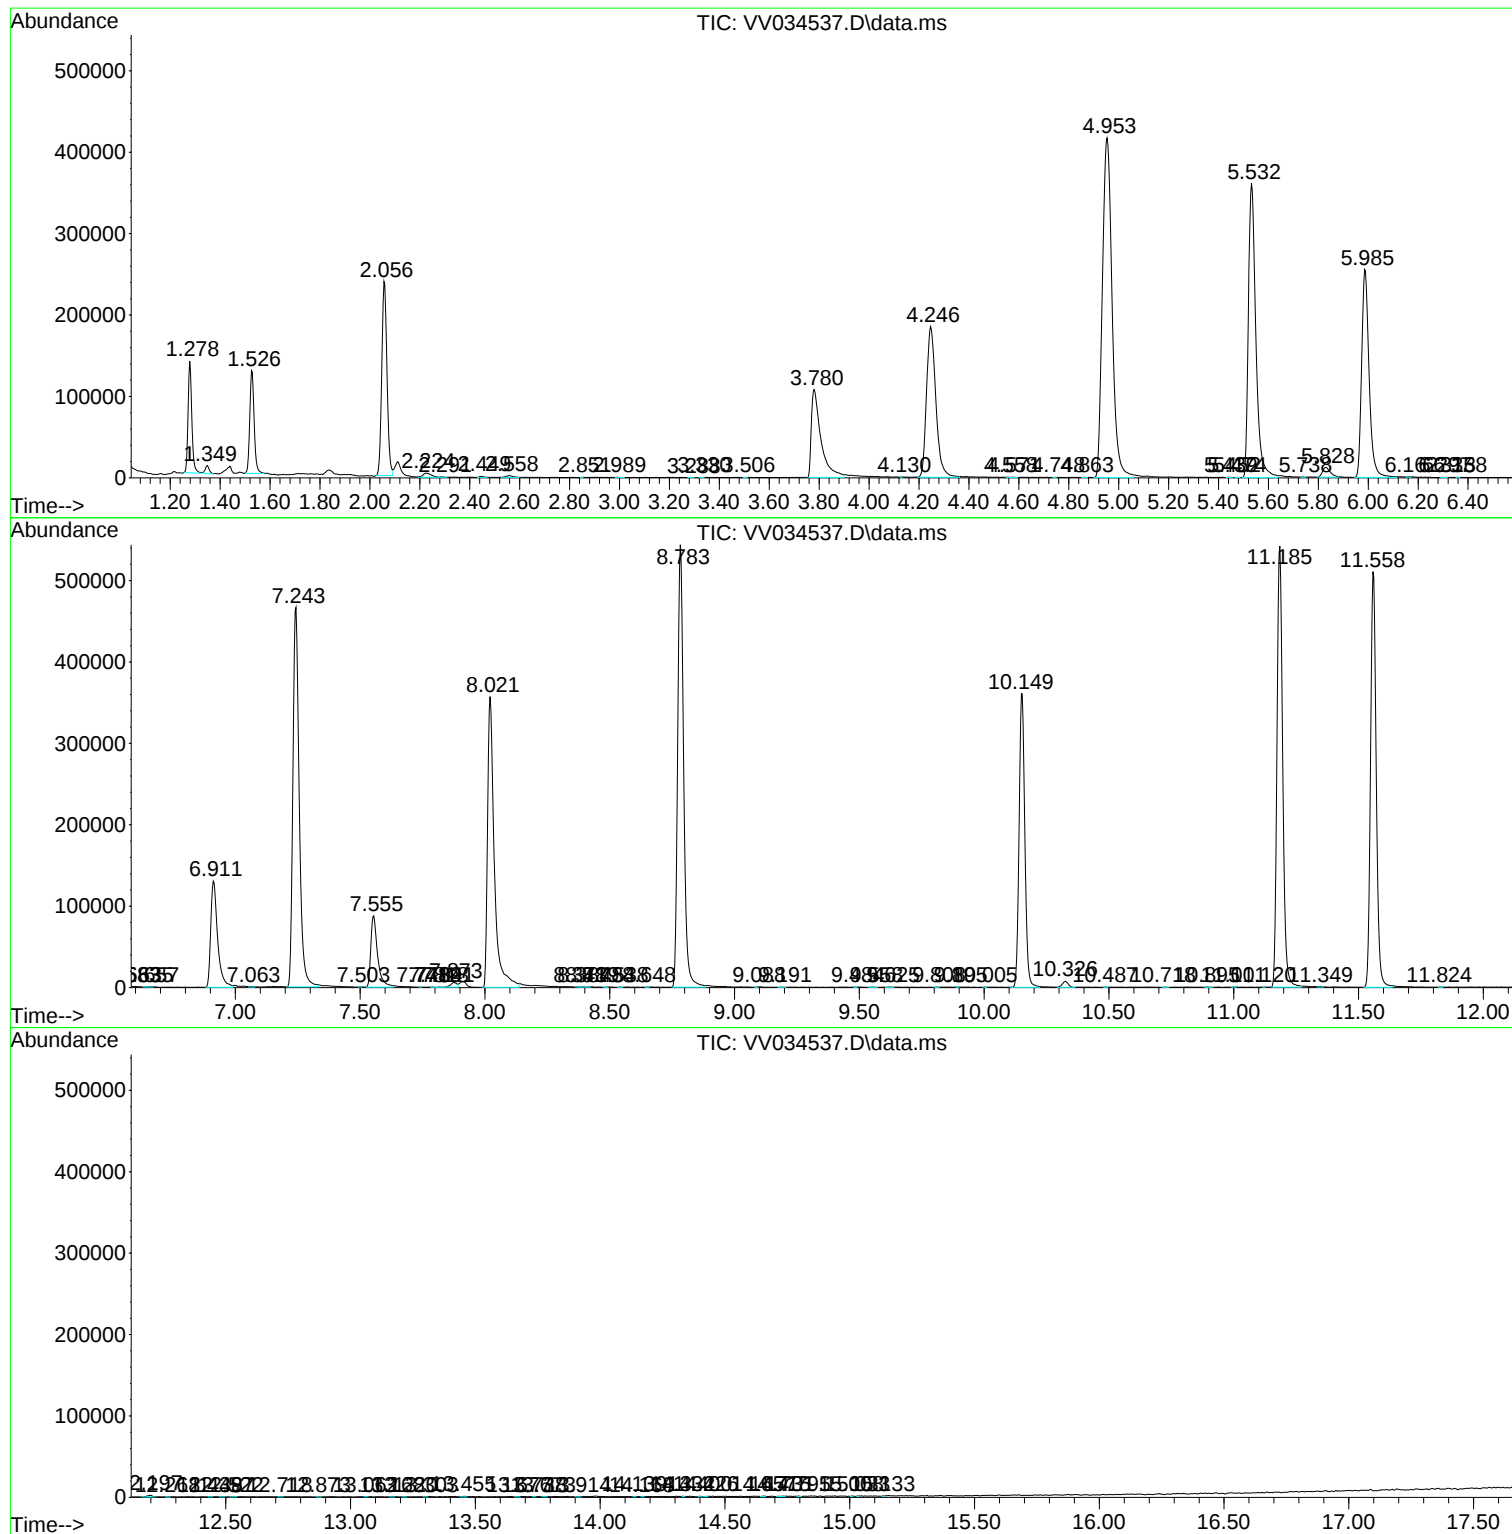

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031124\
Data File : VV034537.D
Acq On : 11 Mar 2024 12:43
Operator : SY/MD
Sample : P1637-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCNR4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031124\
Data File : VV034537.D
Acq On : 11 Mar 2024 12:43
Operator : SY/MD
Sample : P1637-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCNR4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------