

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031124\
 Data File : VV034540.D
 Acq On : 11 Mar 2024 13:54
 Operator : SY/MD
 Sample : VIBLK269
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK269

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034540.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	86	rVB	134811	140204	12.10%	1.574%
2	1.526	144	151	167	rVB	126723	152427	13.16%	1.711%
3	2.056	307	316	334	rVB	233680	334417	28.87%	3.755%
4	2.558	465	472	487	rVB6	1597	3596	0.31%	0.040%
5	2.612	487	489	491	rBV	167	68	0.01%	0.001%
6	2.703	515	517	518	rBV	196	64	0.01%	0.001%
7	2.773	536	539	542	rBV	178	121	0.01%	0.001%
8	2.789	542	544	546	rVV	174	78	0.01%	0.001%
9	2.944	589	592	595	rBV	141	100	0.01%	0.001%
10	2.976	599	602	604	rVB	335	166	0.01%	0.002%
11	3.053	619	626	628	rBV2	317	317	0.03%	0.004%
12	3.365	721	723	725	rBV	102	57	0.00%	0.001%
13	3.535	774	776	778	rBV2	80	46	0.00%	0.001%
14	3.580	787	790	792	rBV2	117	66	0.01%	0.001%
15	3.696	819	826	831	rBV2	229	266	0.02%	0.003%
16	3.719	831	833	836	rVB2	148	44	0.00%	0.000%
17	3.747	836	842	844	rBV2	158	183	0.02%	0.002%
18	3.780	844	852	895	rBV	125278	334559	28.88%	3.756%
19	4.246	981	997	1022	rBV	189653	488468	42.17%	5.484%
20	4.603	1105	1108	1109	rBV2	300	158	0.01%	0.002%
21	4.696	1136	1137	1141	rVB2	297	122	0.01%	0.001%
22	4.728	1143	1147	1154	rVV2	290	401	0.03%	0.005%
23	4.783	1158	1164	1168	rBV2	394	346	0.03%	0.004%
24	4.805	1169	1171	1173	rVB2	327	112	0.01%	0.001%
25	4.834	1177	1180	1184	rBV2	383	346	0.03%	0.004%
26	4.873	1189	1192	1197	rBV3	354	317	0.03%	0.004%
27	4.895	1197	1199	1201	rBV	301	75	0.01%	0.001%
28	4.953	1201	1217	1251	rBV2	432273	1158333	100.00%	13.005%
29	5.265	1312	1314	1315	rBV2	211	84	0.01%	0.001%
30	5.384	1349	1351	1354	rBV2	156	105	0.01%	0.001%
31	5.419	1360	1362	1365	rBV	144	52	0.00%	0.001%
32	5.432	1365	1366	1368	rVV	182	66	0.01%	0.001%
33	5.532	1386	1397	1419	rBV	333875	678832	58.60%	7.622%
34	5.828	1479	1489	1506	rBV3	13276	28585	2.47%	0.321%
35	5.985	1525	1538	1559	rBV	263136	543075	46.88%	6.097%
36	6.201	1603	1605	1610	rVB2	617	342	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031124\
 Data File : VV034540.D
 Acq On : 11 Mar 2024 13:54
 Operator : SY/MD
 Sample : VIBLK269
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK269

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	6.281	1628	1630	1632	rBV2	183	73	0.01%	0.001%
38	6.304	1635	1637	1641	rVB	489	276	0.02%	0.003%
39	6.326	1641	1644	1646	rBV2	129	78	0.01%	0.001%
40	6.342	1646	1649	1652	rVV2	232	190	0.02%	0.002%
41	6.355	1652	1653	1654	rVB	270	52	0.00%	0.001%
42	6.429	1675	1676	1677	rBV	116	26	0.00%	0.000%
43	6.590	1720	1726	1730	rBV4	846	1150	0.10%	0.013%
44	6.780	1782	1785	1789	rVB	174	108	0.01%	0.001%
45	6.834	1801	1802	1803	rVB	227	44	0.00%	0.000%
46	6.911	1815	1826	1852	rBV	133308	253833	21.91%	2.850%
47	7.243	1918	1929	1958	rBV	456914	816225	70.47%	9.164%
48	7.551	2016	2025	2049	rBV	92499	170741	14.74%	1.917%
49	7.812	2104	2106	2107	rBV	171	75	0.01%	0.001%
50	7.911	2130	2137	2147	rVB6	2326	3943	0.34%	0.044%
51	7.960	2150	2152	2153	rBV6	181	85	0.01%	0.001%
52	8.021	2162	2171	2213	rBV	422317	771199	66.58%	8.659%
53	8.538	2330	2332	2337	rBV3	386	256	0.02%	0.003%
54	8.593	2344	2349	2351	rBV3	396	405	0.03%	0.005%
55	8.744	2394	2396	2397	rBV3	343	136	0.01%	0.002%
56	8.783	2397	2408	2434	rVV	499984	819708	70.77%	9.203%
57	9.091	2501	2504	2507	rBV	233	162	0.01%	0.002%
58	9.123	2513	2514	2517	rVB2	251	94	0.01%	0.001%
59	9.210	2537	2541	2544	rVB2	235	150	0.01%	0.002%
60	9.246	2550	2552	2556	rVB	238	134	0.01%	0.002%
61	9.268	2556	2559	2561	rBV	172	109	0.01%	0.001%
62	9.307	2568	2571	2573	rBV	153	122	0.01%	0.001%
63	9.371	2587	2591	2594	rVB3	255	159	0.01%	0.002%
64	9.400	2598	2600	2603	rBV2	142	100	0.01%	0.001%
65	9.490	2625	2628	2631	rVB	284	141	0.01%	0.002%
66	9.503	2631	2632	2635	rBV	180	113	0.01%	0.001%
67	9.567	2647	2652	2657	rBV2	276	359	0.03%	0.004%
68	9.590	2657	2659	2663	rBV	202	126	0.01%	0.001%
69	9.641	2672	2675	2677	rBV2	206	111	0.01%	0.001%
70	9.693	2688	2691	2692	rBV	218	124	0.01%	0.001%
71	9.715	2695	2698	2703	rBB	143	100	0.01%	0.001%
72	9.747	2703	2708	2710	rBV	190	167	0.01%	0.002%
73	9.972	2776	2778	2781	rVB	263	98	0.01%	0.001%
74	10.152	2822	2834	2856	rBV	397056	619332	53.47%	6.954%
75	10.374	2901	2903	2908	rVB2	249	121	0.01%	0.001%
76	10.792	3031	3033	3035	rBV	203	101	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031124\
 Data File : VV034540.D
 Acq On : 11 Mar 2024 13:54
 Operator : SY/MD
 Sample : VIBLK269
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK269

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M

Title : VOC Analysis

77	11.001	3096	3098	3101	rBV	279	147	0.01%	0.002%
78	11.184	3144	3155	3184	rBV	496936	777054	67.08%	8.724%
79	11.561	3258	3272	3301	rBV	498461	801314	69.18%	8.997%
80	11.869	3366	3368	3369	rBV	148	38	0.00%	0.000%
81	12.297	3499	3501	3502	rBV	194	71	0.01%	0.001%
82	12.471	3553	3555	3558	rBV2	286	157	0.01%	0.002%
83	13.053	3733	3736	3739	rBV	329	286	0.02%	0.003%
84	13.503	3874	3876	3882	rBV	656	271	0.02%	0.003%
85	13.924	4003	4007	4012	rVB4	323	290	0.03%	0.003%




Sum of corrected areas: 8906752

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031124\
Data File : VV034540.D
Acq On : 11 Mar 2024 13:54
Operator : SY/MD
Sample : VIBLK269
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK269

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

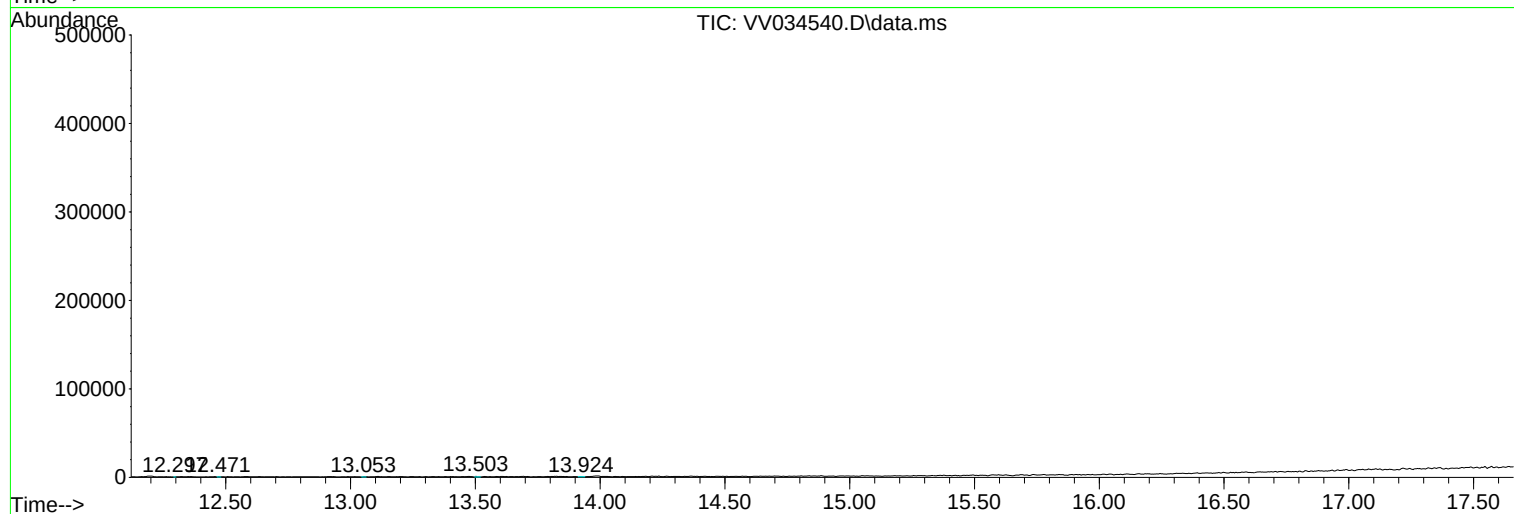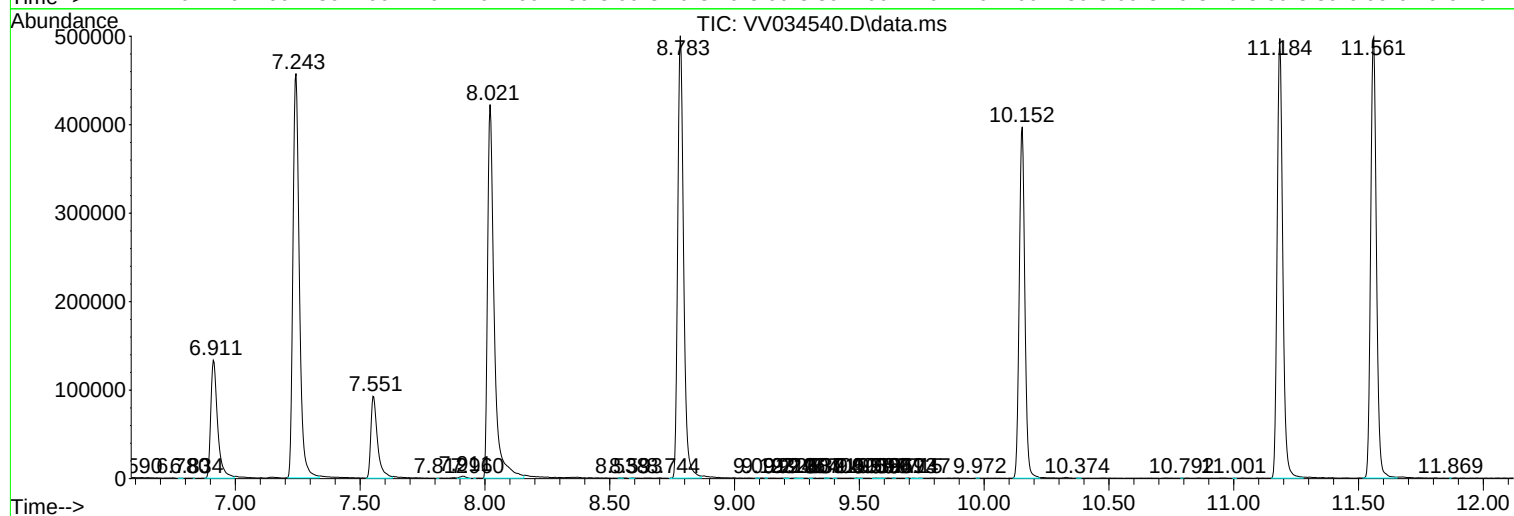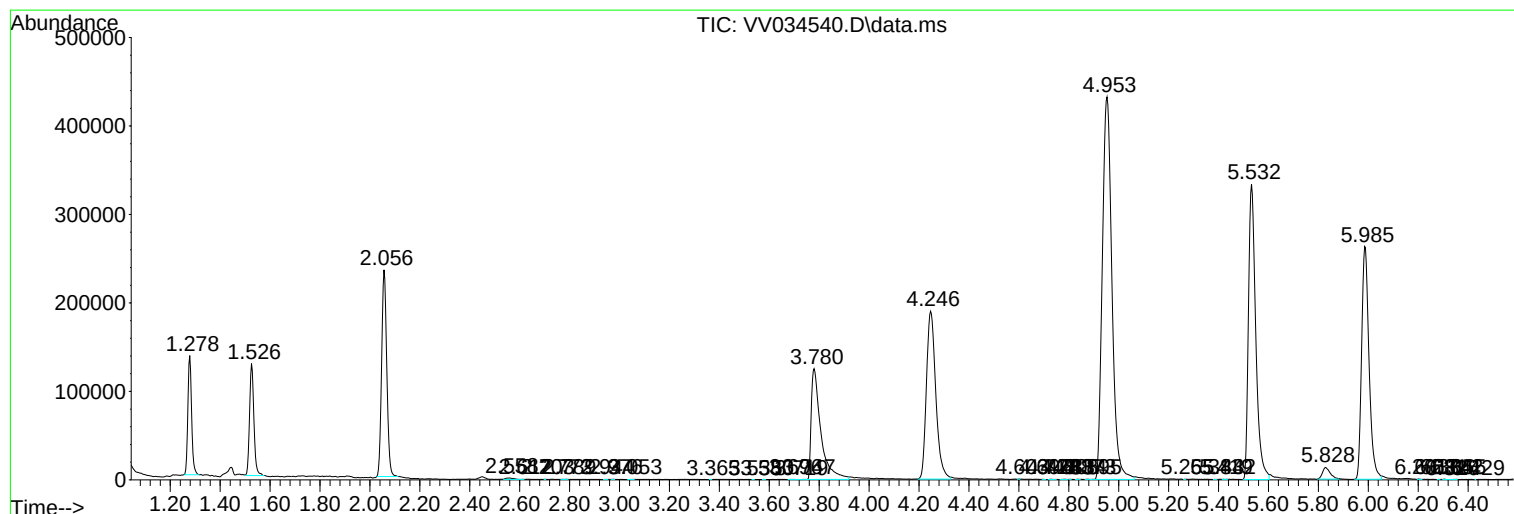

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031124\
Data File : VV034540.D
Acq On : 11 Mar 2024 13:54
Operator : SY/MD
Sample : VIBLK269
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK269

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031124\
Data File : VV034540.D
Acq On : 11 Mar 2024 13:54
Operator : SY/MD
Sample : VIBLK269
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK269

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------