

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031124\
 Data File : VV034541.D
 Acq On : 11 Mar 2024 14:18
 Operator : SY/MD
 Sample : P1637-09DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCNR3DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M

Title : VOC Analysis

Signal : TIC: VV034541.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	90	rVB	155485	155426	13.23%	1.513%
2	1.526	145	151	165	rVB	131330	155727	13.26%	1.515%
3	2.056	306	316	350	rVB	256183	389649	33.17%	3.792%
4	2.388	414	419	426	rBV3	554	655	0.06%	0.006%
5	2.449	428	438	448	rVB2	4123	6866	0.58%	0.067%
6	2.503	454	455	456	rBV2	214	50	0.00%	0.000%
7	2.558	463	472	480	rBV4	1697	2909	0.25%	0.028%
8	2.735	524	527	532	rBV2	225	181	0.02%	0.002%
9	2.886	571	574	576	rBV	180	102	0.01%	0.001%
10	3.037	617	621	624	rBV	319	274	0.02%	0.003%
11	3.153	654	657	659	rBV	172	104	0.01%	0.001%
12	3.230	678	681	682	rBV2	224	130	0.01%	0.001%
13	3.259	687	690	692	rBV	139	73	0.01%	0.001%
14	3.291	697	700	703	rBV2	197	109	0.01%	0.001%
15	3.365	721	723	725	rBV	69	33	0.00%	0.000%
16	3.494	761	763	765	rVB2	159	63	0.01%	0.001%
17	3.577	787	789	792	rBV2	110	58	0.00%	0.001%
18	3.616	795	801	805	rBV2	195	198	0.02%	0.002%
19	3.638	805	808	810	rBV2	118	68	0.01%	0.001%
20	3.674	816	819	822	rBV2	171	119	0.01%	0.001%
21	3.732	832	837	841	rBV2	166	205	0.02%	0.002%
22	3.780	843	852	889	rBV	118743	317958	27.07%	3.094%
23	4.246	981	997	1028	rBV2	193558	500412	42.60%	4.870%
24	4.587	1101	1103	1108	rVB2	437	258	0.02%	0.003%
25	4.635	1116	1118	1122	rVB	413	214	0.02%	0.002%
26	4.661	1124	1126	1128	rVB	419	112	0.01%	0.001%
27	4.674	1128	1130	1132	rBV2	262	115	0.01%	0.001%
28	4.699	1137	1138	1139	rBV	268	72	0.01%	0.001%
29	4.732	1146	1148	1150	rBV2	225	94	0.01%	0.001%
30	4.841	1177	1182	1186	rBV2	439	402	0.03%	0.004%
31	4.860	1186	1188	1190	rBV2	312	206	0.02%	0.002%
32	4.953	1198	1217	1249	rBV2	443848	1174781	100.00%	11.432%
33	5.346	1338	1339	1342	rVB2	328	105	0.01%	0.001%
34	5.413	1355	1360	1361	rBV2	184	161	0.01%	0.002%
35	5.490	1380	1384	1386	rBV3	349	286	0.02%	0.003%
36	5.532	1386	1397	1428	rBV	364102	744558	63.38%	7.246%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031124\
 Data File : VV034541.D
 Acq On : 11 Mar 2024 14:18
 Operator : SY/MD
 Sample : P1637-09DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCNR3DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	5.831	1480	1490	1510	rVB6	12600	28209	2.40%	0.275%
38	5.985	1525	1538	1565	rBV2	261017	547391	46.60%	5.327%
39	6.272	1625	1627	1631	rVB2	230	96	0.01%	0.001%
40	6.291	1631	1633	1635	rBV	231	88	0.01%	0.001%
41	6.336	1644	1647	1649	rBV2	235	155	0.01%	0.002%
42	6.387	1660	1663	1665	rBV	209	128	0.01%	0.001%
43	6.567	1715	1719	1720	rBV2	248	170	0.01%	0.002%
44	6.786	1785	1787	1794	rVB2	315	263	0.02%	0.003%
45	6.818	1794	1797	1803	rVB2	333	329	0.03%	0.003%
46	6.847	1803	1806	1807	rBV	78	43	0.00%	0.000%
47	6.912	1816	1826	1850	rBV	137916	258554	22.01%	2.516%
48	7.243	1918	1929	1955	rBV	488145	862711	73.44%	8.396%
49	7.551	2016	2025	2051	rBV	93032	172475	14.68%	1.678%
50	7.747	2084	2086	2088	rBV	225	146	0.01%	0.001%
51	7.786	2096	2098	2099	rBV	125	29	0.00%	0.000%
52	7.828	2110	2111	2112	rBV	110	31	0.00%	0.000%
53	7.902	2122	2134	2158	rBV	620976	1045667	89.01%	10.176%
54	8.021	2162	2171	2206	rBV	411487	727074	61.89%	7.076%
55	8.535	2330	2331	2332	rBV	129	39	0.00%	0.000%
56	8.583	2344	2346	2347	rBV	223	83	0.01%	0.001%
57	8.593	2347	2349	2352	rVB2	330	138	0.01%	0.001%
58	8.783	2398	2408	2437	rBV	546611	896192	76.29%	8.721%
59	9.018	2478	2481	2483	rBV	393	222	0.02%	0.002%
60	9.085	2499	2502	2504	rVB	292	156	0.01%	0.002%
61	9.111	2505	2510	2514	rVV4	379	302	0.03%	0.003%
62	9.169	2526	2528	2529	rBV2	177	50	0.00%	0.000%
63	9.214	2540	2542	2543	rBV2	266	90	0.01%	0.001%
64	9.448	2613	2615	2617	rBV	184	91	0.01%	0.001%
65	9.600	2660	2662	2669	rVB2	218	104	0.01%	0.001%
66	9.661	2678	2681	2683	rVB2	125	64	0.01%	0.001%
67	9.680	2684	2687	2688	rBV	162	89	0.01%	0.001%
68	9.741	2703	2706	2709	rBV2	151	124	0.01%	0.001%
69	9.760	2710	2712	2717	rVB2	288	157	0.01%	0.002%
70	9.915	2757	2760	2765	rBV2	181	175	0.01%	0.002%
71	9.963	2773	2775	2781	rVB2	251	185	0.02%	0.002%
72	10.153	2822	2834	2855	rBV	384231	607297	51.69%	5.910%
73	10.484	2934	2937	2940	rVB2	294	137	0.01%	0.001%
74	10.529	2943	2951	2953	rBV2	284	366	0.03%	0.004%
75	10.706	3004	3006	3008	rBV2	109	51	0.00%	0.000%
76	10.744	3017	3018	3019	rBV2	178	60	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031124\
Data File : VV034541.D
Acq On : 11 Mar 2024 14:18
Operator : SY/MD
Sample : P1637-09DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCNR3DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M

Title : VOC Analysis

77	11.185	3144	3155	3182	rBV	539976	842813	71.74%	8.202%
78	11.558	3260	3271	3295	rBV	518665	829055	70.57%	8.068%
79	11.844	3357	3360	3365	rBV2	362	285	0.02%	0.003%
80	12.030	3416	3418	3420	rBV2	348	176	0.01%	0.002%
81	12.178	3461	3464	3466	rBV2	376	258	0.02%	0.003%
82	13.336	3821	3824	3826	rBV2	314	179	0.02%	0.002%
83	13.850	3982	3984	3989	rBV2	377	350	0.03%	0.003%
84	14.866	4298	4300	4301	rBV	683	242	0.02%	0.002%




Sum of corrected areas: 10275822

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031124\
Data File : VV034541.D
Acq On : 11 Mar 2024 14:18
Operator : SY/MD
Sample : P1637-09DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCNR3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

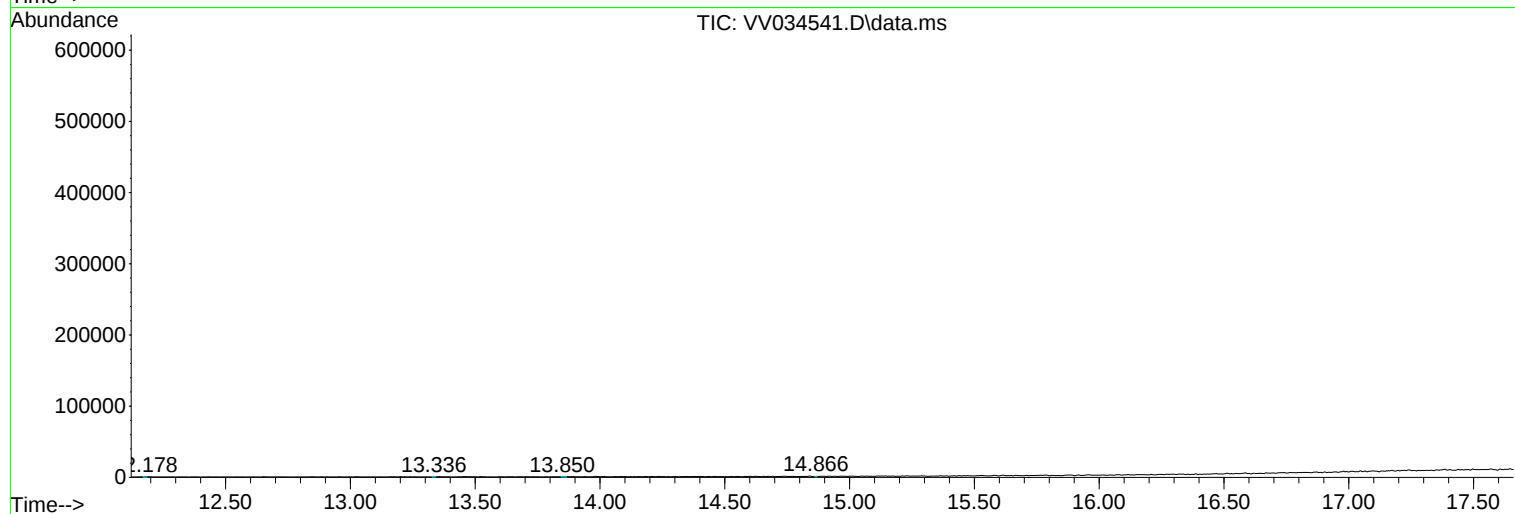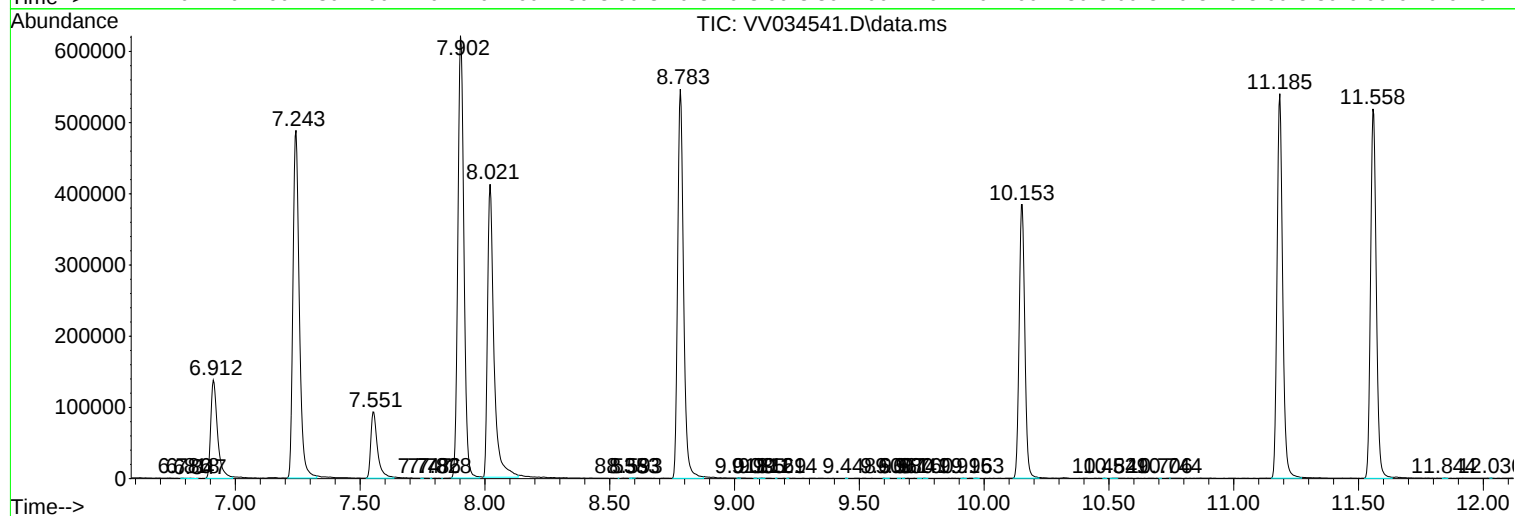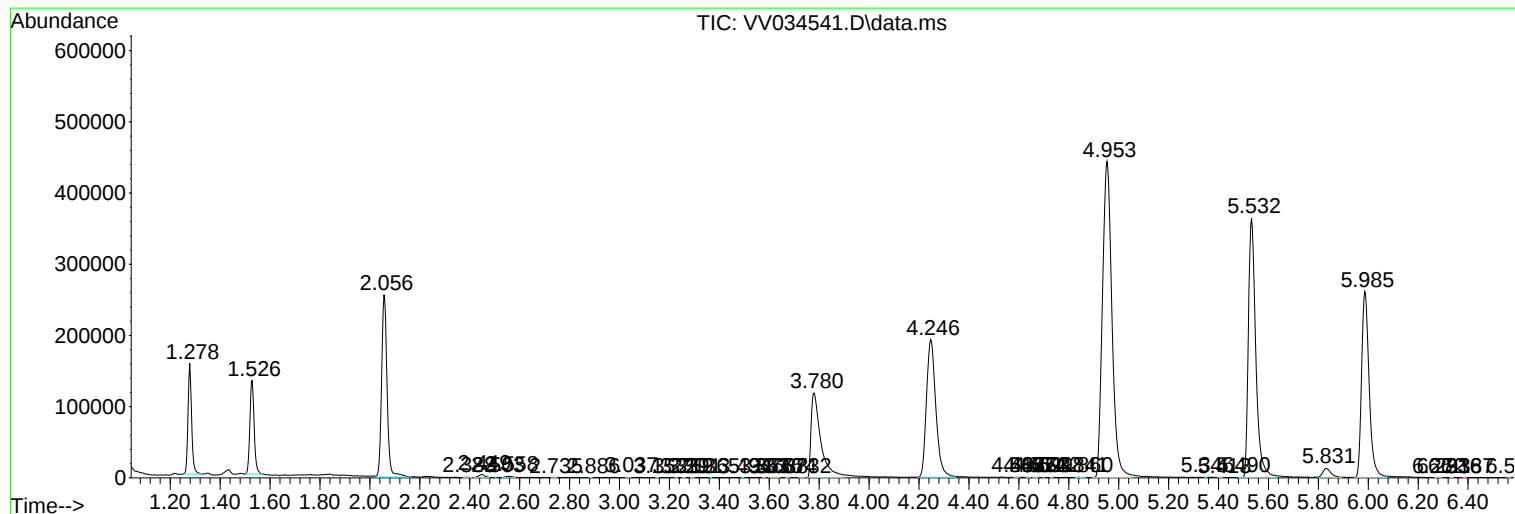

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031124\
Data File : VV034541.D
Acq On : 11 Mar 2024 14:18
Operator : SY/MD
Sample : P1637-09DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCNR3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031124\
Data File : VV034541.D
Acq On : 11 Mar 2024 14:18
Operator : SY/MD
Sample : P1637-09DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCNR3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------