

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031124\
 Data File : VV034546.D
 Acq On : 11 Mar 2024 16:29
 Operator : SY/MD
 Sample : P1637-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034546.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	89	rVB	149358	155619	13.22%	1.663%
2	1.526	144	151	170	rVB	134148	165831	14.09%	1.772%
3	2.056	306	316	340	rBV	259043	380645	32.34%	4.068%
4	2.449	431	438	447	rVB4	2147	3164	0.27%	0.034%
5	2.484	447	449	450	rBV	299	78	0.01%	0.001%
6	2.523	459	461	465	rBV2	198	144	0.01%	0.002%
7	2.651	498	501	507	rBV2	153	197	0.02%	0.002%
8	2.700	513	516	519	rBV3	319	217	0.02%	0.002%
9	2.770	536	538	539	rBV	227	87	0.01%	0.001%
10	3.015	606	614	615	rBV2	266	285	0.02%	0.003%
11	3.085	634	636	642	rBV2	192	168	0.01%	0.002%
12	3.121	645	647	650	rBV	204	81	0.01%	0.001%
13	3.191	666	669	670	rBV	246	110	0.01%	0.001%
14	3.291	695	700	705	rBV	216	228	0.02%	0.002%
15	3.320	705	709	712	rVB	167	123	0.01%	0.001%
16	3.339	712	715	717	rBV	177	113	0.01%	0.001%
17	3.442	745	747	750	rVB2	137	78	0.01%	0.001%
18	3.462	750	753	759	rBV2	198	180	0.02%	0.002%
19	3.526	770	773	775	rBV2	143	79	0.01%	0.001%
20	3.568	784	786	789	rVB2	175	95	0.01%	0.001%
21	3.606	795	798	802	rVB2	153	110	0.01%	0.001%
22	3.629	802	805	812	rVB2	171	191	0.02%	0.002%
23	3.674	812	819	823	rBV2	265	275	0.02%	0.003%
24	3.699	823	827	831	rBV2	218	219	0.02%	0.002%
25	3.780	844	852	893	rBV	122355	327302	27.80%	3.498%
26	4.246	982	997	1034	rBV	194303	497651	42.28%	5.319%
27	4.648	1120	1122	1124	rBV	234	157	0.01%	0.002%
28	4.674	1128	1130	1133	rVB	176	78	0.01%	0.001%
29	4.699	1135	1138	1139	rBV	250	119	0.01%	0.001%
30	4.741	1149	1151	1156	rBV2	232	160	0.01%	0.002%
31	4.767	1156	1159	1161	rBV2	179	121	0.01%	0.001%
32	4.825	1175	1177	1182	rVB2	351	231	0.02%	0.002%
33	4.851	1183	1185	1187	rBV2	148	85	0.01%	0.001%
34	4.953	1201	1217	1249	rBV2	441486	1177134	100.00%	12.581%
35	5.243	1305	1307	1311	rBV2	410	256	0.02%	0.003%
36	5.336	1333	1336	1337	rBV2	264	151	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031124\
 Data File : VV034546.D
 Acq On : 11 Mar 2024 16:29
 Operator : SY/MD
 Sample : P1637-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	5.394	1351	1354	1355	rBV	299	115	0.01%	0.001%
38	5.410	1357	1359	1361	rBV	174	86	0.01%	0.001%
39	5.449	1368	1371	1373	rBV	289	165	0.01%	0.002%
40	5.532	1385	1397	1430	rBV	369511	759152	64.49%	8.114%
41	5.831	1480	1490	1506	rBV3	13262	27670	2.35%	0.296%
42	5.915	1515	1516	1520	rVB	270	110	0.01%	0.001%
43	5.986	1526	1538	1569	rBV	263653	551512	46.85%	5.894%
44	6.178	1596	1598	1600	rBV	379	194	0.02%	0.002%
45	6.220	1609	1611	1614	rBV2	463	345	0.03%	0.004%
46	6.269	1622	1626	1629	rBV2	315	314	0.03%	0.003%
47	6.429	1673	1676	1678	rBV2	193	136	0.01%	0.001%
48	6.442	1678	1680	1685	rVB2	333	173	0.01%	0.002%
49	6.564	1716	1718	1720	rBV	157	80	0.01%	0.001%
50	6.580	1720	1723	1726	rBV2	638	557	0.05%	0.006%
51	6.693	1755	1758	1760	rBV	286	170	0.01%	0.002%
52	6.719	1764	1766	1770	rVB3	420	214	0.02%	0.002%
53	6.738	1770	1772	1776	rBV2	324	261	0.02%	0.003%
54	6.828	1798	1800	1803	rBV	226	99	0.01%	0.001%
55	6.912	1816	1826	1857	rBV	138125	261344	22.20%	2.793%
56	7.243	1917	1929	1956	rBV	490042	865292	73.51%	9.248%
57	7.551	2016	2025	2051	rBV	94910	174261	14.80%	1.862%
58	7.812	2103	2106	2109	rBV3	219	177	0.02%	0.002%
59	7.879	2117	2127	2130	rBV3	587	991	0.08%	0.011%
60	7.912	2133	2137	2145	rVB4	1098	1259	0.11%	0.013%
61	7.966	2151	2154	2155	rBV	147	92	0.01%	0.001%
62	8.021	2162	2171	2205	rBV	418045	743681	63.18%	7.948%
63	8.683	2375	2377	2378	rBV	162	91	0.01%	0.001%
64	8.693	2378	2380	2383	rVB2	282	133	0.01%	0.001%
65	8.783	2397	2408	2443	rBV	557952	904453	76.84%	9.667%
66	9.037	2485	2487	2490	rVB2	331	194	0.02%	0.002%
67	9.220	2542	2544	2548	rBV2	196	111	0.01%	0.001%
68	9.272	2557	2560	2564	rVB2	177	151	0.01%	0.002%
69	9.394	2596	2598	2602	rVB	212	133	0.01%	0.001%
70	9.458	2614	2618	2621	rVB2	233	179	0.02%	0.002%
71	9.493	2624	2629	2635	rBV2	642	646	0.05%	0.007%
72	9.538	2641	2643	2646	rBV2	340	235	0.02%	0.003%
73	9.654	2677	2679	2681	rBV2	224	93	0.01%	0.001%
74	9.809	2724	2727	2728	rBV	236	135	0.01%	0.001%
75	9.870	2744	2746	2748	rBV	340	228	0.02%	0.002%
76	9.953	2761	2772	2776	rBV	362	677	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031124\
 Data File : VV034546.D
 Acq On : 11 Mar 2024 16:29
 Operator : SY/MD
 Sample : P1637-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	9.989	2780	2783	2785	rBV	202	106	0.01%	0.001%
78	10.149	2821	2833	2856	rBV	385957	611669	51.96%	6.537%
79	10.288	2874	2876	2877	rBV	251	81	0.01%	0.001%
80	10.317	2882	2885	2887	rBV3	628	448	0.04%	0.005%
81	10.487	2932	2938	2943	rBV4	595	778	0.07%	0.008%
82	10.616	2975	2978	2981	rBV2	233	145	0.01%	0.002%
83	10.667	2991	2994	2999	rBV2	168	183	0.02%	0.002%
84	10.722	3008	3011	3017	rVB	271	163	0.01%	0.002%
85	10.799	3032	3035	3040	rVB	598	415	0.04%	0.004%
86	10.828	3040	3044	3046	rBV	212	154	0.01%	0.002%
87	11.130	3130	3138	3143	rBV4	1395	1643	0.14%	0.018%
88	11.185	3144	3155	3178	rBV	557884	862234	73.25%	9.215%
89	11.362	3208	3210	3214	rBV3	625	443	0.04%	0.005%
90	11.419	3225	3228	3230	rBV2	328	202	0.02%	0.002%
91	11.558	3259	3271	3294	rBV	533805	840926	71.44%	8.988%
92	12.091	3434	3437	3442	rBV3	293	308	0.03%	0.003%
93	12.345	3514	3516	3521	rBV2	236	201	0.02%	0.002%
94	12.590	3587	3592	3602	rBV5	1392	2127	0.18%	0.023%
95	12.882	3681	3683	3685	rVB2	223	91	0.01%	0.001%
96	13.207	3778	3784	3794	rBV5	2866	4258	0.36%	0.046%
97	13.448	3851	3859	3871	rBV	9831	16318	1.39%	0.174%
98	13.686	3927	3933	3946	rVB5	3636	5468	0.46%	0.058%
99	14.033	4036	4041	4042	rBV2	320	307	0.03%	0.003%
100	14.185	4086	4088	4090	rBV2	409	204	0.02%	0.002%




Sum of corrected areas: 9356543

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031124\
Data File : VV034546.D
Acq On : 11 Mar 2024 16:29
Operator : SY/MD
Sample : P1637-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

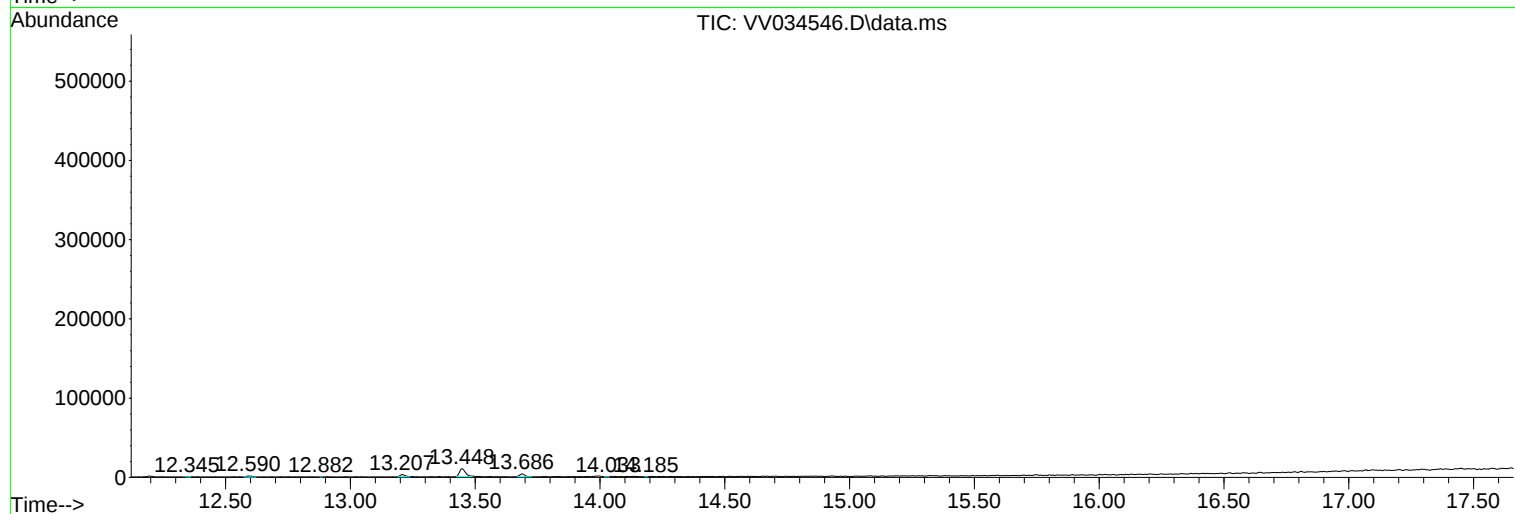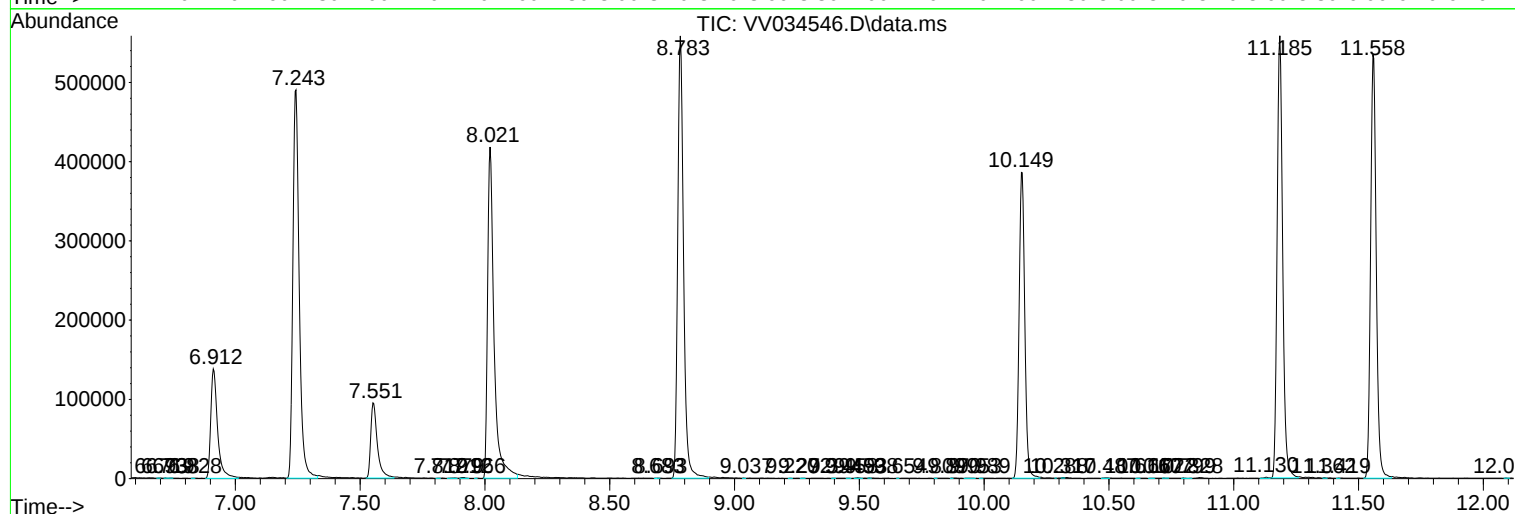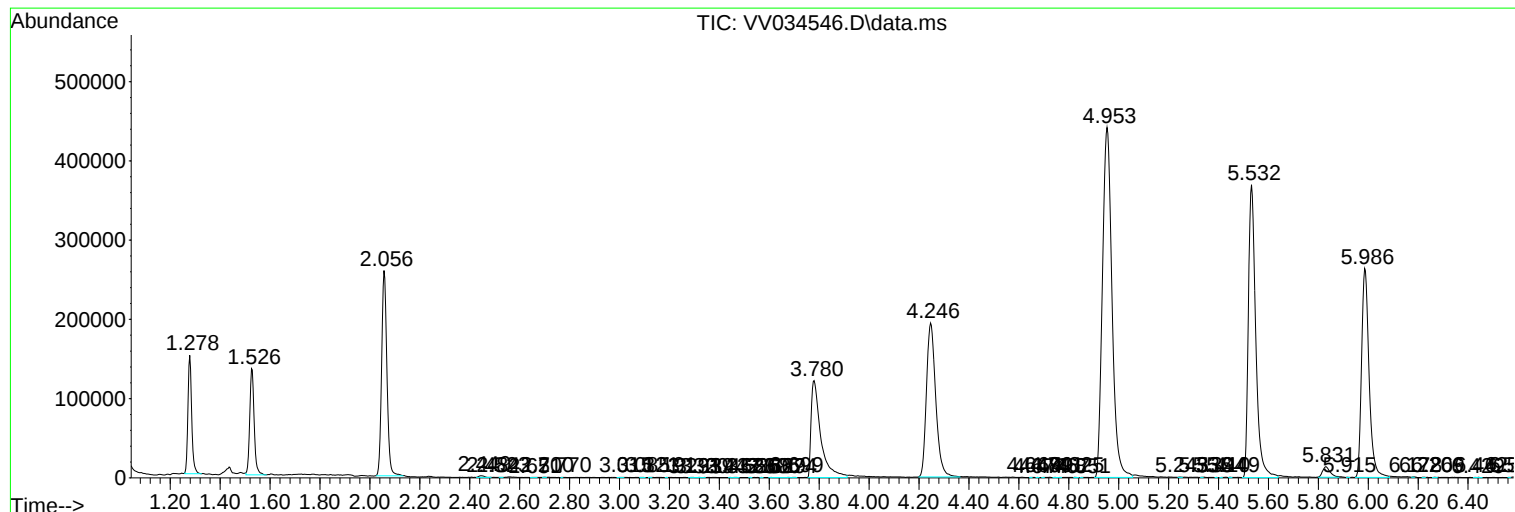

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031124\
Data File : VV034546.D
Acq On : 11 Mar 2024 16:29
Operator : SY/MD
Sample : P1637-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031124\
Data File : VV034546.D
Acq On : 11 Mar 2024 16:29
Operator : SY/MD
Sample : P1637-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------