

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031219\
 Data File : VV009609.D
 Acq On : 12 Mar 2019 17:30
 Operator : SY/MD
 Sample : K1789-02ME
 Misc : 5.59g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFON8ME

Quant Time: Mar 13 05:06:39 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031219WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 13 02:20:07 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	163408	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	158407	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	72058	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	39288	40.62	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	81.24%
7) Chloroethane-d5	1.55	69	23162	23.01	ug/L	-0.03
Spiked Amount	50.000	Range	70 - 130	Recovery	=	46.02%#
11) 1,1-Dichloroethene-d2	2.10	63	90704	35.55	ug/L	-0.03
Spiked Amount	50.000	Range	60 - 125	Recovery	=	71.10%
21) 2-Butanone-d5	3.95	46	59237	82.88	ug/L	0.02
Spiked Amount	100.000	Range	40 - 130	Recovery	=	82.88%
24) Chloroform-d	4.40	84	90345	42.76	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	85.52%
26) 1,2-Dichloroethane-d4	5.08	65	65761	47.04	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.08%
32) Benzene-d6	5.09	84	196995	47.83	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.66%
36) 1,2-Dichloropropane-d6	6.12	67	60897	49.44	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	98.88%
41) Toluene-d8	7.36	98	193712	48.27	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	96.54%
43) trans-1,3-Dichloropropene-	7.67	79	29322	46.09	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	92.18%
47) 2-Hexanone-d5	8.14	63	54065	100.36	ug/L	0.02
Spiked Amount	100.000	Range	45 - 130	Recovery	=	100.36%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	93778	47.40	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	94.80%
64) 1,2-Dichlorobenzene-d4	11.68	152	69645	45.82	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	91.64%


Target Compounds					Qvalue
46) Tetrachloroethene	8.02	164	10615	12.724 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV031219\
Data File : VV009609.D
Acq On : 12 Mar 2019 17:30
Operator : SY/MD
Sample : K1789-02ME
Misc : 5.59g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BF0N8ME

Quant Time: Mar 13 05:06:39 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031219WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Mar 13 02:20:07 2019
Response via : Initial Calibration

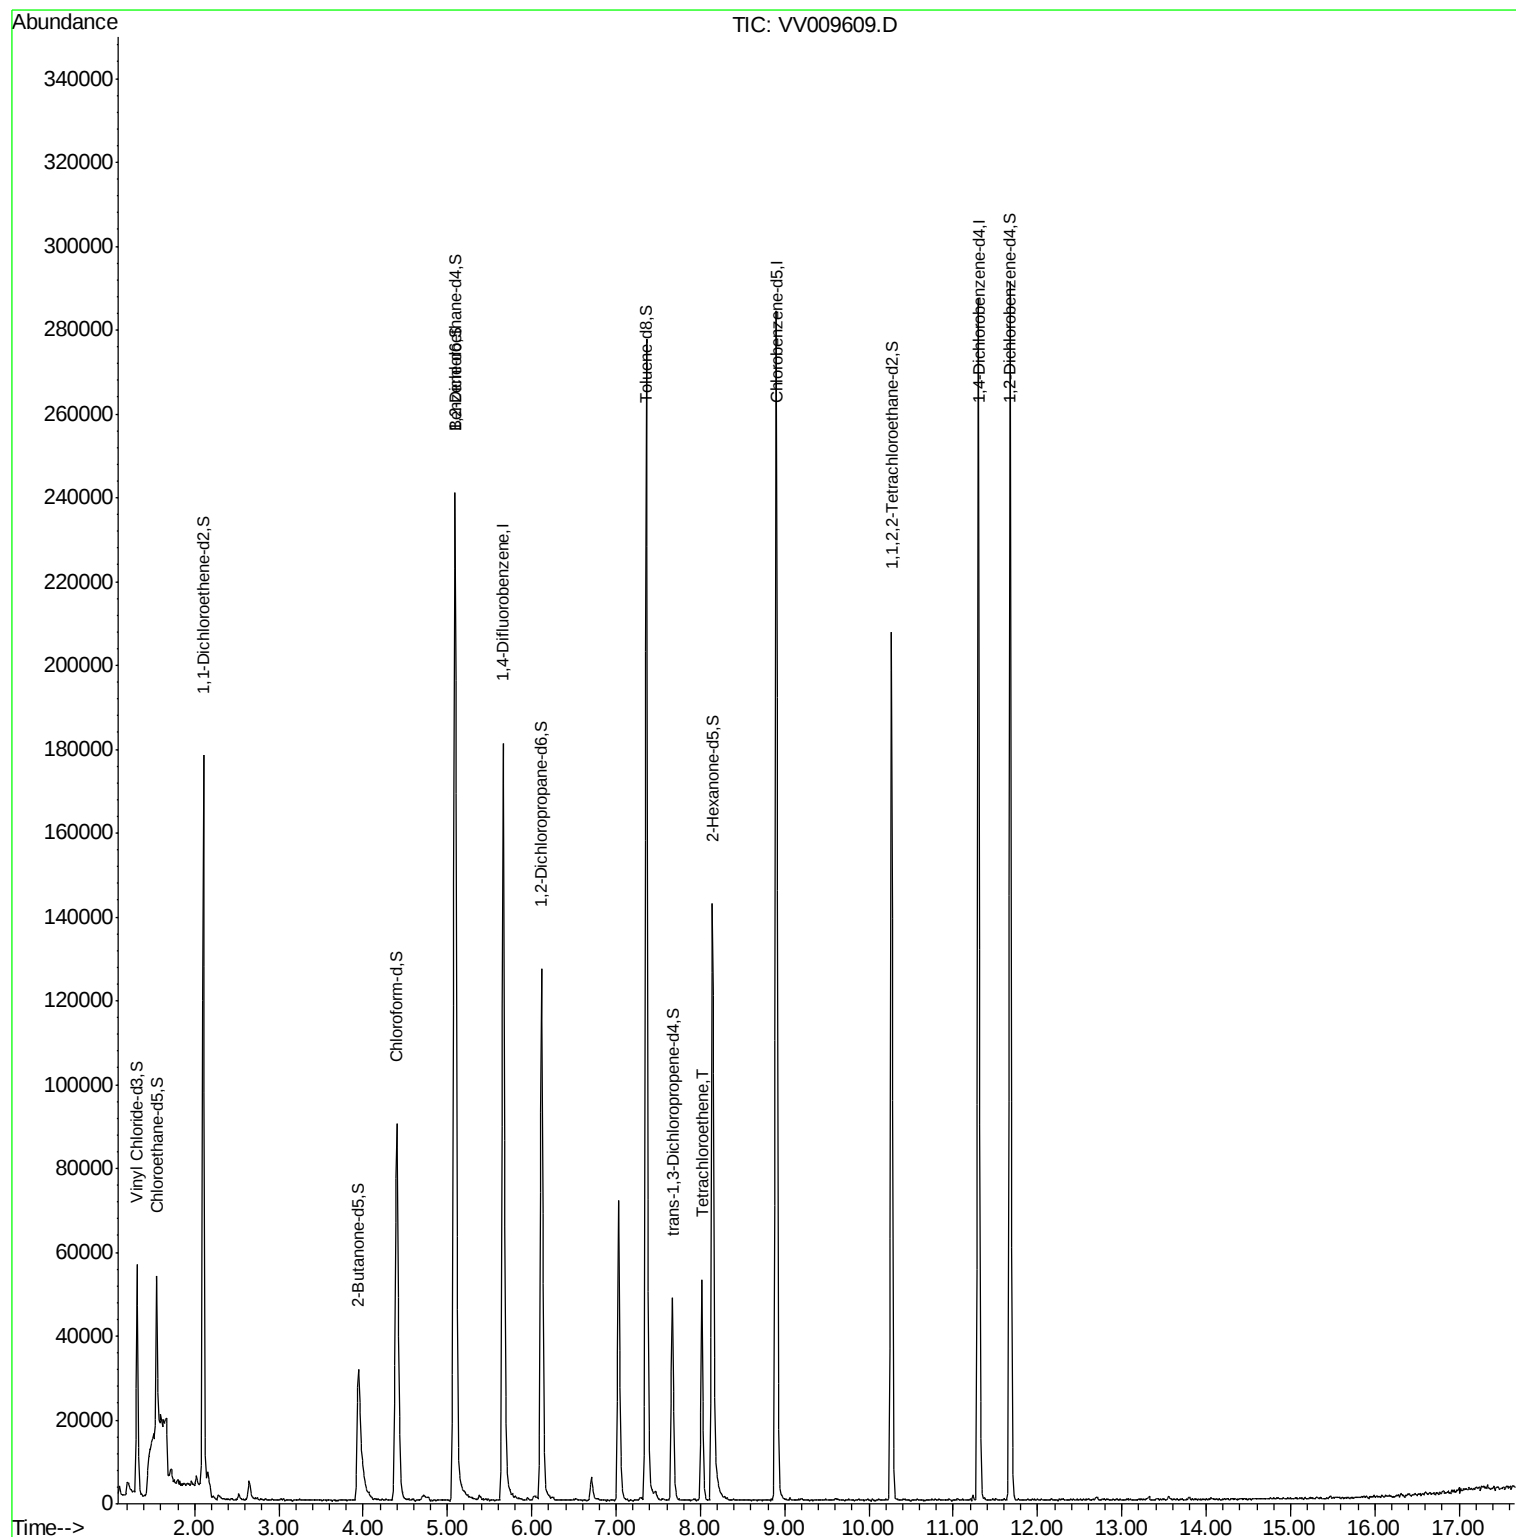

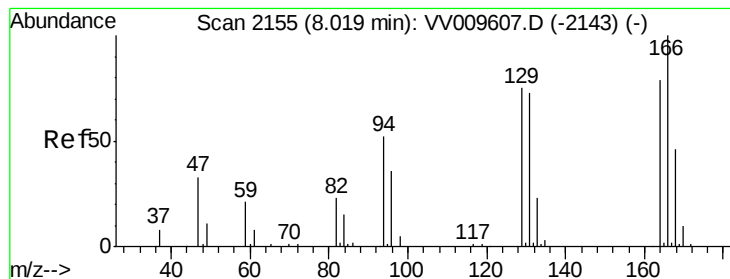

#46

Tetrachloroethene

Concen: 12.724 ug/L

RT: 8.02 min Scan# 2155

Delta R.T. 0.00 min

Lab File: VV009609.D

Acq: 12 Mar 2019 17:30

Instrument :

MSVOA_V

ClientSampleId :

BFON8ME

Tgt Ion:164 Resp: 10615


Ion Ratio Lower Upper

164 100

129 102.1 70.8 131.6

131 95.6 68.3 126.9

166 129.9 89.5 166.3

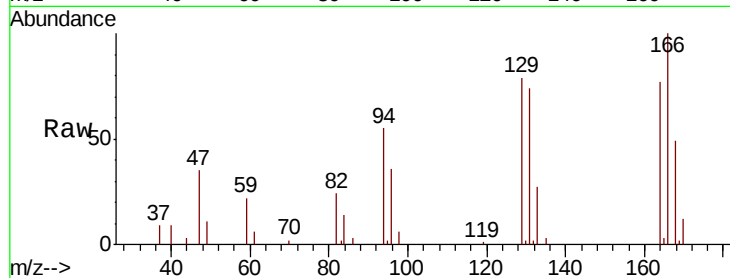

Abundance Ion 164.00 (163.70 to 164.70): V

Ion 129.00 (128.70 to 129.70): V

Ion 131.00 (130.70 to 131.70): V

Ion 166.00 (165.70 to 166.70): V

