

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031219\
 Data File : VV009628.D
 Acq On : 13 Mar 2019 00:59
 Operator : SY/MD
 Sample : K1838-03
 Misc : 5.47g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BF0S4

Quant Time: Mar 13 07:13:11 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031219WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 13 02:20:07 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	172011	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	176084	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	77787	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	40627	39.91	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	79.82%
7) Chloroethane-d5	1.55	69	24767	23.37	ug/L	-0.03
Spiked Amount	50.000	Range	70 - 130	Recovery	=	46.74%#
11) 1,1-Dichloroethene-d2	2.10	63	86823	32.33	ug/L	-0.03
Spiked Amount	50.000	Range	60 - 125	Recovery	=	64.66%
21) 2-Butanone-d5	3.95	46	68406	90.93	ug/L	0.02
Spiked Amount	100.000	Range	40 - 130	Recovery	=	90.93%
24) Chloroform-d	4.40	84	99658	44.81	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.62%
26) 1,2-Dichloroethane-d4	5.08	65	68509	46.56	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.12%
32) Benzene-d6	5.09	84	203442	44.43	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.86%
36) 1,2-Dichloropropane-d6	6.12	67	63397	46.31	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	92.62%
41) Toluene-d8	7.36	98	200107	44.86	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	89.72%
43) trans-1,3-Dichloropropene-	7.67	79	30924	43.73	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	87.46%
47) 2-Hexanone-d5	8.14	63	55872	93.31	ug/L	0.02
Spiked Amount	100.000	Range	45 - 130	Recovery	=	93.31%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	96588	43.92	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	87.84%
64) 1,2-Dichlorobenzene-d4	11.68	152	74879	45.63	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	91.26%


Target Compounds					Qvalue
46) Tetrachloroethene	8.02	164	145175	156.553 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV031219\
Data File : VV009628.D
Acq On : 13 Mar 2019 00:59
Operator : SY/MD
Sample : K1838-03
Misc : 5.47g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BF0S4

Quant Time: Mar 13 07:13:11 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031219WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Mar 13 02:20:07 2019
Response via : Initial Calibration

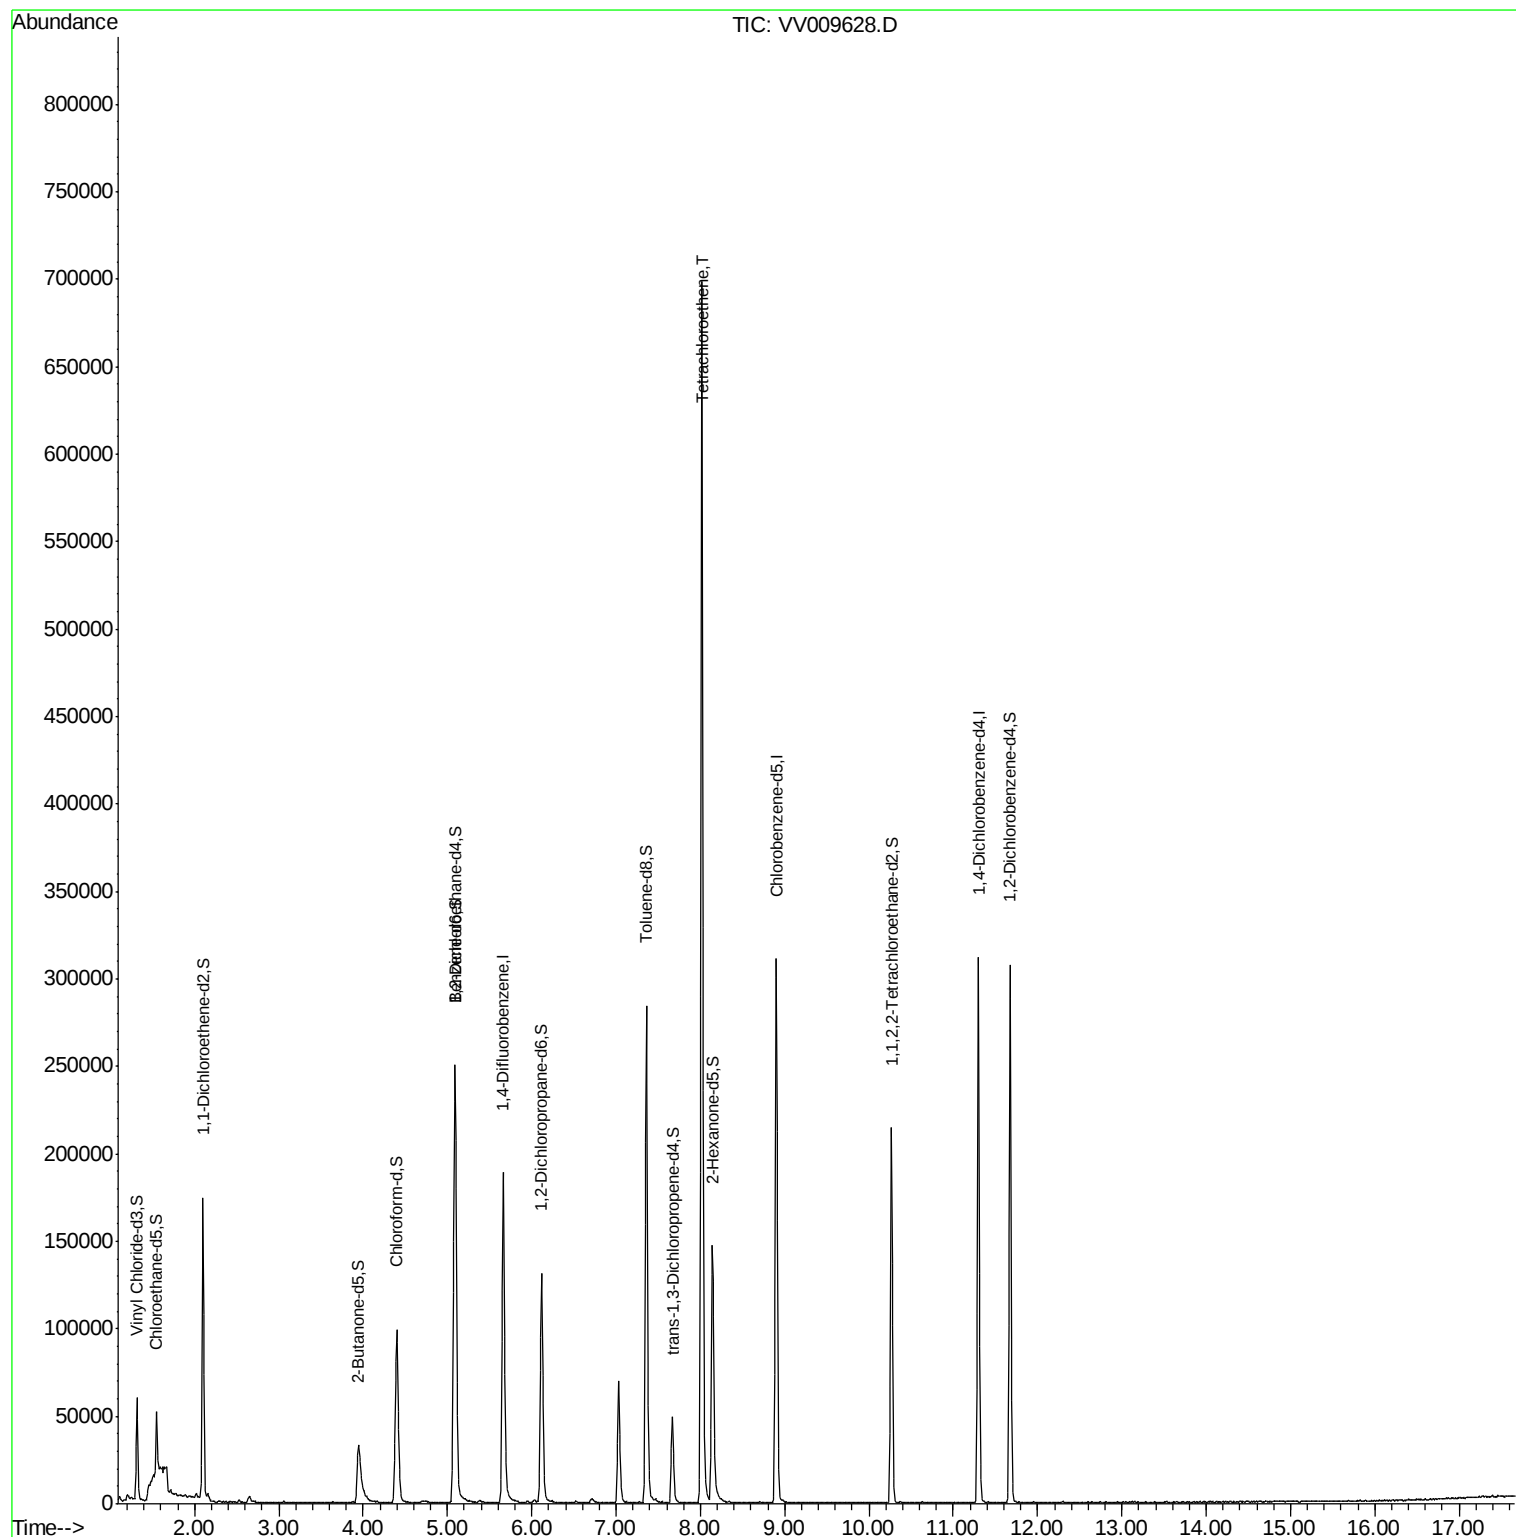

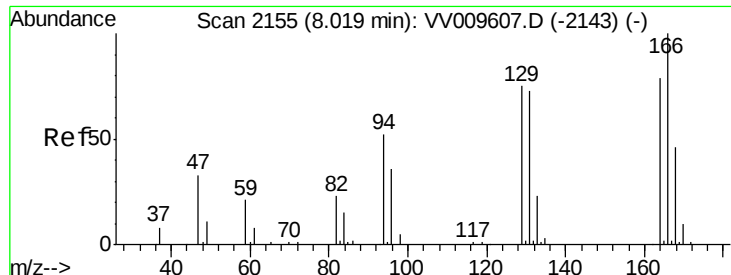

#46

Tetrachloroethene

Concen: 156.553 ug/L

RT: 8.02 min Scan# 2155

Delta R.T. 0.00 min

Lab File: VV009628.D


Acq: 13 Mar 2019 00:59

Instrument :

MSVOA_V

ClientSampleId :

BF0S4

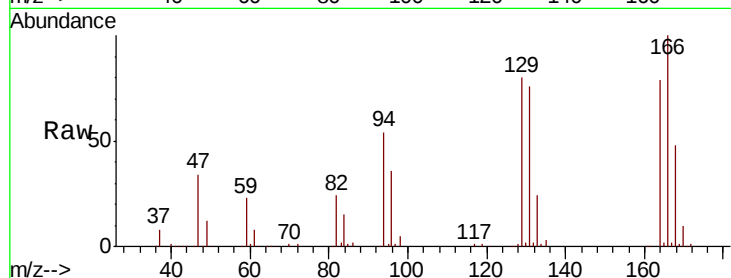

Tgt Ion:164 Resp: 145175

Ion Ratio Lower Upper

164 100

129 101.0 70.8 131.6

131 96.0 68.3 126.9

166 126.4 89.5 166.3

Abundance Ion 164.00 (163.70 to 164.70): V

Ion 129.00 (128.70 to 129.70): V

Ion 131.00 (130.70 to 131.70): V

Ion 166.00 (165.70 to 166.70): V

