


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031219\
 Data File : VV009600.D
 Acq On : 12 Mar 2019 10:11
 Operator : SY/MD
 Sample : BFB70
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB70

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031219WMA.M
 Title : VOC Analysis
 Last Update : Wed Mar 13 02:20:07 2019

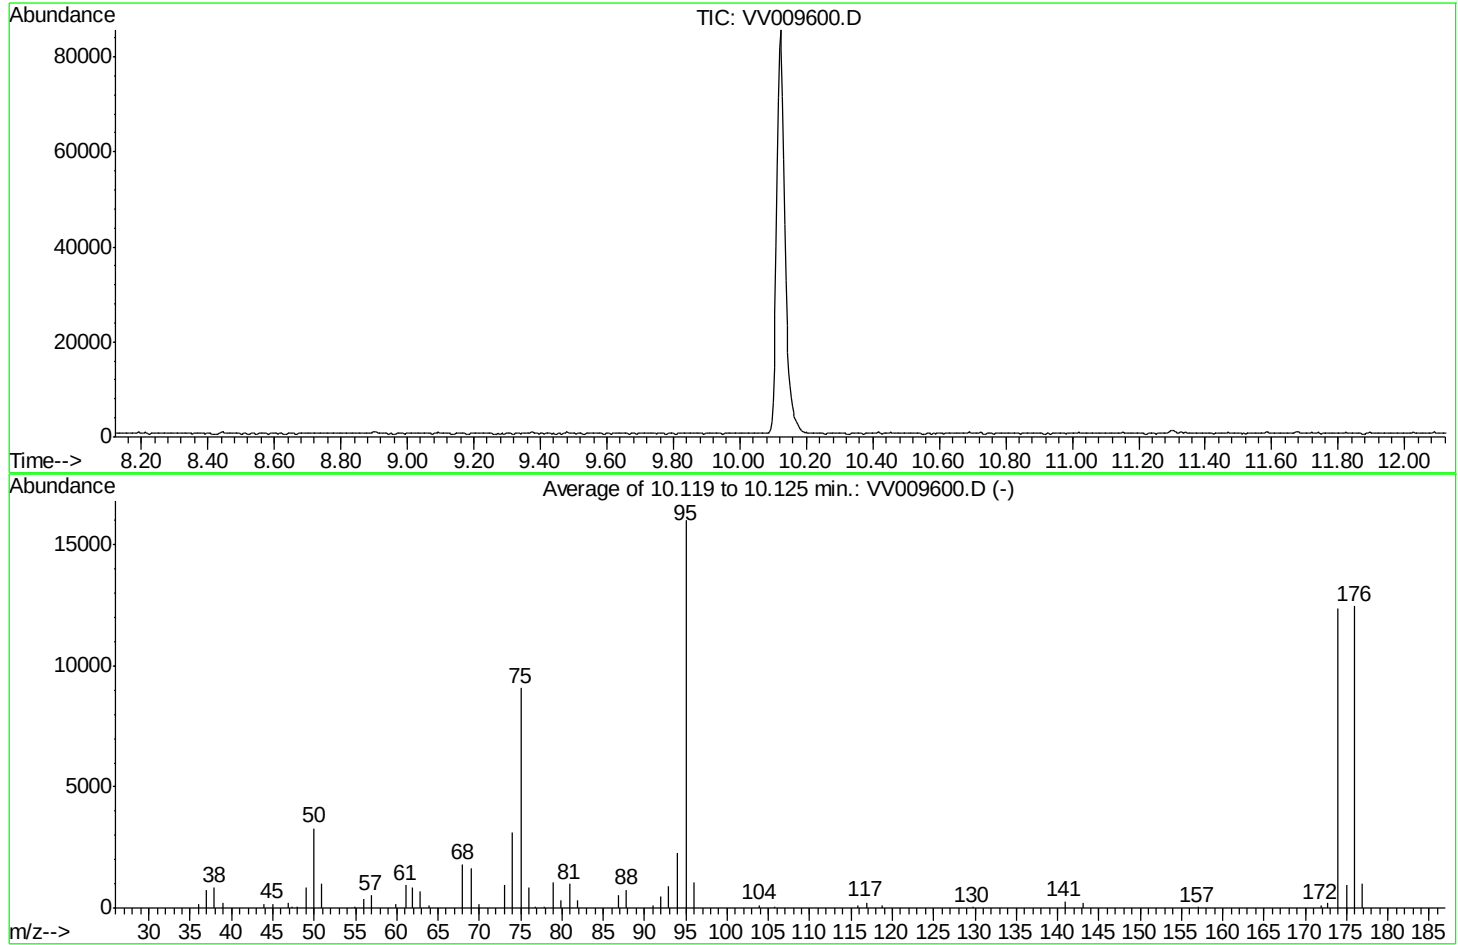

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.5	3291	PASS
75	95	30	80	56.8	9095	PASS
95	95	100	100	100.0	16015	PASS
96	95	5	9	6.6	1056	PASS
173	174	0.00	2	1.5	187	PASS
174	95	50	120	77.4	12402	PASS
175	174	5	9	7.6	937	PASS
176	174	95	101	100.6	12477	PASS
177	176	5	9	8.1	1009	PASS

m/z	Abundance
39.90	587.0
43.90	172.0

Instrument :
MSVOA_V
ClientSampleId :
BFB70

m/z	Abundance
36.00	170.0
37.00	698.0
37.90	843.0
39.00	154.0
39.90	537.0
43.80	336.0
45.10	197.0
46.80	235.0
49.00	799.0
50.00	3099.0
50.90	1046.0
54.90	103.0
56.00	345.0
56.90	595.0
59.90	145.0
61.00	982.0
61.90	857.0
62.80	687.0
63.90	124.0
68.00	1723.0
69.00	1744.0
69.90	205.0
73.00	973.0
74.00	3070.0
75.00	9379.0
76.00	919.0
76.70	162.0
78.90	1056.0
79.90	333.0
80.90	925.0
81.90	312.0
86.80	474.0
87.80	736.0
92.00	473.0
93.00	961.0
94.00	2191.0
95.00	15414.0
96.00	1168.0
103.90	101.0
105.80	108.0
116.80	211.0
118.80	113.0
140.90	237.0
143.10	234.0
171.90	125.0
172.90	166.0
174.00	12286.0
174.90	947.0
176.00	12123.0
177.00	1004.0

Instrument :
MSVOA_V
ClientSampleId :
BFB70

m/z	Abundance
35.90	143.0
36.90	764.0
37.90	871.0
39.00	227.0
39.90	571.0
43.80	303.0
44.90	182.0
46.80	224.0
48.00	102.0
49.00	892.0
50.00	3382.0
50.90	1044.0
54.90	105.0
56.00	387.0
56.90	531.0
59.80	149.0
61.10	996.0
62.00	874.0
62.90	702.0
63.90	140.0
68.00	1847.0
69.00	1667.0
69.90	172.0
73.00	1006.0
74.00	3137.0
75.00	9355.0
76.00	829.0
77.90	104.0
78.90	1089.0
79.90	332.0
80.90	1035.0
81.90	347.0
86.90	544.0
87.80	812.0
91.00	142.0
92.00	502.0
92.90	928.0
94.00	2349.0
95.00	16480.0
96.00	1074.0
104.00	136.0
115.90	121.0
116.90	252.0
118.70	131.0
129.70	101.0
140.80	255.0
143.10	220.0
157.00	102.0
171.90	126.0
172.70	180.0
174.00	12788.0
174.90	945.0
175.90	12933.0
176.90	1031.0

Instrument :
MSVOA_V
ClientSampleId :
BFB70

m/z	Abundance
35.90	125.0
36.90	753.0
37.90	768.0
39.00	281.0
39.90	610.0
43.90	311.0
44.90	174.0
46.90	216.0
47.40	100.0
49.00	875.0
50.00	3393.0
50.90	1004.0
56.00	373.0
56.90	425.0
60.00	161.0
61.10	850.0
62.00	870.0
62.90	670.0
63.90	122.0
68.00	1799.0
69.00	1503.0
69.90	154.0
73.00	841.0
74.00	3099.0
75.00	8553.0
76.00	737.0
77.90	108.0
78.90	1054.0
79.90	286.0
80.90	1031.0
81.90	337.0
87.00	582.0
87.80	729.0
90.90	169.0
92.00	520.0
92.90	830.0
94.00	2286.0
95.00	16151.0
96.00	927.0
103.90	160.0
115.80	149.0
116.90	219.0
118.70	129.0
140.80	269.0
143.10	192.0
171.90	112.0
172.70	215.0
173.90	12133.0
175.00	920.0
175.90	12377.0
176.90	993.0

Instrument :
MSVOA_V
ClientSampleId :
BFB70