

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031220\
 Data File : VV014869.D
 Acq On : 12 Mar 2020 15:40
 Operator : SY/MD
 Sample : L1835-01 50X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DK5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	83	rVB	182153	187302	13.23%	1.622%
2	1.579	144	152	171	rBV	131438	163385	11.54%	1.415%
3	2.119	310	320	331	rBV	278733	397443	28.06%	3.442%
4	2.688	494	497	499	rBV2	688	470	0.03%	0.004%
5	2.746	511	515	518	rBV4	800	493	0.03%	0.004%
6	2.888	557	559	562	rBV	592	360	0.03%	0.003%
7	2.933	571	573	578	rVB2	755	526	0.04%	0.005%
8	2.958	578	581	585	rBV3	652	586	0.04%	0.005%
9	3.032	600	604	605	rBV	392	306	0.02%	0.003%
10	3.077	614	618	620	rBV3	906	690	0.05%	0.006%
11	3.138	633	637	639	rBV4	884	609	0.04%	0.005%
12	3.190	652	653	656	rVB	614	281	0.02%	0.002%
13	3.203	656	657	659	rBV	329	144	0.01%	0.001%
14	3.216	659	661	662	rBV2	269	114	0.01%	0.001%
15	3.251	668	672	675	rBV3	582	518	0.04%	0.004%
16	3.283	680	682	684	rVB2	464	205	0.01%	0.002%
17	3.296	684	686	688	rBV	357	111	0.01%	0.001%
18	3.335	696	698	699	rBV	406	158	0.01%	0.001%
19	3.367	703	708	709	rBV	408	308	0.02%	0.003%
20	3.425	724	726	728	rBV	245	151	0.01%	0.001%
21	3.437	728	730	736	rVV2	502	457	0.03%	0.004%
22	3.505	748	751	754	rVB3	518	344	0.02%	0.003%
23	3.531	755	759	761	rBV2	471	290	0.02%	0.003%
24	3.556	766	767	769	rBV	235	98	0.01%	0.001%
25	3.566	769	770	772	rVB	246	71	0.01%	0.001%
26	3.605	780	782	784	rBV	462	194	0.01%	0.002%
27	3.646	792	795	798	rVB2	673	508	0.04%	0.004%
28	3.659	798	799	802	rBV3	268	162	0.01%	0.001%
29	3.682	802	806	812	rBV5	394	461	0.03%	0.004%
30	3.704	812	813	816	rBV	247	119	0.01%	0.001%
31	3.717	816	817	818	rBV	322	87	0.01%	0.001%
32	3.791	836	840	841	rBV2	470	298	0.02%	0.003%
33	3.868	862	864	867	rVB2	252	91	0.01%	0.001%
34	3.888	867	870	872	rBV	512	292	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031220\
 Data File : VV014869.D
 Acq On : 12 Mar 2020 15:40
 Operator : SY/MD
 Sample : L1835-01 50X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DK5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
 Title : VOC Analysis

35	3.929	872	883	909	rBV2	61727	240762	17.00%	2.085%
36	4.302	995	999	1004	rBV4	953	935	0.07%	0.008%
37	4.376	1004	1022	1046	rBV	233335	563537	39.79%	4.880%
38	4.563	1079	1080	1081	rBV	420	99	0.01%	0.001%
39	4.572	1081	1083	1084	rVV	641	218	0.02%	0.002%
40	4.589	1084	1088	1091	rVB3	731	544	0.04%	0.005%
41	4.614	1091	1096	1101	rBV4	775	1005	0.07%	0.009%
42	4.942	1193	1198	1199	rBV	678	437	0.03%	0.004%
43	4.971	1205	1207	1212	rVB3	528	414	0.03%	0.004%
44	4.997	1212	1215	1218	rBV2	374	225	0.02%	0.002%
45	5.016	1218	1221	1222	rBV2	421	260	0.02%	0.002%
46	5.074	1222	1239	1278	rVV2	559644	1416203	100.00%	12.263%
47	5.354	1323	1326	1329	rBV3	1002	844	0.06%	0.007%
48	5.370	1329	1331	1335	rVV3	852	607	0.04%	0.005%
49	5.643	1387	1416	1433	rBV	516689	1265064	89.33%	10.954%
50	6.097	1546	1557	1579	rVB	308812	623696	44.04%	5.401%
51	7.010	1830	1841	1858	rBV	177700	312758	22.08%	2.708%
52	7.338	1932	1943	1962	rBV	708070	1204645	85.06%	10.431%
53	7.643	2028	2038	2056	rBV	124460	210837	14.89%	1.826%
54	8.116	2174	2185	2215	rBV	362288	751596	53.07%	6.508%
55	8.875	2409	2421	2443	rBV	713342	1186190	83.76%	10.271%
56	9.344	2562	2567	2570	rBV2	979	809	0.06%	0.007%
57	9.903	2739	2741	2744	rBV2	736	428	0.03%	0.004%
58	9.948	2751	2755	2756	rBV4	724	496	0.04%	0.004%
59	10.238	2833	2845	2864	rBV	458759	716658	50.60%	6.206%
60	10.450	2908	2911	2912	rBV2	724	397	0.03%	0.003%
61	10.508	2924	2929	2931	rBV3	776	602	0.04%	0.005%
62	10.592	2953	2955	2956	rBV	465	237	0.02%	0.002%
63	10.665	2976	2978	2981	rBV2	661	433	0.03%	0.004%
64	10.801	3018	3020	3023	rBV2	792	440	0.03%	0.004%
65	10.878	3039	3044	3047	rBV3	885	792	0.06%	0.007%
66	10.897	3047	3050	3051	rBV2	628	295	0.02%	0.003%
67	11.202	3135	3145	3154	rBV5	3755	6538	0.46%	0.057%
68	11.270	3154	3166	3187	rBV	721633	1148128	81.07%	9.942%
69	11.540	3245	3250	3251	rBV3	869	729	0.05%	0.006%
70	11.553	3251	3254	3259	rVV5	1719	1667	0.12%	0.014%
71	11.646	3271	3283	3298	rBV	723587	1122914	79.29%	9.723%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031220\
 Data File : VV014869.D
 Acq On : 12 Mar 2020 15:40
 Operator : SY/MD
 Sample : L1835-01 50X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DK5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
 Title : VOC Analysis

72	12.038	3403	3405	3407	rVB2	600	194	0.01%	0.002%
73	12.055	3407	3410	3416	rBV5	650	762	0.05%	0.007%
74	12.170	3445	3446	3450	rBV	480	279	0.02%	0.002%
75	12.222	3460	3462	3464	rBV3	624	295	0.02%	0.003%
76	12.302	3485	3487	3490	rBV2	883	616	0.04%	0.005%
77	12.331	3494	3496	3499	rVV3	819	442	0.03%	0.004%
78	12.389	3513	3514	3516	rVB2	391	115	0.01%	0.001%
79	12.411	3519	3521	3522	rBV2	506	250	0.02%	0.002%
80	12.521	3550	3555	3556	rBV3	836	620	0.04%	0.005%
81	12.579	3571	3573	3575	rBV2	731	370	0.03%	0.003%
82	12.977	3694	3697	3699	rBV3	914	646	0.05%	0.006%
83	13.071	3724	3726	3729	rBV2	486	261	0.02%	0.002%
84	13.199	3758	3766	3770	rBV4	853	1330	0.09%	0.012%
85	13.505	3858	3861	3863	rBV3	891	594	0.04%	0.005%
86	13.653	3904	3907	3910	rBV3	747	534	0.04%	0.005%
87	13.797	3949	3952	3954	rBV3	1022	564	0.04%	0.005%
88	14.418	4142	4145	4147	rBV3	923	515	0.04%	0.004%


Sum of corrected areas: 11548458

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV031220\
Data File : VV014869.D
Acq On : 12 Mar 2020 15:40
Operator : SY/MD
Sample : L1835-01 50X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DK5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

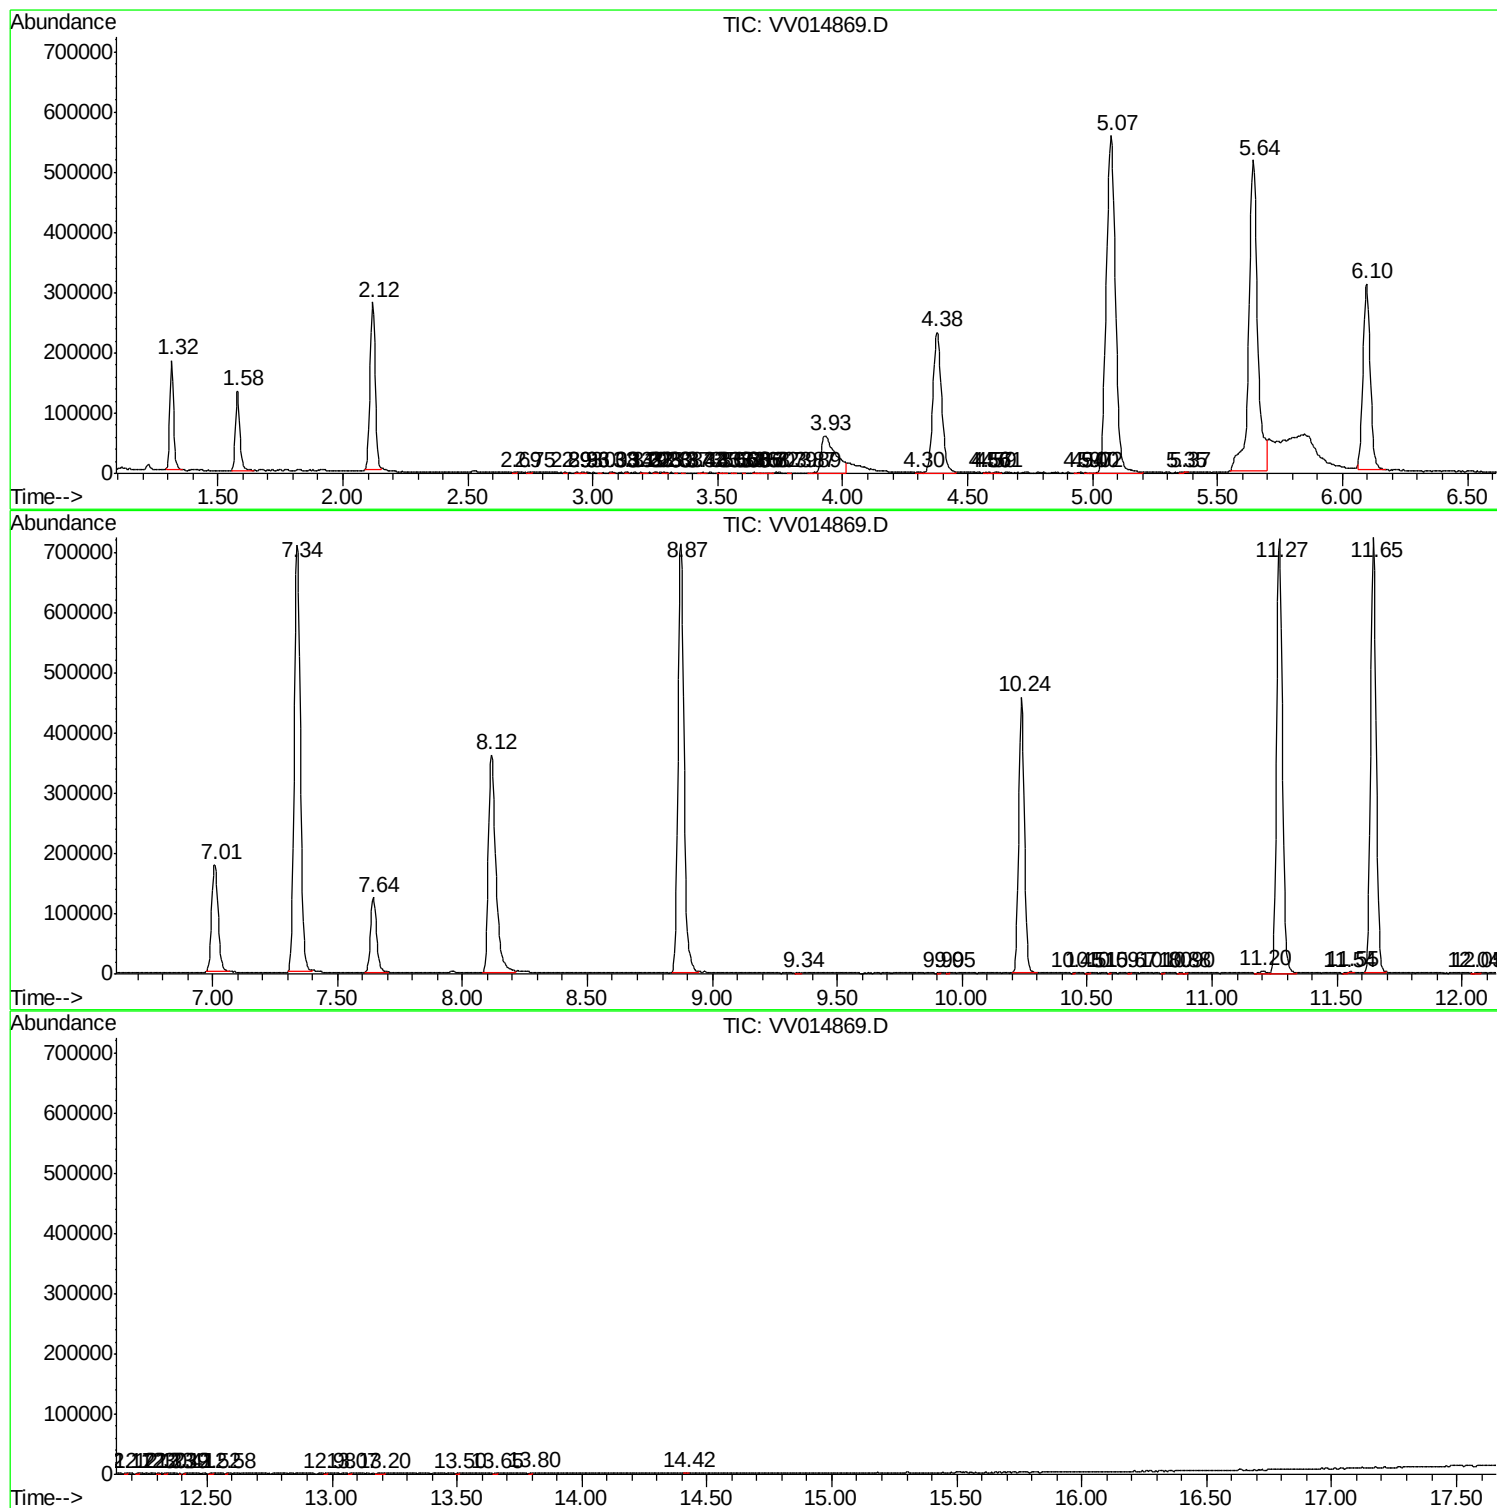

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV031220\
Data File : VV014869.D
Acq On : 12 Mar 2020 15:40
Operator : SY/MD
Sample : L1835-01 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DK5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV031220\
Data File : VV014869.D
Acq On : 12 Mar 2020 15:40
Operator : SY/MD
Sample : L1835-01 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DK5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc