

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031220\
 Data File : VV014871.D
 Acq On : 12 Mar 2020 16:37
 Operator : SY/MD
 Sample : VV0312WBL02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK83

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	63	69	84	rVB	182121	192718	13.66%	1.702%
2	1.576	144	151	163	rBV	134768	163590	11.60%	1.445%
3	2.119	310	320	334	rVB	277324	399607	28.33%	3.530%
4	2.463	423	427	430	rBV2	1166	1045	0.07%	0.009%
5	2.765	519	521	522	rBV2	1028	401	0.03%	0.004%
6	2.884	556	558	562	rBV2	479	338	0.02%	0.003%
7	2.926	567	571	574	rBV3	528	390	0.03%	0.003%
8	2.949	574	578	582	rVB5	555	423	0.03%	0.004%
9	2.978	585	587	591	rBV3	717	350	0.02%	0.003%
10	2.997	591	593	594	rBV2	912	392	0.03%	0.003%
11	3.045	605	608	610	rBV2	761	455	0.03%	0.004%
12	3.122	631	632	635	rBV2	561	295	0.02%	0.003%
13	3.180	648	650	652	rVB	590	215	0.02%	0.002%
14	3.193	652	654	656	rBV	701	281	0.02%	0.002%
15	3.261	673	675	679	rVB3	409	245	0.02%	0.002%
16	3.286	679	683	684	rBV	452	264	0.02%	0.002%
17	3.309	688	690	693	rVB	477	239	0.02%	0.002%
18	3.412	720	722	723	rBV	600	270	0.02%	0.002%
19	3.515	750	754	758	rVB2	434	330	0.02%	0.003%
20	3.547	761	764	765	rBV2	512	221	0.02%	0.002%
21	3.589	775	777	779	rBV2	587	341	0.02%	0.003%
22	3.624	783	788	790	rBV	323	287	0.02%	0.003%
23	3.637	790	792	796	rVB	632	336	0.02%	0.003%
24	3.662	796	800	801	rBV2	671	418	0.03%	0.004%
25	3.717	815	817	819	rBV	582	217	0.02%	0.002%
26	3.765	828	832	838	rVB4	512	452	0.03%	0.004%
27	3.791	838	840	842	rBV2	544	232	0.02%	0.002%
28	3.929	871	883	904	rBV	56065	207438	14.70%	1.832%
29	4.373	1007	1021	1041	rBV2	224062	543522	38.53%	4.801%
30	4.582	1082	1086	1087	rBV3	915	573	0.04%	0.005%
31	4.627	1096	1100	1101	rBV3	392	279	0.02%	0.002%
32	4.730	1128	1132	1135	rVB2	437	386	0.03%	0.003%
33	4.749	1135	1138	1140	rVB	635	327	0.02%	0.003%
34	4.833	1160	1164	1166	rVB4	379	219	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031220\
 Data File : VV014871.D
 Acq On : 12 Mar 2020 16:37
 Operator : SY/MD
 Sample : VV0312WBL02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK83

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
 Title : VOC Analysis

35	4.891	1180	1182	1186	rVB3	489	226	0.02%	0.002%
36	5.071	1220	1238	1263	rBV2	563780	1410772	100.00%	12.461%
37	5.392	1336	1338	1344	rBV4	432	324	0.02%	0.003%
38	5.640	1395	1415	1433	rBV	499787	1062528	75.32%	9.385%
39	6.093	1545	1556	1587	rVB	311563	637610	45.20%	5.632%
40	7.006	1829	1840	1866	rBV	180942	322271	22.84%	2.847%
41	7.251	1914	1916	1919	rBV2	1299	961	0.07%	0.008%
42	7.338	1931	1943	1962	rBV	704912	1218152	86.35%	10.760%
43	7.643	2026	2038	2057	rBV	126563	221320	15.69%	1.955%
44	8.116	2173	2185	2219	rBV	340019	728661	51.65%	6.436%
45	8.698	2364	2366	2369	rBV4	622	289	0.02%	0.003%
46	8.871	2408	2420	2440	rBV	711446	1162645	82.41%	10.270%
47	9.199	2519	2522	2524	rBV2	697	368	0.03%	0.003%
48	9.254	2537	2539	2541	rVB	498	235	0.02%	0.002%
49	9.453	2597	2601	2604	rBV3	648	483	0.03%	0.004%
50	9.566	2630	2636	2637	rBV4	1691	1733	0.12%	0.015%
51	9.698	2675	2677	2681	rBV2	628	411	0.03%	0.004%
52	9.855	2722	2726	2731	rVB4	729	754	0.05%	0.007%
53	9.887	2733	2736	2738	rBV2	797	405	0.03%	0.004%
54	9.948	2748	2755	2757	rBV5	1518	1475	0.10%	0.013%
55	9.997	2768	2770	2777	rBV4	600	568	0.04%	0.005%
56	10.096	2798	2801	2806	rVB2	761	604	0.04%	0.005%
57	10.238	2829	2845	2863	rBV	445406	711334	50.42%	6.283%
58	10.402	2893	2896	2898	rBV2	694	381	0.03%	0.003%
59	10.447	2907	2910	2912	rBV2	557	368	0.03%	0.003%
60	10.489	2921	2923	2927	rBV2	663	454	0.03%	0.004%
61	10.556	2940	2944	2952	rVB7	1823	2181	0.15%	0.019%
62	10.620	2962	2964	2967	rBV	393	284	0.02%	0.003%
63	10.688	2982	2985	2988	rVB3	954	704	0.05%	0.006%
64	10.714	2988	2993	2994	rBV2	716	515	0.04%	0.005%
65	10.791	3014	3017	3018	rBV3	395	246	0.02%	0.002%
66	10.800	3018	3020	3026	rVB2	412	300	0.02%	0.003%
67	10.871	3039	3042	3043	rBV2	638	394	0.03%	0.003%
68	10.916	3052	3056	3057	rBV	910	615	0.04%	0.005%
69	11.045	3094	3096	3098	rBV2	669	369	0.03%	0.003%
70	11.074	3103	3105	3108	rBV	354	227	0.02%	0.002%
71	11.132	3119	3123	3125	rBV3	655	462	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031220\
 Data File : VV014871.D
 Acq On : 12 Mar 2020 16:37
 Operator : SY/MD
 Sample : VV0312WBL02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK83

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
 Title : VOC Analysis

72	11.196	3140	3143	3144	rBV2	1566	994	0.07%	0.009%
73	11.267	3154	3165	3183	rBV	742048	1145735	81.21%	10.120%
74	11.431	3212	3216	3222	rVB4	601	531	0.04%	0.005%
75	11.460	3222	3225	3227	rBV	564	374	0.03%	0.003%
76	11.534	3246	3248	3251	rBV	532	281	0.02%	0.002%
77	11.556	3251	3255	3257	rBV2	624	493	0.03%	0.004%
78	11.646	3271	3283	3302	rBV	725598	1127807	79.94%	9.962%
79	11.849	3344	3346	3352	rVB3	899	761	0.05%	0.007%
80	11.878	3352	3355	3360	rBV5	911	944	0.07%	0.008%
81	12.231	3462	3465	3467	rBV	414	214	0.02%	0.002%
82	12.395	3514	3516	3518	rBV3	580	358	0.03%	0.003%
83	12.460	3533	3536	3541	rBV3	713	582	0.04%	0.005%
84	12.530	3556	3558	3560	rBV3	600	336	0.02%	0.003%
85	12.617	3583	3585	3589	rVV2	671	483	0.03%	0.004%
86	12.672	3597	3602	3610	rVB7	3853	4720	0.33%	0.042%
87	12.890	3667	3670	3672	rVB4	820	410	0.03%	0.004%
88	12.974	3694	3696	3698	rBV	497	218	0.02%	0.002%
89	13.067	3722	3725	3726	rBV4	523	298	0.02%	0.003%
90	13.138	3745	3747	3750	rBV2	456	346	0.02%	0.003%
91	13.212	3765	3770	3772	rBV3	885	846	0.06%	0.007%
92	13.283	3784	3792	3801	rBV7	5513	8436	0.60%	0.075%
93	13.408	3828	3831	3834	rBV3	573	511	0.04%	0.005%
94	13.524	3864	3867	3879	rVB3	4661	6272	0.44%	0.055%
95	13.601	3889	3891	3893	rBV3	564	299	0.02%	0.003%
96	13.771	3936	3944	3953	rVB7	5394	8349	0.59%	0.074%
97	14.029	4021	4024	4027	rBV2	880	554	0.04%	0.005%
98	14.170	4066	4068	4069	rBV2	637	261	0.02%	0.002%
99	14.215	4079	4082	4083	rBV3	784	416	0.03%	0.004%
100	14.398	4136	4139	4141	rBV	1004	676	0.05%	0.006%


Sum of corrected areas: 11321230

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV031220\
Data File : VV014871.D
Acq On : 12 Mar 2020 16:37
Operator : SY/MD
Sample : VV0312WBL02
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK83

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

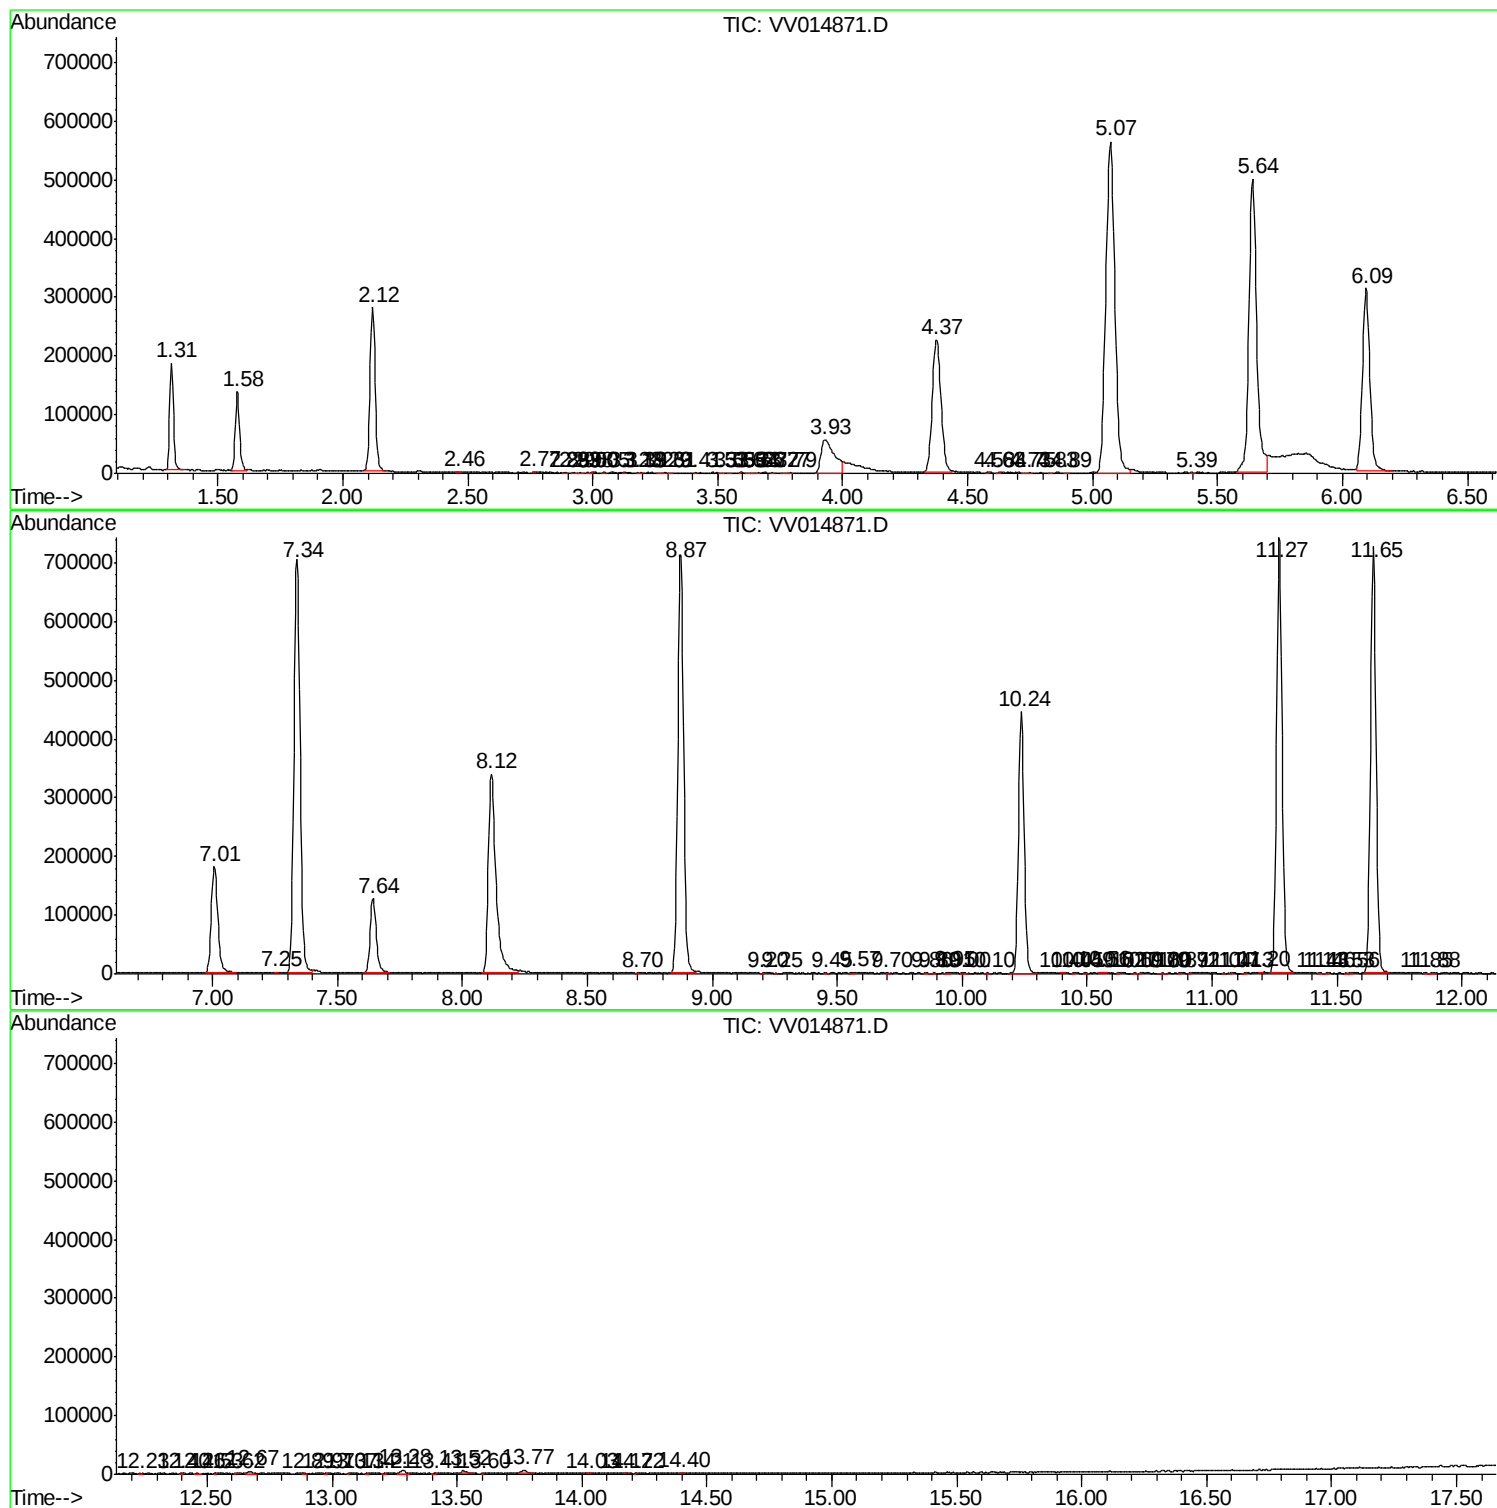

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV031220\
Data File : VV014871.D
Acq On : 12 Mar 2020 16:37
Operator : SY/MD
Sample : VV0312WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK83

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031220\
Data File : VV014871.D
Acq On : 12 Mar 2020 16:37
Operator : SY/MD
Sample : VV0312WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK83

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc