

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031220\
 Data File : VV014872.D
 Acq On : 12 Mar 2020 17:01
 Operator : SY/MD
 Sample : L1884-10
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0N75

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	86	rVB	163602	177845	13.20%	1.673%
2	1.579	145	152	167	rVB	118102	146502	10.87%	1.378%
3	2.119	311	320	333	rBV	263827	373796	27.74%	3.517%
4	2.936	570	574	575	rBV3	655	454	0.03%	0.004%
5	2.965	582	583	585	rBV	281	128	0.01%	0.001%
6	2.974	585	586	589	rVB	578	203	0.02%	0.002%
7	2.994	589	592	595	rBV3	732	375	0.03%	0.004%
8	3.058	611	612	616	rBV3	523	322	0.02%	0.003%
9	3.087	619	621	625	rBV2	413	277	0.02%	0.003%
10	3.129	630	634	639	rVB3	606	605	0.04%	0.006%
11	3.155	639	642	648	rBV3	814	740	0.05%	0.007%
12	3.183	648	651	655	rVB2	358	284	0.02%	0.003%
13	3.216	658	661	663	rBV3	546	274	0.02%	0.003%
14	3.254	669	673	675	rBV2	458	227	0.02%	0.002%
15	3.267	675	677	680	rBV2	466	259	0.02%	0.002%
16	3.347	700	702	704	rVB2	442	208	0.02%	0.002%
17	3.367	706	708	709	rVB	236	62	0.00%	0.001%
18	3.376	709	711	712	rBV	372	94	0.01%	0.001%
19	3.450	732	734	738	rVB	593	403	0.03%	0.004%
20	3.470	738	740	741	rBV	158	61	0.00%	0.001%
21	3.489	741	746	750	rVV4	697	746	0.06%	0.007%
22	3.518	750	755	758	rVB3	589	388	0.03%	0.004%
23	3.547	761	764	767	rVB3	609	308	0.02%	0.003%
24	3.569	767	771	774	rBV3	430	317	0.02%	0.003%
25	3.585	774	776	781	rVB5	544	410	0.03%	0.004%
26	3.608	781	783	784	rBV	393	111	0.01%	0.001%
27	3.618	784	786	788	rBV	350	169	0.01%	0.002%
28	3.714	812	816	819	rBV2	319	273	0.02%	0.003%
29	3.733	819	822	825	rBV2	243	159	0.01%	0.001%
30	3.756	825	829	830	rBV3	746	467	0.03%	0.004%
31	3.798	838	842	844	rBV	425	259	0.02%	0.002%
32	3.820	847	849	850	rBV	249	134	0.01%	0.001%
33	3.868	861	864	866	rVB2	432	217	0.02%	0.002%
34	3.888	866	870	871	rBV2	624	406	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031220\
 Data File : VV014872.D
 Acq On : 12 Mar 2020 17:01
 Operator : SY/MD
 Sample : L1884-10
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0N75

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
 Title : VOC Analysis

35	3.936	872	885	928	rBV2	55671	276796	20.54%	2.604%
36	4.380	1007	1023	1043	rBV	217999	532420	39.51%	5.009%
37	4.730	1129	1132	1134	rBV3	401	233	0.02%	0.002%
38	4.788	1147	1150	1155	rBV2	592	416	0.03%	0.004%
39	4.810	1155	1157	1161	rVB2	496	312	0.02%	0.003%
40	4.830	1161	1163	1165	rBV	439	282	0.02%	0.003%
41	4.862	1171	1173	1174	rBV	465	124	0.01%	0.001%
42	4.907	1185	1187	1190	rVB2	603	337	0.03%	0.003%
43	4.920	1190	1191	1193	rBV2	285	143	0.01%	0.001%
44	4.952	1197	1201	1203	rBV3	615	489	0.04%	0.005%
45	4.965	1203	1205	1206	rVB	375	93	0.01%	0.001%
46	4.974	1206	1208	1210	rBV	365	210	0.02%	0.002%
47	5.003	1214	1217	1219	rBV3	556	345	0.03%	0.003%
48	5.074	1220	1239	1260	rBV2	538745	1347655	100.00%	12.680%
49	5.325	1315	1317	1319	rBV2	363	179	0.01%	0.002%
50	5.341	1319	1322	1325	rBV3	602	520	0.04%	0.005%
51	5.392	1336	1338	1342	rVB2	845	457	0.03%	0.004%
52	5.425	1345	1348	1349	rBV2	759	395	0.03%	0.004%
53	5.531	1380	1381	1383	rVB	426	85	0.01%	0.001%
54	5.550	1383	1387	1388	rBV2	644	495	0.04%	0.005%
55	5.643	1401	1416	1439	rBV	459848	1008200	74.81%	9.486%
56	6.097	1545	1557	1579	rVB	297282	595042	44.15%	5.599%
57	7.010	1830	1841	1860	rBV2	158843	281322	20.87%	2.647%
58	7.338	1931	1943	1969	rBV	664335	1151375	85.44%	10.833%
59	7.643	2027	2038	2057	rBV	110961	190341	14.12%	1.791%
60	7.830	2091	2096	2100	rBV5	1083	1121	0.08%	0.011%
61	7.926	2124	2126	2128	rBV2	701	369	0.03%	0.003%
62	8.119	2174	2186	2210	rBV	334431	682601	50.65%	6.422%
63	8.473	2294	2296	2298	rBV2	484	196	0.01%	0.002%
64	8.566	2323	2325	2328	rBV3	769	503	0.04%	0.005%
65	8.875	2409	2421	2438	rBV	668833	1073735	79.67%	10.102%
66	9.106	2491	2493	2495	rBV	621	310	0.02%	0.003%
67	9.254	2537	2539	2544	rBV3	640	409	0.03%	0.004%
68	9.370	2574	2575	2579	rBV2	698	536	0.04%	0.005%
69	9.514	2618	2620	2621	rBV2	321	175	0.01%	0.002%
70	9.929	2745	2749	2752	rBV4	1023	868	0.06%	0.008%
71	10.100	2798	2802	2804	rBV2	673	527	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031220\
 Data File : VV014872.D
 Acq On : 12 Mar 2020 17:01
 Operator : SY/MD
 Sample : L1884-10
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CON75

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
 Title : VOC Analysis

72	10.129	2809	2811	2814	rBV	312	178	0.01%	0.002%
73	10.157	2814	2820	2822	rBV2	769	711	0.05%	0.007%
74	10.238	2833	2845	2859	rBV	426229	674973	50.08%	6.351%
75	10.399	2889	2895	2899	rBV4	2364	2738	0.20%	0.026%
76	10.608	2957	2960	2963	rBV4	506	455	0.03%	0.004%
77	10.720	2993	2995	2998	rBV3	673	457	0.03%	0.004%
78	10.756	3004	3006	3009	rBV	464	259	0.02%	0.002%
79	10.900	3049	3051	3052	rBV	506	139	0.01%	0.001%
80	11.055	3095	3099	3102	rBV3	556	462	0.03%	0.004%
81	11.116	3113	3118	3119	rBV2	602	458	0.03%	0.004%
82	11.270	3154	3166	3181	rBV	676577	1035113	76.81%	9.739%
83	11.437	3216	3218	3222	rVB3	914	635	0.05%	0.006%
84	11.511	3237	3241	3242	rBV2	555	261	0.02%	0.002%
85	11.646	3270	3283	3301	rBV	676949	1050905	77.98%	9.888%
86	11.923	3367	3369	3373	rBV4	570	436	0.03%	0.004%
87	12.215	3457	3460	3461	rBV2	496	236	0.02%	0.002%
88	12.238	3465	3467	3469	rBV	422	146	0.01%	0.001%
89	12.447	3530	3532	3535	rBV3	777	494	0.04%	0.005%
90	12.588	3573	3576	3578	rBV	568	361	0.03%	0.003%
91	13.186	3760	3762	3766	rVB	444	236	0.02%	0.002%
92	13.222	3770	3773	3775	rBV3	790	430	0.03%	0.004%
93	13.427	3834	3837	3838	rBV2	923	421	0.03%	0.004%
94	13.492	3854	3857	3862	rBV6	1046	809	0.06%	0.008%


Sum of corrected areas: 10628412

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV031220\
Data File : VV014872.D
Acq On : 12 Mar 2020 17:01
Operator : SY/MD
Sample : L1884-10
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CON75

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

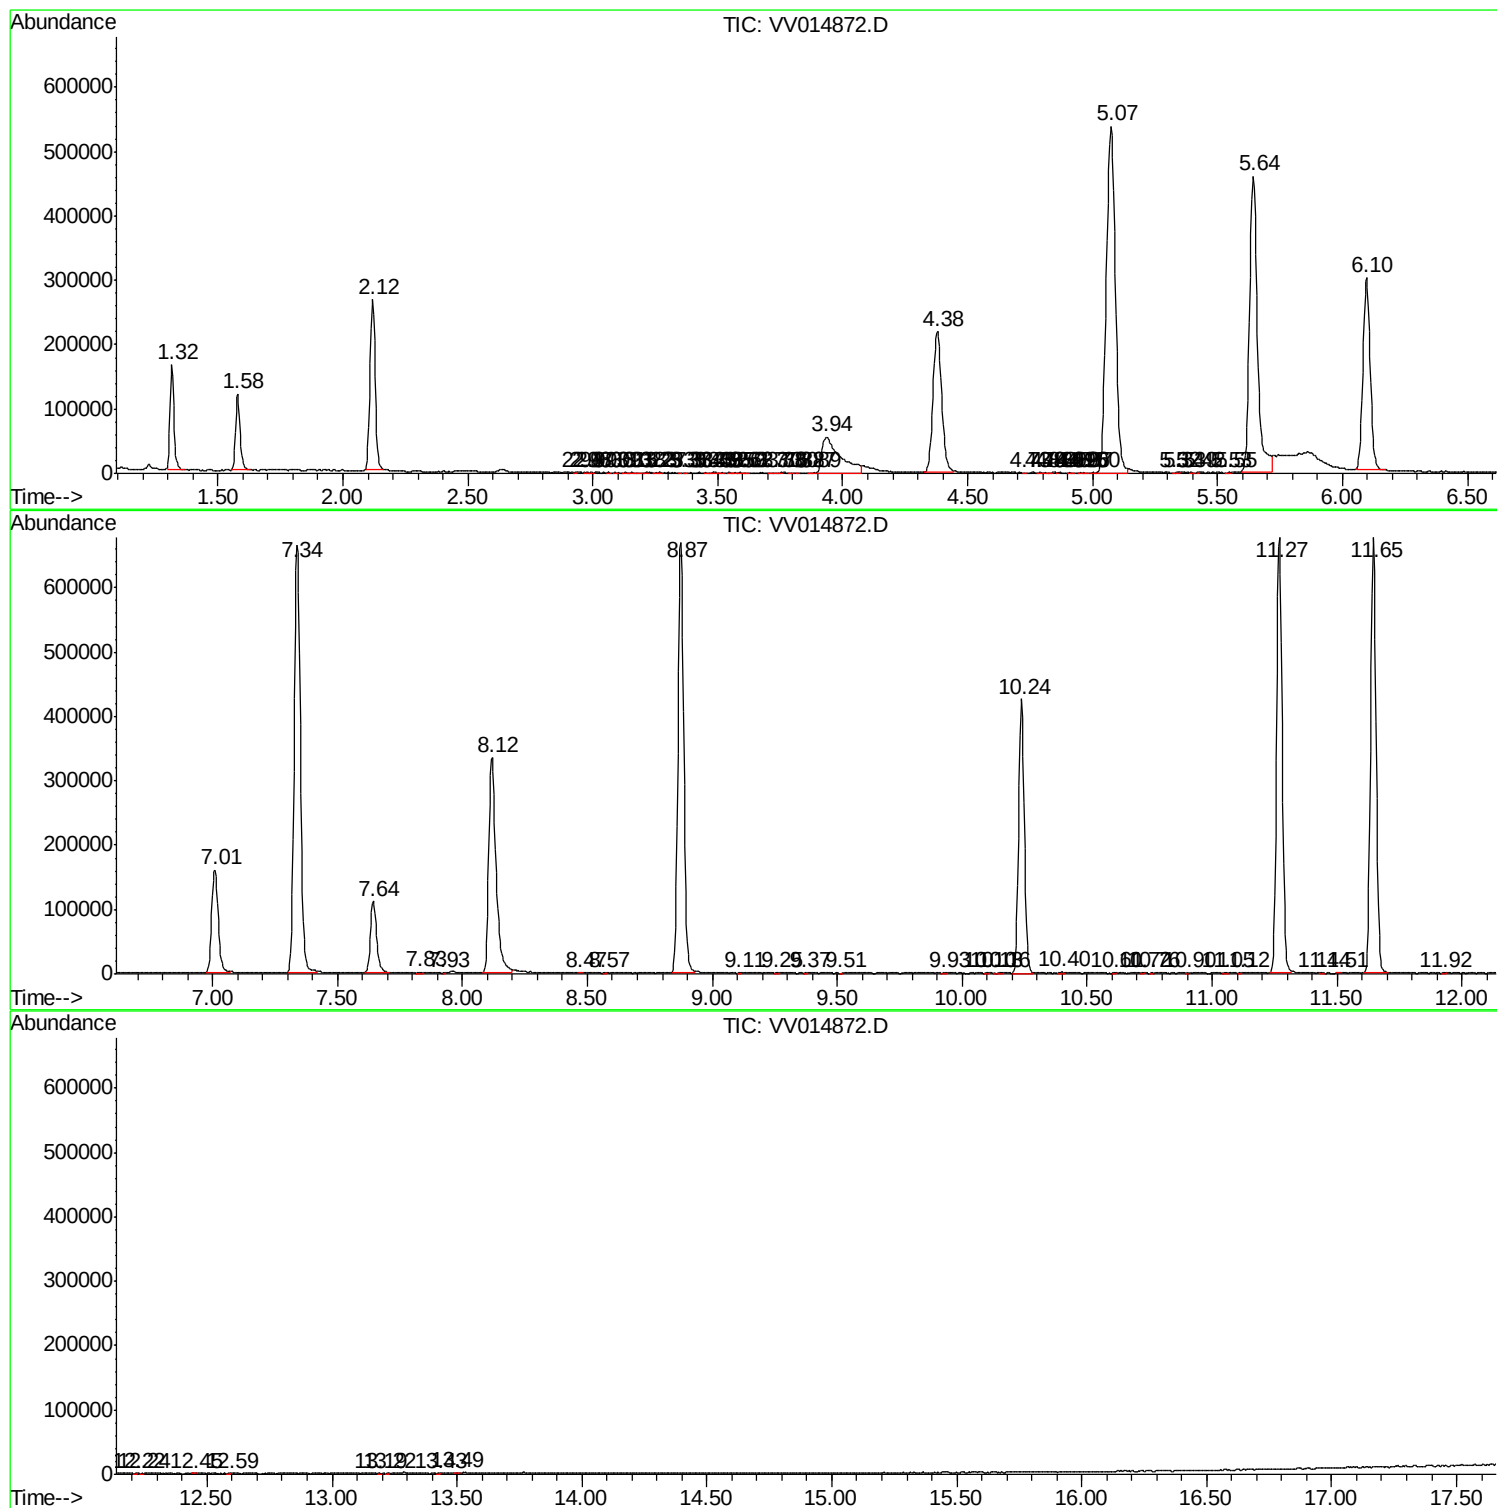

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV031220\
Data File : VV014872.D
Acq On : 12 Mar 2020 17:01
Operator : SY/MD
Sample : L1884-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CON75

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031220\
Data File : VV014872.D
Acq On : 12 Mar 2020 17:01
Operator : SY/MD
Sample : L1884-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0N75

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc