


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV031220\
 Data File : VV014859.D
 Acq On : 12 Mar 2020 11:24
 Operator : SY/MD
 Sample : BFB62
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB62

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
 Title : VOC Analysis
 Last Update : Fri Mar 13 04:10:22 2020

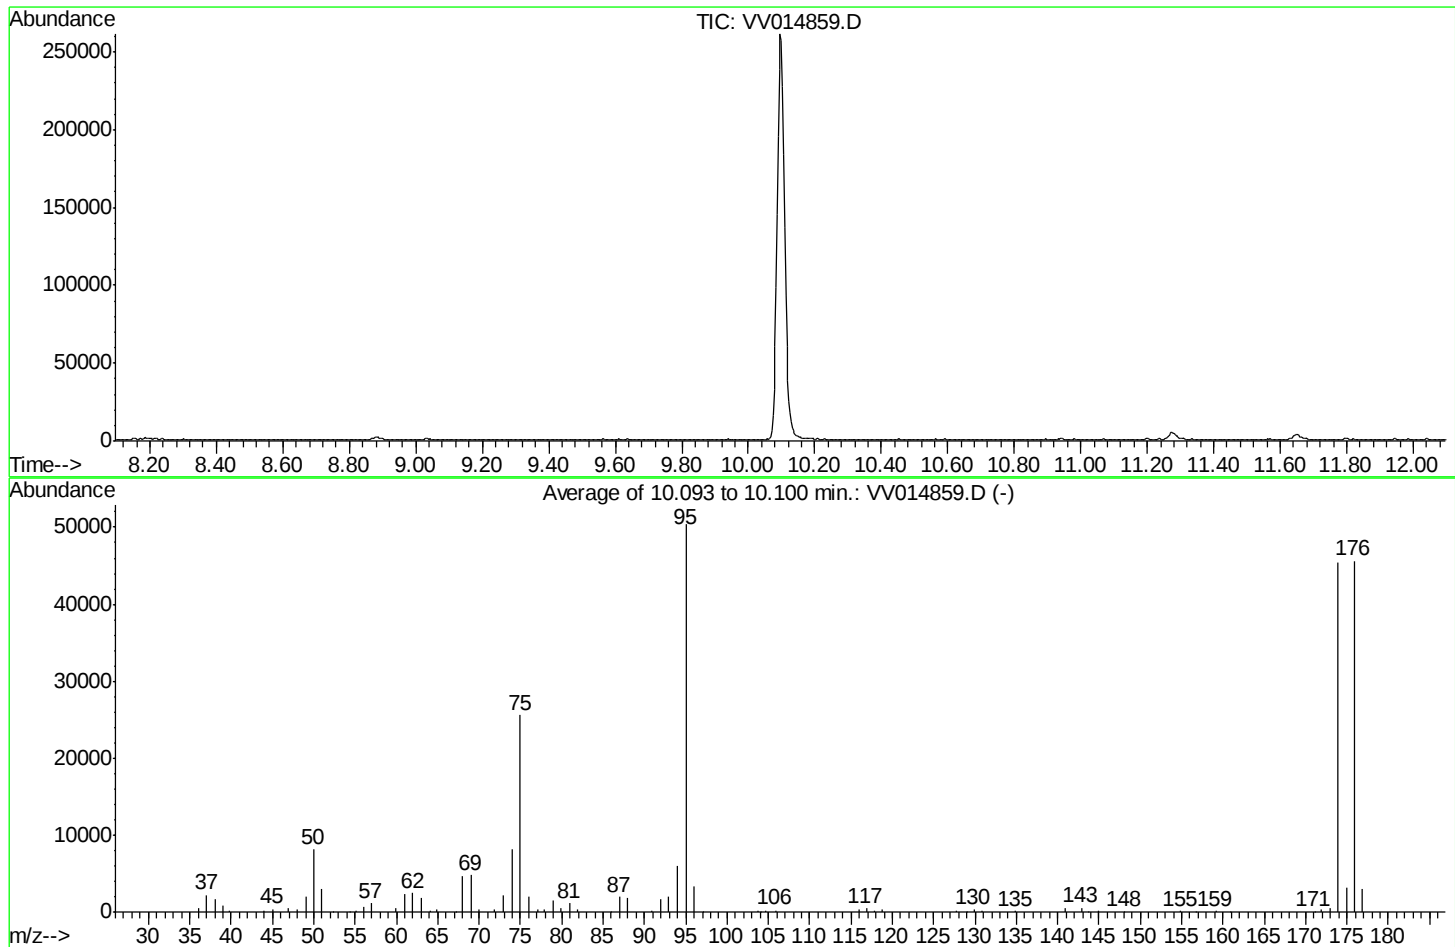

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2789

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.1	8130	PASS
75	95	30	80	50.8	25589	PASS
95	95	100	100	100.0	50381	PASS
96	95	5	9	6.7	3400	PASS
173	174	0.00	2	0.9	426	PASS
174	95	50	120	90.3	45490	PASS
175	174	5	9	6.9	3147	PASS
176	174	95	101	100.3	45605	PASS
177	176	5	9	6.7	3050	PASS

m/z	Abundance
36.00	430.0
37.00	2237.0
38.00	1651.0
39.00	894.0
39.90	472.0
44.00	544.0
45.00	522.0
46.90	639.0
48.00	265.0
49.00	1897.0
50.00	7700.0
51.00	2844.0
52.20	138.0
55.10	237.0
56.00	684.0
56.90	1040.0
59.90	413.0
61.00	1976.0
62.00	2190.0
63.00	1705.0
64.10	177.0
64.90	279.0
68.00	4285.0
69.00	4874.0
70.00	348.0
71.80	294.0
73.00	2107.0
74.00	7940.0
75.00	24840.0
76.00	1859.0
77.10	279.0
77.90	295.0
78.90	1354.0
79.80	454.0
80.90	1099.0
81.90	282.0
87.00	1833.0
87.90	1823.0
90.90	258.0
91.90	1528.0
93.00	1917.0
94.00	5712.0
95.00	48008.0
96.00	3285.0
97.00	109.0
103.80	144.0
104.10	157.0
105.80	153.0
115.90	228.0
116.80	485.0
117.80	158.0
118.80	317.0
127.80	198.0
129.80	220.0
130.90	192.0
134.90	159.0
140.90	541.0
142.90	579.0
145.00	146.0
154.80	122.0
156.70	105.0
159.20	122.0
171.10	105.0
172.00	211.0
173.00	410.0
173.90	42416.0
174.90	3010.0
175.90	41888.0
176.90	3025.0

Instrument :
MSVOA_V
ClientSampleId :
BFB62

m/z	Abundance
36.00	435.0
37.00	2308.0
38.00	1754.0
39.00	960.0
39.80	476.0
44.00	589.0
45.00	548.0
46.90	629.0
48.00	294.0
49.00	2001.0
50.00	8345.0
51.00	3103.0
52.30	111.0
54.30	102.0
55.10	196.0
56.00	611.0
56.90	1142.0
59.90	440.0
61.00	2380.0
62.00	2543.0
63.00	1929.0
64.10	174.0
64.80	282.0
68.00	4733.0
69.00	4907.0
70.00	428.0
71.90	274.0
73.00	2283.0
74.00	8479.0
75.00	26416.0
76.00	2009.0
77.10	357.0
77.90	309.0
78.90	1497.0
79.80	503.0
80.90	1201.0
81.90	325.0
87.00	1990.0
88.00	1957.0
90.90	241.0
92.00	1764.0
92.90	2143.0
94.00	6170.0
95.00	52368.0
96.00	3509.0
103.80	191.0
104.70	110.0
105.90	243.0
115.90	284.0
116.90	435.0
117.80	232.0
118.80	399.0
127.70	226.0
129.90	275.0
130.90	250.0
134.90	148.0
140.90	584.0
142.90	609.0
144.90	173.0
148.10	105.0
154.80	161.0
159.20	119.0
160.90	109.0
171.80	288.0
173.00	437.0
173.90	46928.0
174.90	3243.0
175.90	47632.0
176.90	3118.0

Instrument :
MSVOA_V
ClientSampleId :
BFB62

m/z	Abundance
36.00	425.0
37.00	1965.0
38.00	1602.0
38.90	840.0
39.80	390.0
44.00	642.0
45.00	513.0
46.90	485.0
48.00	290.0
49.00	1868.0
50.00	8345.0
51.00	2825.0
54.30	124.0
55.00	148.0
56.00	537.0
56.90	1101.0
59.90	451.0
61.00	2472.0
62.00	2606.0
63.00	1959.0
64.10	160.0
64.80	224.0
67.20	158.0
68.00	4894.0
69.00	4606.0
70.00	404.0
71.90	281.0
72.90	2303.0
74.00	7963.0
75.00	25512.0
76.00	1991.0
77.10	387.0
77.90	332.0
78.90	1417.0
79.90	501.0
80.90	1194.0
81.90	335.0
85.90	121.0
87.00	2004.0
88.00	1880.0
90.80	208.0
92.00	1766.0
93.00	2112.0
94.00	6263.0
95.00	50768.0
96.00	3407.0
103.80	213.0
104.70	173.0
106.00	284.0
115.90	294.0
116.90	384.0
117.80	247.0
118.80	406.0
127.80	228.0
128.90	124.0
129.80	285.0
130.90	213.0
134.90	121.0
140.90	591.0
142.90	540.0
143.70	102.0
144.90	151.0
148.10	116.0
154.90	192.0
159.00	113.0
160.90	139.0
171.80	376.0
172.90	431.0
173.90	47128.0
174.90	3189.0
175.90	47296.0
176.90	3009.0

Instrument :
MSVOA_V
ClientSampleId :
BFB62

m/z	Abundance
39.90	319.0
42.90	105.0
44.00	458.0
45.20	150.0
45.70	107.0
57.50	137.0

Instrument :
MSVOA_V
ClientSampleId :
BFB62