

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW031221\
 Data File : VW020540.D
 Acq On : 11 Mar 2021 16:29
 Operator : SY/MD
 Sample : M1610-11
 Misc : 5.87G/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG564

Manual Integrations
 APPROVED

MMDadoda
 3/15/2021 12:38:46 PM

Quant Time: Mar 12 07:33:31 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Mar 12 04:11:04 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	580479	50.00	ug/L	# 0.00
28) Chlorobenzene-d5	8.860	117	592829	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.262	152	298978	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	185970	43.71	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	87.42%
7) Chloroethane-d5	1.571	69	141519	42.95	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	85.90%
11) 1,1-Dichloroethene-d2	2.085	63	177616	24.77	ug/L	-0.02
Spiked Amount	50.000	Range	60 - 125	Recovery	=	49.54%#
21) 2-Butanone-d5	3.925	46	170554	79.15	ug/L	0.03
Spiked Amount	100.000	Range	40 - 130	Recovery	=	79.15%
24) Chloroform-d	4.349	84	327988	44.58	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.16%
26) 1,2-Dichloroethane-d4	5.034	65	214236	47.40	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.80%
32) Benzene-d6	5.047	84	709723	47.46	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.92%
36) 1,2-Dichloropropane-d6	6.072	67	208574	46.14	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	92.28%
41) Toluene-d8	7.320	98	685103	47.37	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	94.74%
43) trans-1,3-Dichloroprop...	7.629	79	96980	45.06	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	90.12%
47) 2-Hexanone-d5	8.130	63	153427	94.90	ug/L	0.04
Spiked Amount	100.000	Range	45 - 130	Recovery	=	94.90%
57) 1,1,2,2-Tetrachloroeth...	10.233	84	253852	42.39	ug/L	0.01
Spiked Amount	50.000	Range	65 - 120	Recovery	=	84.78%
64) 1,2-Dichlorobenzene-d4	11.635	152	308504	52.70	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	105.40%
Target Compounds						
					Qvalue	
25) Chloroform	4.378	83	11851	1.63	ug/L	97
34) Trichloroethene	5.915	95	422580	91.26	ug/L	86
46) Tetrachloroethene	7.979	164	2201315	566.63	ug/L	92
48) 2-Hexanone	8.162	43	14436m	4.13	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
Data File : VV020540.D
Acq On : 11 Mar 2021 16:29
Operator : SY/MD
Sample : M1610-11
Misc : 5.87G/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
BG564

Manual Integrations
APPROVED

MMDadoda
3/15/2021 12:38:46 PM

Quant Time: Mar 12 07:33:31 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 12 04:11:04 2021
Response via : Initial Calibration

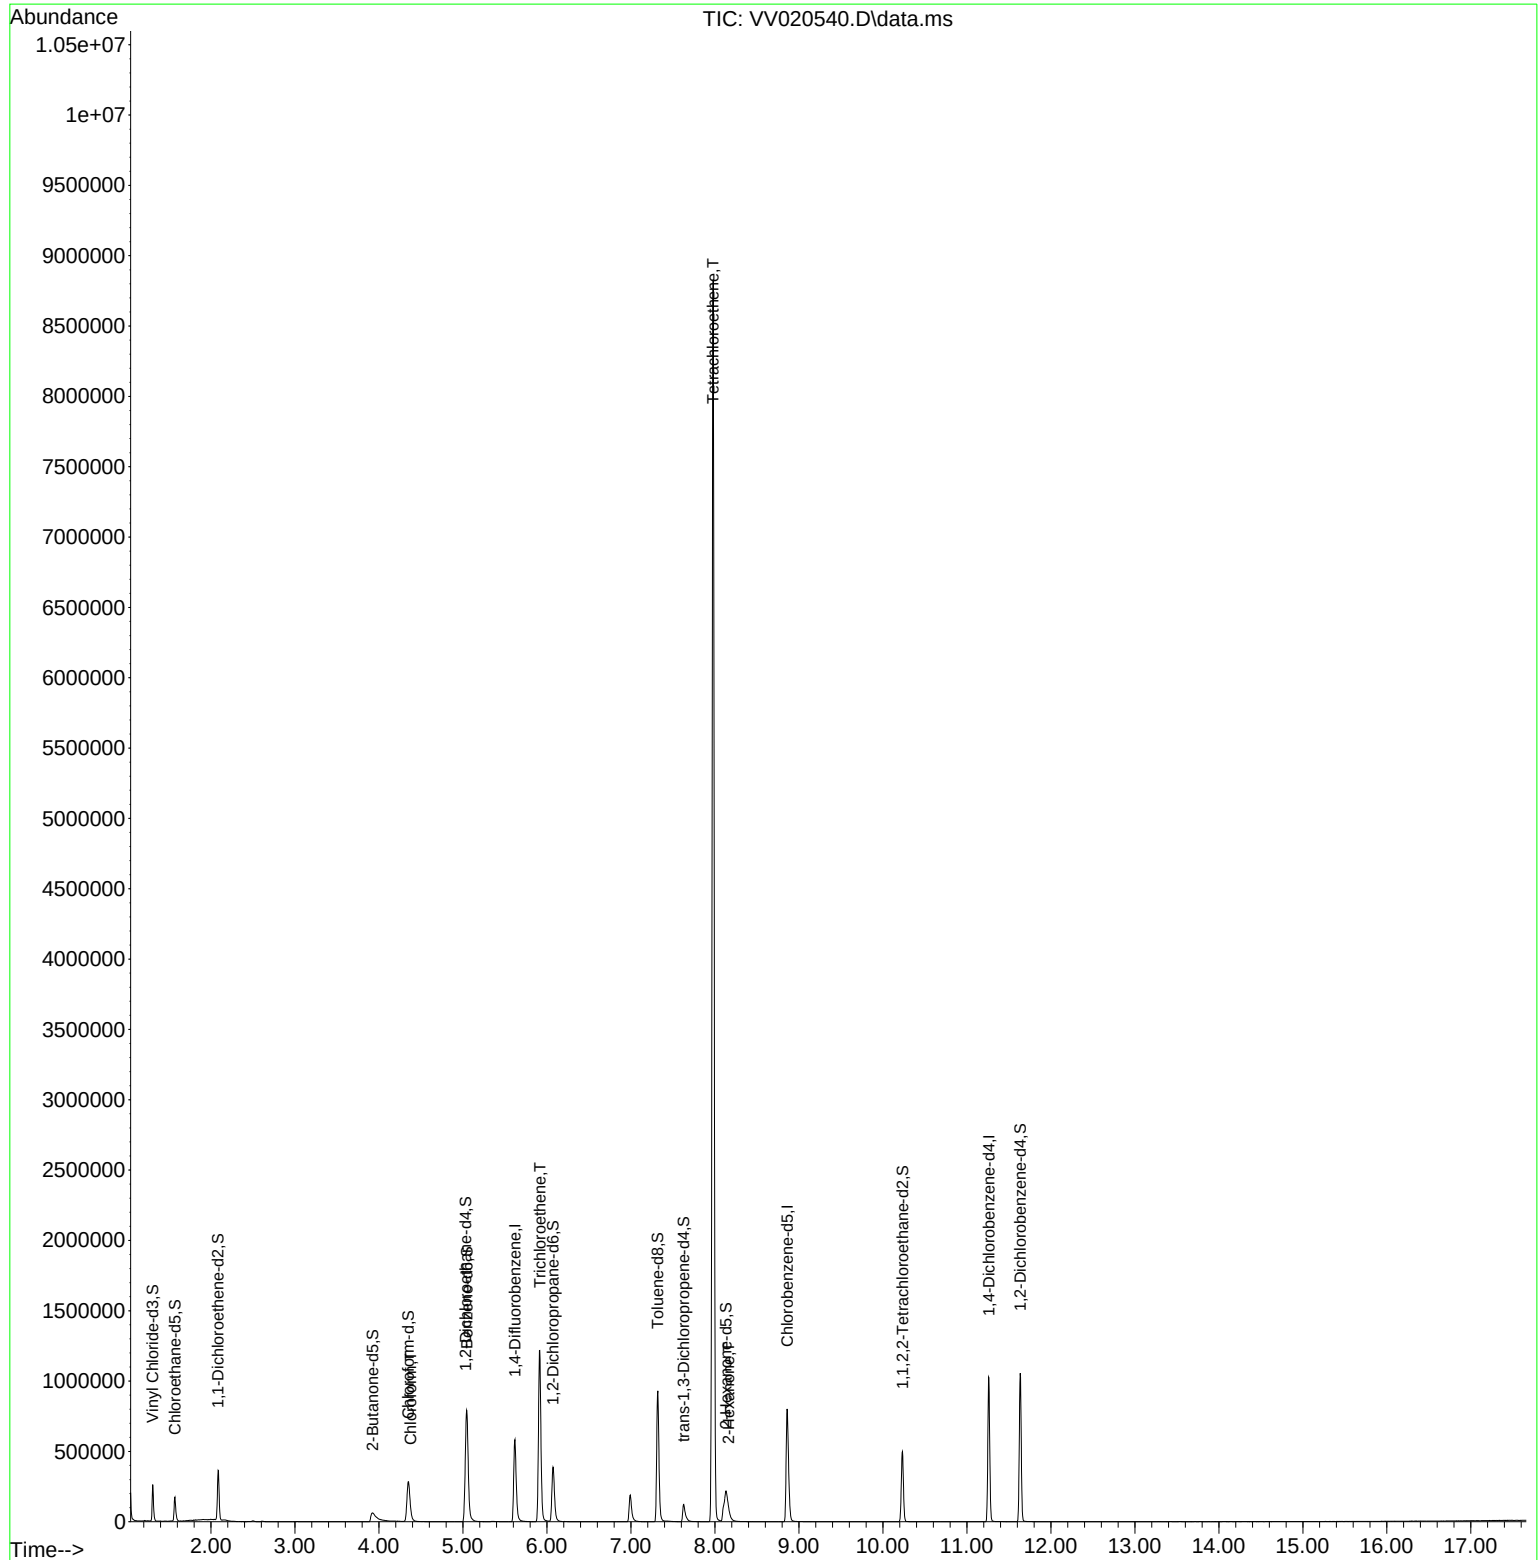

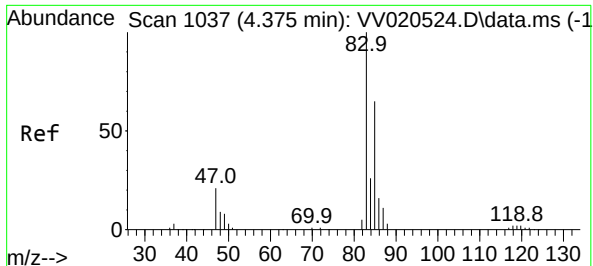





#25
Chloroform
Concen: 1.63 ug/L
RT: 4.378 min Scan# 1038
Delta R.T. 0.003 min
Lab File: VV020540.D
Acq: 11 Mar 2021 16:29

Tgt Ion: 83 Resp: 11851
Ion Ratio Lower Upper
83 100
85 65.7 44.2 82.2

Instrument :
MSVOA_V
ClientSampled :
BG564




Manual Integrations
APPROVED


MMDadoda
3/15/2021 12:38:46 PM

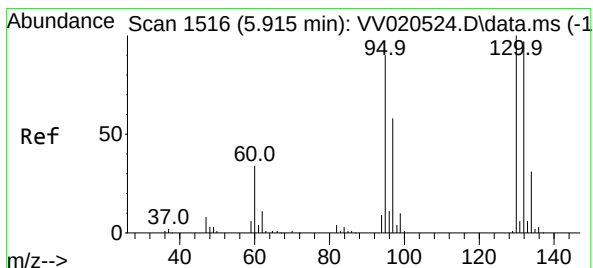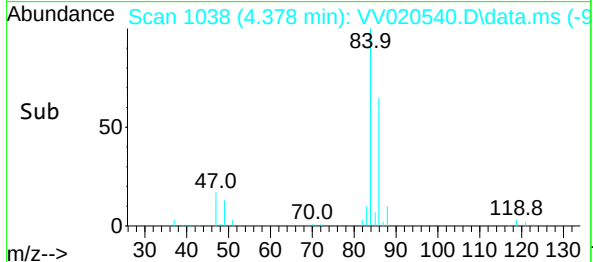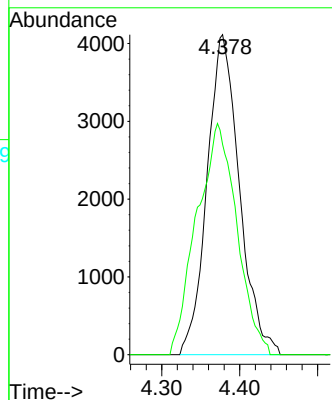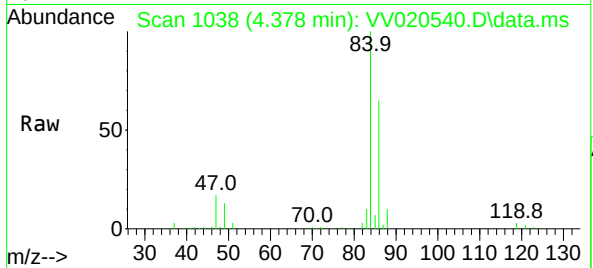

#34
Trichloroethene
Concen: 91.26 ug/L
RT: 5.915 min Scan# 1516
Delta R.T. 0.000 min
Lab File: VV020540.D
Acq: 11 Mar 2021 16:29


Tgt Ion: 95 Resp: 422580
Ion Ratio Lower Upper
95 100
97 64.5 44.5 82.7
132 108.5 63.4 117.8
130 113.6 67.1 124.5

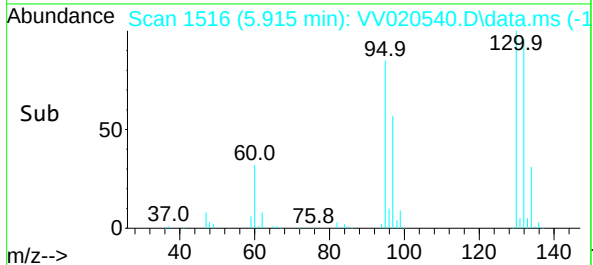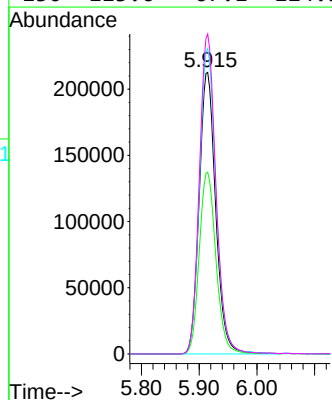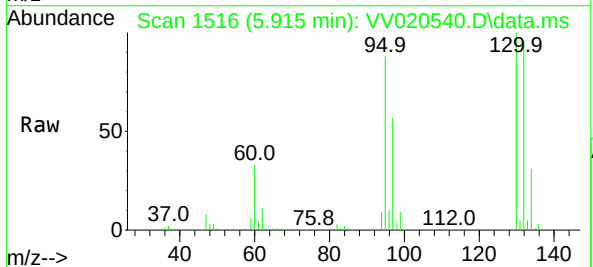

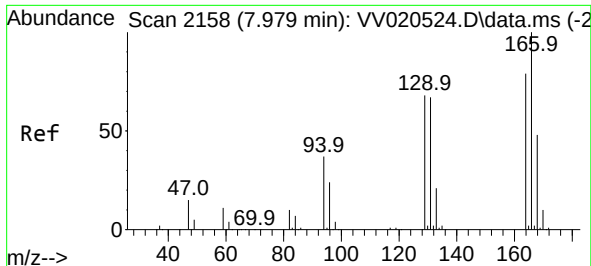

#46
Tetrachloroethene
Concen: 566.63 ug/L
RT: 7.979 min Scan# 2158
Delta R.T. 0.000 min
Lab File: VV020540.D
Acq: 11 Mar 2021 16:29




Instrument :
MSVOA_V
ClientSampled :
BG564

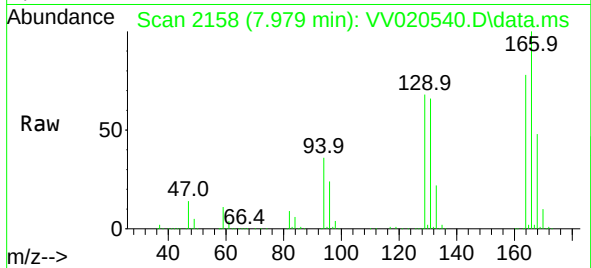


Tgt Ion:164 Resp: 2201315
Ion Ratio Lower Upper
164 100
129 87.0 70.6 131.0
131 84.2 66.8 124.0
166 128.0 88.2 163.8

Manual Integrations
APPROVED

MMDadoda
3/15/2021 12:38:46 PM

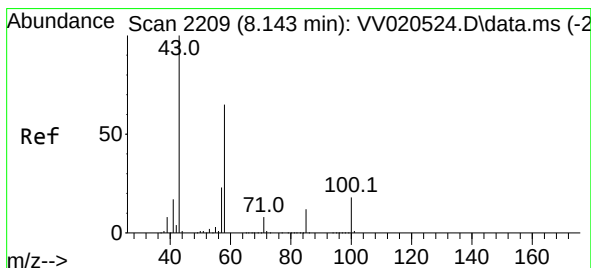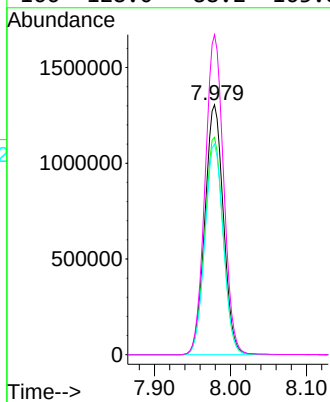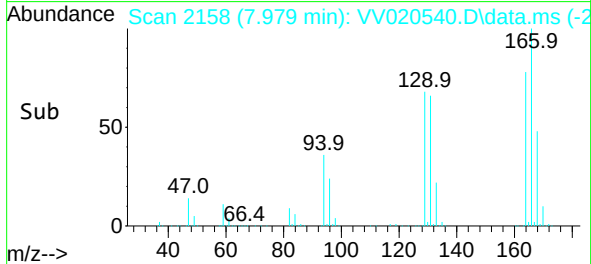

#48
2-Hexanone
Concen: 4.13 ug/L m
RT: 8.162 min Scan# 2215
Delta R.T. 0.019 min
Lab File: VV020540.D
Acq: 11 Mar 2021 16:29

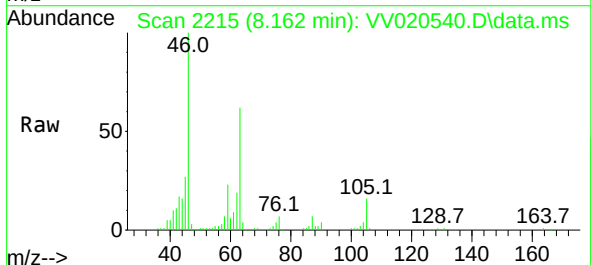

Tgt Ion: 43 Resp: 14436
Ion Ratio Lower Upper
43 100
58 32.3 41.8 62.6#
57 18.0 15.0 22.4
100 0.7 8.9 13.3#

