

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
 Data File : VV020547.D
 Acq On : 11 Mar 2021 20:01
 Operator : SY/MD
 Sample : VV0312WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK65

Quant Time: Mar 12 07:54:54 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Mar 12 07:54:21 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	535261	50.00	ug/L	# 0.00
28) Chlorobenzene-d5	8.857	117	525152	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.255	152	271436	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	153296	39.07	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	78.14%
7) Chloroethane-d5	1.571	69	132555	43.63	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	87.26%
11) 1,1-Dichloroethene-d2	2.108	63	207281	31.35	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	62.70%
21) 2-Butanone-d5	3.905	46	184338	92.78	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	92.78%
24) Chloroform-d	4.352	84	302706	44.62	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.24%
26) 1,2-Dichloroethane-d4	5.037	65	193161	46.34	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.68%
32) Benzene-d6	5.053	84	624334	47.13	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.26%
36) 1,2-Dichloropropane-d6	6.072	67	187085	46.72	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	93.44%
41) Toluene-d8	7.320	98	568810	44.40	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	88.80%
43) trans-1,3-Dichloroprop...	7.625	79	84771	44.47	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	88.94%
47) 2-Hexanone-d5	8.095	63	126477	88.31	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	88.31%
57) 1,1,2,2-Tetrachloroeth...	10.220	84	230879	43.52	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	87.04%
64) 1,2-Dichlorobenzene-d4	11.632	152	278940	52.49	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	104.98%
Target Compounds						
48) 2-Hexanone	8.146	43	11629	3.76	ug/L	# 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
Data File : VV020547.D
Acq On : 11 Mar 2021 20:01
Operator : SY/MD
Sample : VV0312WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK65


Quant Time: Mar 12 07:54:54 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 12 07:54:21 2021
Response via : Initial Calibration

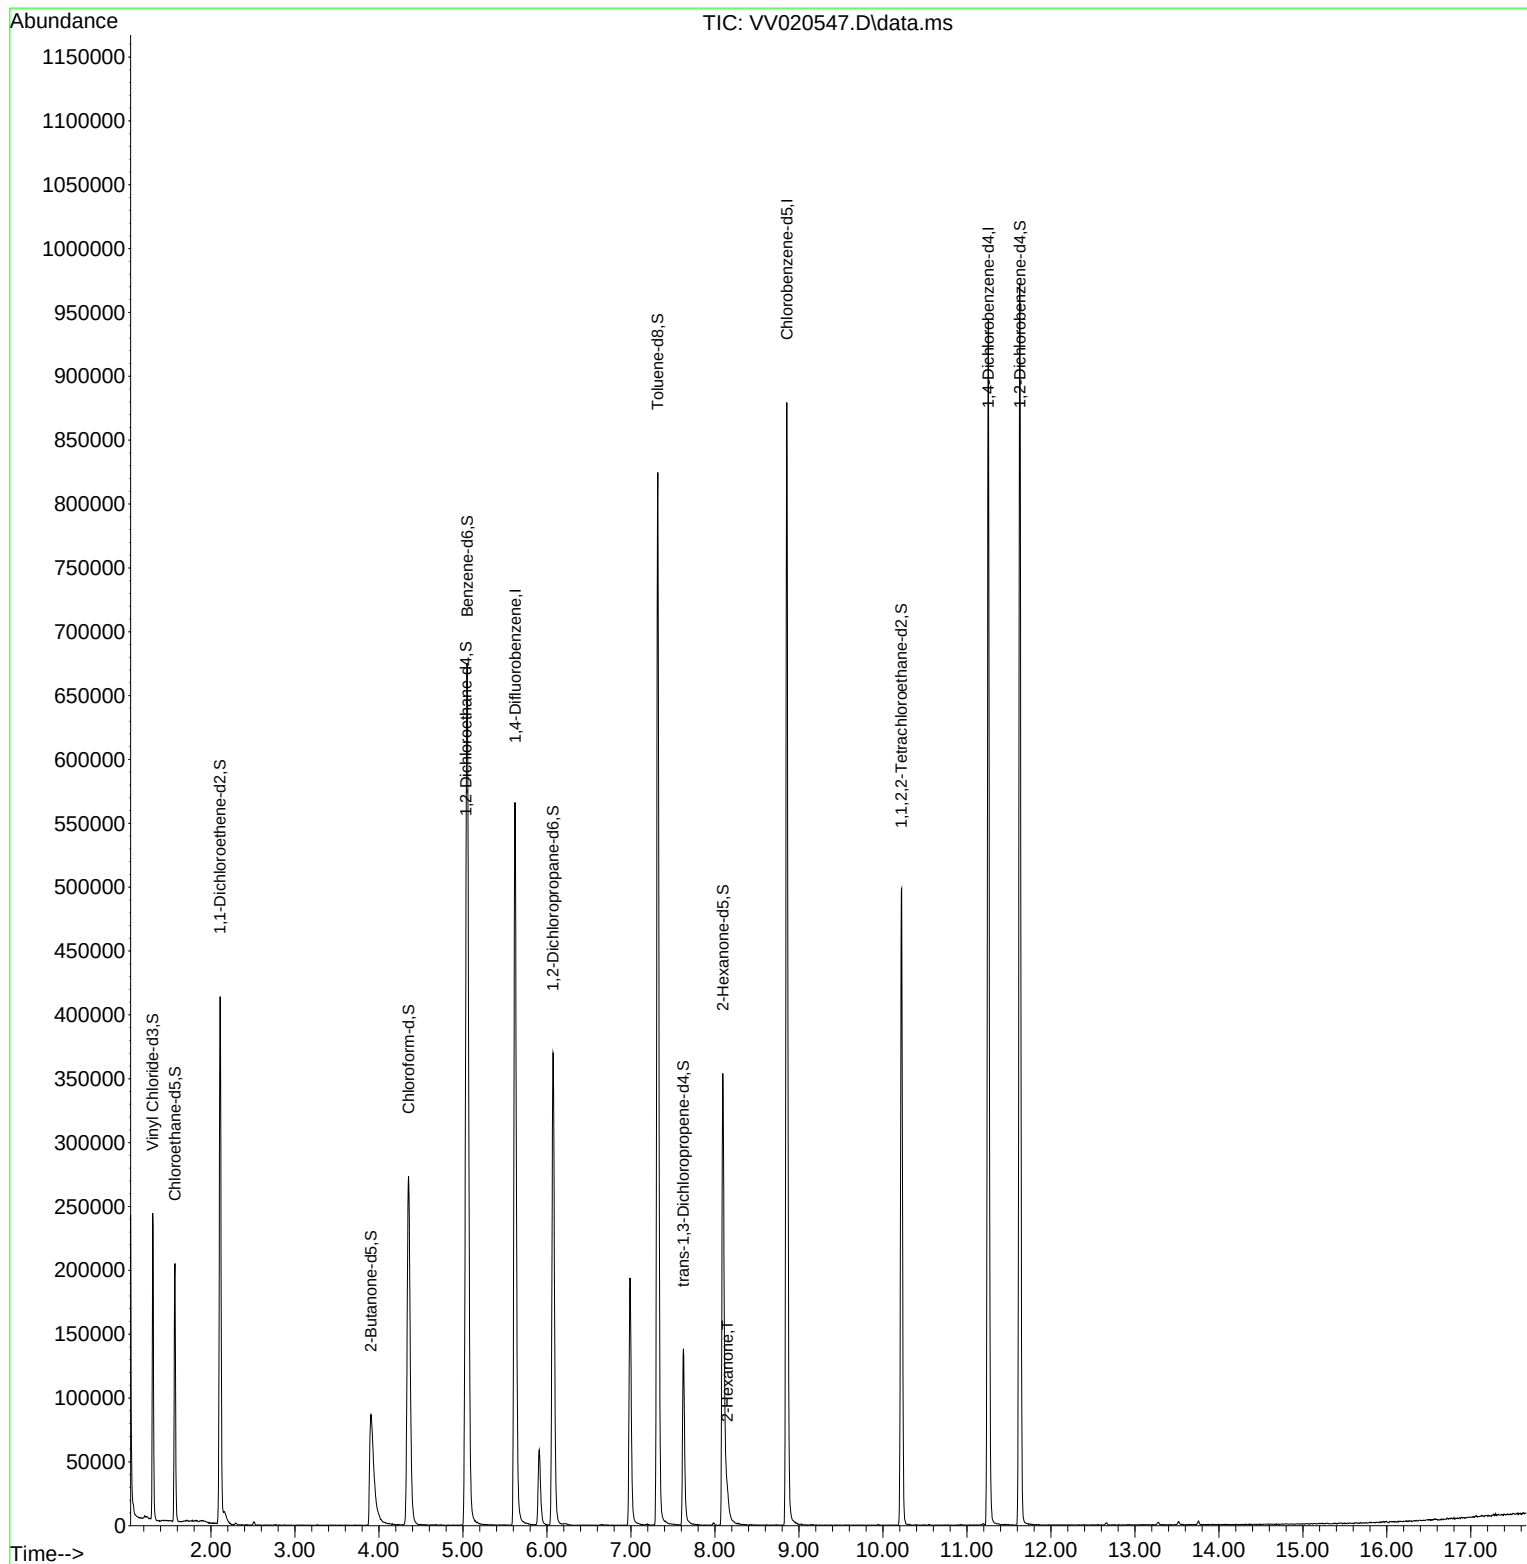

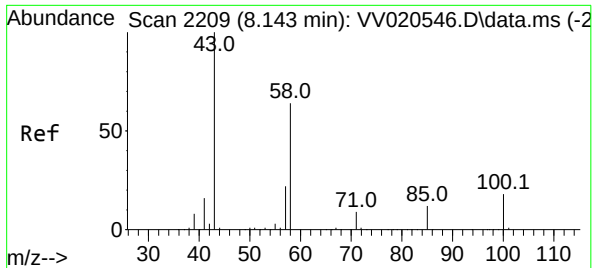

#48
 2-Hexanone
 Concen: 3.76 ug/L
 RT: 8.146 min Scan# 2210
 Delta R.T. 0.003 min
 Lab File: VV020547.D
 Acq: 11 Mar 2021 20:01

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK65

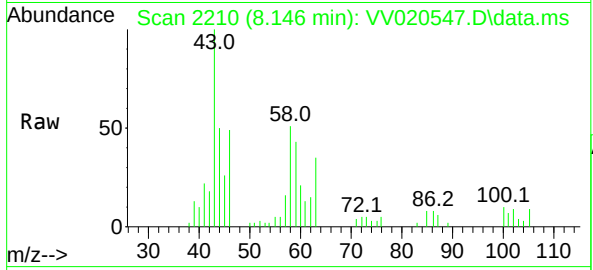

Tgt Ion: 43 Resp: 11629

Ion	Ratio	Lower	Upper
43	100		
58	51.6	41.8	62.6
57	10.2	15.0	22.4#
100	9.2	8.9	13.3

