

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
 Data File : VV020525.D
 Acq On : 11 Mar 2021 10:35
 Operator : SY/MD
 Sample : VV0312MBL01
 Misc : 5.00G/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK63

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M

Title : VOC Analysis

Signal : TIC: VV020525.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	104	rVB	270071	272611	15.12%	1.900%
2	1.571	157	165	177	rBV	217055	243865	13.53%	1.700%
3	1.970	285	289	293	rBV3	714	673	0.04%	0.005%
4	2.108	321	332	363	rVB	455752	680212	37.73%	4.741%
5	2.294	380	390	397	rBV2	1377	2041	0.11%	0.014%
6	2.510	450	457	458	rBV3	2067	2189	0.12%	0.015%
7	2.622	489	492	498	rVB3	268	235	0.01%	0.002%
8	2.754	526	533	535	rBV5	401	297	0.02%	0.002%
9	2.773	537	539	544	rVV2	354	217	0.01%	0.002%
10	2.818	550	553	556	rVB	246	161	0.01%	0.001%
11	2.841	556	560	570	rVB	364	458	0.03%	0.003%
12	2.883	570	573	576	rBV2	252	165	0.01%	0.001%
13	3.285	694	698	702	rVB2	233	168	0.01%	0.001%
14	3.375	722	726	731	rVB2	218	184	0.01%	0.001%
15	3.404	731	735	740	rBV2	172	197	0.01%	0.001%
16	3.513	762	769	771	rBV2	405	423	0.02%	0.003%
17	3.600	793	796	800	rBV	349	166	0.01%	0.001%
18	3.667	812	817	821	rBV2	162	173	0.01%	0.001%
19	3.899	878	889	932	rBV	99600	336676	18.68%	2.347%
20	4.265	1000	1003	1005	rBV2	247	191	0.01%	0.001%
21	4.352	1013	1030	1058	rBV	289218	727557	40.36%	5.071%
22	4.664	1126	1127	1132	rVB	225	171	0.01%	0.001%
23	4.725	1143	1146	1147	rBV	316	160	0.01%	0.001%
24	4.773	1159	1161	1164	rVV2	294	184	0.01%	0.001%
25	5.050	1230	1247	1284	rBV2	710500	1802654	100.00%	12.566%
26	5.413	1358	1360	1368	rVB4	476	562	0.03%	0.004%
27	5.490	1380	1384	1385	rBV	288	224	0.01%	0.002%
28	5.535	1393	1398	1402	rVB	380	298	0.02%	0.002%
29	5.561	1402	1406	1410	rBV2	360	288	0.02%	0.002%
30	5.622	1410	1425	1454	rBV	581450	1161582	64.44%	8.097%
31	5.908	1502	1514	1539	rVB	62023	129026	7.16%	0.899%
32	5.998	1539	1542	1548	rVB4	678	591	0.03%	0.004%
33	6.072	1548	1565	1590	rBV	386734	787267	43.67%	5.488%
34	6.304	1633	1637	1641	rVV3	265	236	0.01%	0.002%
35	6.416	1666	1672	1674	rBV	168	179	0.01%	0.001%
36	6.513	1699	1702	1706	rVB2	232	179	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
 Data File : VV020525.D
 Acq On : 11 Mar 2021 10:35
 Operator : SY/MD
 Sample : VV0312MBL01
 Misc : 5.00G/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK63

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
 Title : VOC Analysis

37	6.651	1736	1745	1748	rBV5	663	963	0.05%	0.007%
38	6.667	1748	1750	1754	rVB2	476	242	0.01%	0.002%
39	6.796	1788	1790	1794	rVB2	304	204	0.01%	0.001%
40	6.831	1794	1801	1809	rBV2	240	379	0.02%	0.003%
41	6.989	1839	1850	1877	rBV	201925	370021	20.53%	2.579%
42	7.137	1895	1896	1900	rVB3	594	300	0.02%	0.002%
43	7.320	1940	1953	1976	rBV	881020	1501342	83.29%	10.465%
44	7.625	2036	2048	2080	rBV	146311	255598	14.18%	1.782%
45	7.809	2102	2105	2108	rBV3	322	168	0.01%	0.001%
46	7.928	2139	2142	2146	rBV	300	230	0.01%	0.002%
47	7.982	2149	2159	2162	rBV3	972	1057	0.06%	0.007%
48	8.095	2183	2194	2232	rBV2	375993	773701	42.92%	5.393%
49	8.455	2304	2306	2310	rVB2	318	173	0.01%	0.001%
50	8.481	2310	2314	2318	rBV2	373	253	0.01%	0.002%
51	8.516	2318	2325	2329	rVB3	348	415	0.02%	0.003%
52	8.538	2329	2332	2339	rBV3	330	373	0.02%	0.003%
53	8.577	2339	2344	2347	rVB3	212	191	0.01%	0.001%
54	8.616	2352	2356	2360	rVB	328	279	0.02%	0.002%
55	8.754	2393	2399	2402	rBV2	218	184	0.01%	0.001%
56	8.857	2419	2431	2466	rBV	911963	1460347	81.01%	10.179%
57	9.098	2501	2506	2509	rBV3	522	501	0.03%	0.003%
58	9.153	2520	2523	2526	rBV2	564	346	0.02%	0.002%
59	9.230	2538	2547	2551	rBV3	253	349	0.02%	0.002%
60	9.355	2579	2586	2592	rVB2	230	388	0.02%	0.003%
61	9.702	2692	2694	2699	rVB	203	163	0.01%	0.001%
62	9.789	2714	2721	2723	rBV2	172	179	0.01%	0.001%
63	9.944	2763	2769	2777	rVB3	475	746	0.04%	0.005%
64	9.989	2777	2783	2788	rBV2	250	304	0.02%	0.002%
65	10.066	2799	2807	2811	rBV2	189	226	0.01%	0.002%
66	10.114	2816	2822	2826	rBV2	168	227	0.01%	0.002%
67	10.223	2843	2856	2881	rBV	513410	807096	44.77%	5.626%
68	10.442	2920	2924	2927	rBV2	273	208	0.01%	0.001%
69	10.464	2927	2931	2935	rBV2	218	222	0.01%	0.002%
70	10.558	2954	2960	2963	rBV2	351	390	0.02%	0.003%
71	10.648	2985	2988	2992	rVB	211	168	0.01%	0.001%
72	10.696	2998	3003	3006	rBV	182	195	0.01%	0.001%
73	10.744	3016	3018	3024	rVB	258	169	0.01%	0.001%
74	10.921	3069	3073	3083	rVB3	483	760	0.04%	0.005%
75	11.175	3150	3152	3154	rBV2	436	300	0.02%	0.002%
76	11.191	3154	3157	3160	rVV2	364	335	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
 Data File : VV020525.D
 Acq On : 11 Mar 2021 10:35
 Operator : SY/MD
 Sample : VV0312MBL01
 Misc : 5.00G/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK63

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M

Title : VOC Analysis

77	11.255	3165	3177	3201	rBV	952086	1465359	81.29%	10.214%
78	11.468	3241	3243	3246	rBV3	341	209	0.01%	0.001%
79	11.632	3281	3294	3313	rBV	983002	1535393	85.17%	10.703%
80	11.799	3343	3346	3348	rVB	649	312	0.02%	0.002%
81	11.879	3368	3371	3374	rBV2	246	201	0.01%	0.001%
82	12.207	3470	3473	3478	rVV3	395	364	0.02%	0.003%
83	12.358	3516	3520	3521	rBV	220	162	0.01%	0.001%
84	12.410	3533	3536	3541	rVB2	301	231	0.01%	0.002%
85	12.513	3565	3568	3571	rBV2	244	191	0.01%	0.001%
86	12.558	3576	3582	3583	rBV	374	259	0.01%	0.002%
87	12.660	3607	3614	3623	rBV	1545	2195	0.12%	0.015%
88	12.722	3629	3633	3635	rBV2	350	233	0.01%	0.002%
89	12.924	3693	3696	3702	rVB2	351	288	0.02%	0.002%
90	13.104	3749	3752	3754	rBV2	329	185	0.01%	0.001%
91	13.281	3798	3807	3813	rVB4	1749	2590	0.14%	0.018%
92	13.445	3854	3858	3864	rBV3	326	396	0.02%	0.003%
93	13.490	3869	3872	3874	rBV2	281	176	0.01%	0.001%
94	13.516	3876	3880	3881	rBV	863	610	0.03%	0.004%
95	13.760	3949	3956	3963	rBV4	1977	2881	0.16%	0.020%
96	14.059	4045	4049	4051	rBV	281	210	0.01%	0.001%
97	14.104	4058	4063	4067	rBV2	342	397	0.02%	0.003%
98	14.210	4093	4096	4098	rBV	331	224	0.01%	0.002%
99	14.332	4132	4134	4137	rVB	437	229	0.01%	0.002%
100	15.348	4447	4450	4454	rBV4	635	562	0.03%	0.004%




Sum of corrected areas: 14346009

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
Data File : VV020525.D
Acq On : 11 Mar 2021 10:35
Operator : SY/MD
Sample : VV0312MBL01
Misc : 5.00G/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK63

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

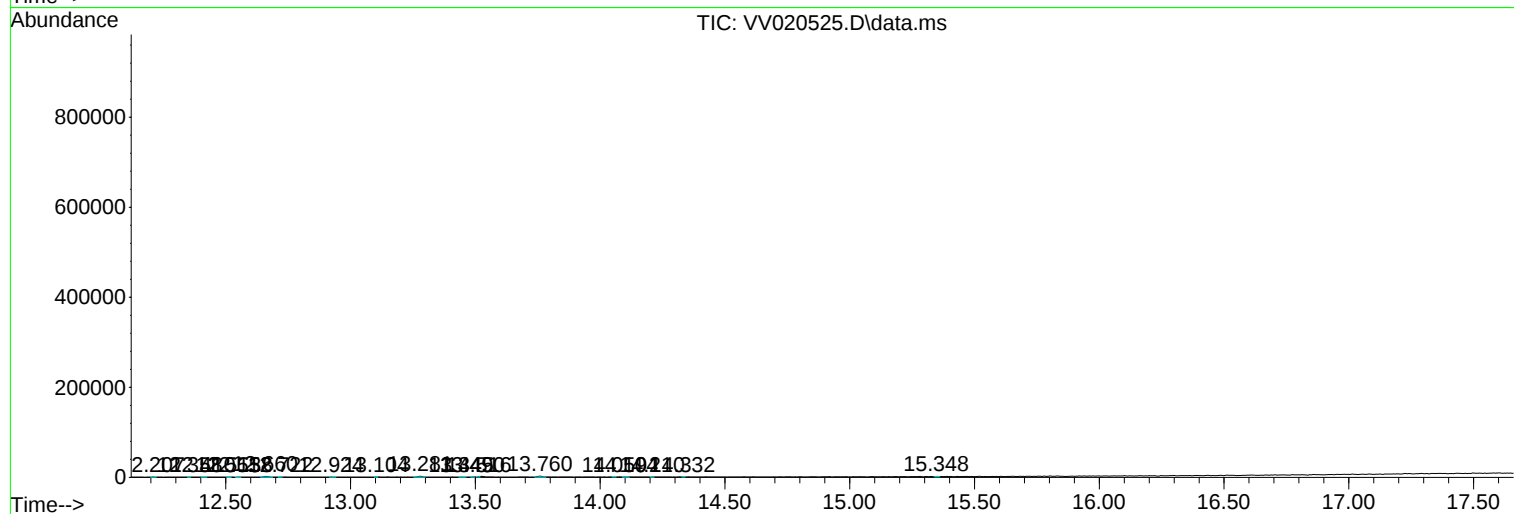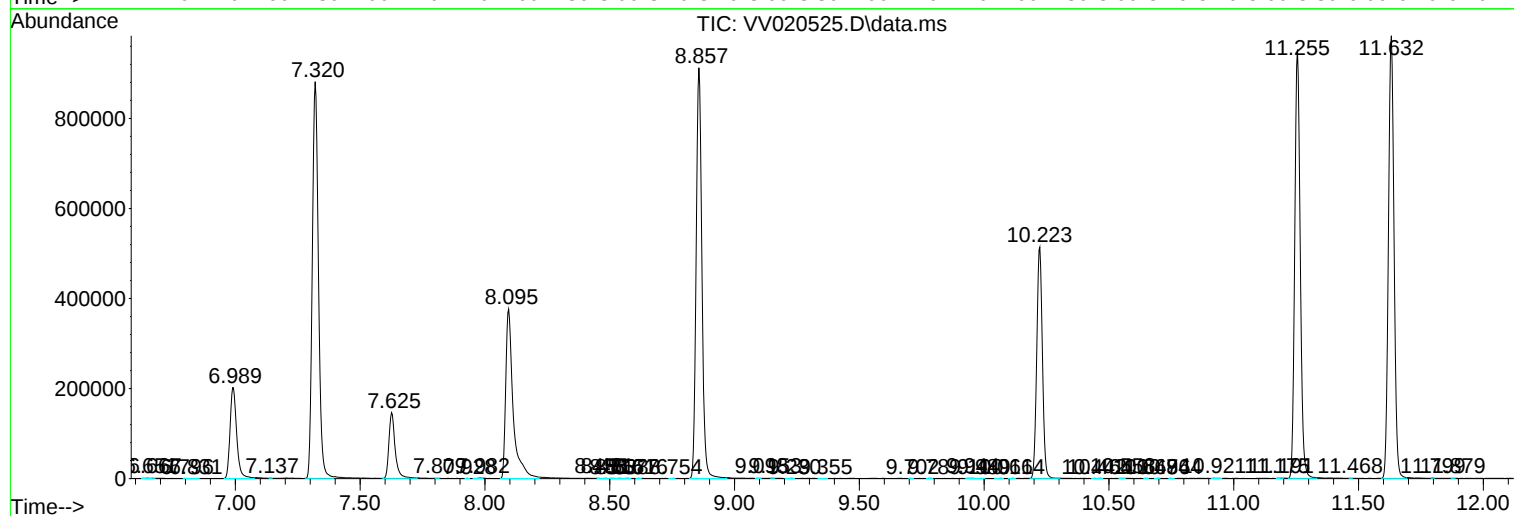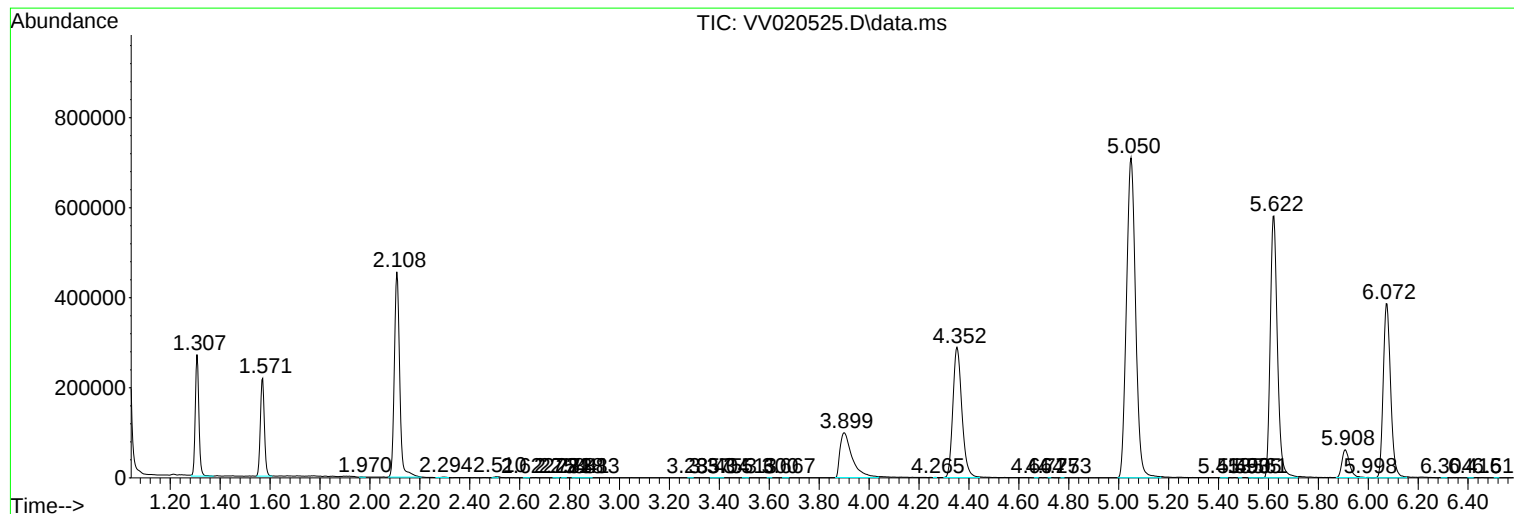

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
Data File : VV020525.D
Acq On : 11 Mar 2021 10:35
Operator : SY/MD
Sample : VV0312MBL01
Misc : 5.00G/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK63

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
Data File : VV020525.D
Acq On : 11 Mar 2021 10:35
Operator : SY/MD
Sample : VV0312MBL01
Misc : 5.00G/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK63

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
