

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
 Data File : VV020527.D
 Acq On : 11 Mar 2021 11:22
 Operator : SY/MD
 Sample : M1610-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M

Title : VOC Analysis

Signal : TIC: VV020527.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	97	rVB	247515	255658	15.03%	1.865%
2	1.568	156	164	177	rVB	205685	229432	13.48%	1.674%
3	2.108	320	332	365	rVB	422439	637359	37.46%	4.649%
4	2.510	451	457	466	rVB4	1558	2438	0.14%	0.018%
5	2.677	506	509	511	rVB2	263	163	0.01%	0.001%
6	2.693	511	514	520	rBV2	312	227	0.01%	0.002%
7	2.728	520	525	531	rBV2	292	333	0.02%	0.002%
8	2.863	564	567	571	rBV2	208	247	0.01%	0.002%
9	3.066	627	630	634	rVB	269	193	0.01%	0.001%
10	3.596	791	795	799	rBV2	227	219	0.01%	0.002%
11	3.661	812	815	825	rVB2	235	353	0.02%	0.003%
12	3.902	878	890	928	rBV	90465	311075	18.28%	2.269%
13	4.352	1013	1030	1060	rBV2	270283	681943	40.08%	4.974%
14	4.526	1081	1084	1088	rVB3	532	455	0.03%	0.003%
15	4.548	1088	1091	1093	rBV	375	264	0.02%	0.002%
16	4.564	1094	1096	1103	rVB4	436	294	0.02%	0.002%
17	4.632	1113	1117	1119	rBV2	232	156	0.01%	0.001%
18	4.645	1119	1121	1129	rVV4	228	224	0.01%	0.002%
19	4.748	1149	1153	1155	rBV3	264	187	0.01%	0.001%
20	4.760	1155	1157	1162	rVB2	331	234	0.01%	0.002%
21	4.809	1166	1172	1174	rBV	274	205	0.01%	0.001%
22	5.050	1229	1247	1277	rBV2	677194	1701506	100.00%	12.411%
23	5.223	1298	1301	1305	rBV4	363	292	0.02%	0.002%
24	5.619	1412	1424	1451	rBV	578989	1153551	67.80%	8.414%
25	5.860	1497	1499	1502	rBV2	321	232	0.01%	0.002%
26	5.908	1502	1514	1537	rVV	58370	120405	7.08%	0.878%
27	6.008	1542	1545	1548	rVB3	404	296	0.02%	0.002%
28	6.072	1552	1565	1588	rBV	364308	742314	43.63%	5.415%
29	6.194	1600	1603	1605	rBV2	554	317	0.02%	0.002%
30	6.211	1605	1608	1610	rBV3	588	451	0.03%	0.003%
31	6.272	1625	1627	1630	rBV2	251	161	0.01%	0.001%
32	6.301	1634	1636	1640	rVB3	328	212	0.01%	0.002%
33	6.452	1677	1683	1685	rBB2	274	199	0.01%	0.001%
34	6.493	1688	1696	1698	rBV	197	233	0.01%	0.002%
35	6.590	1723	1726	1731	rBV	252	166	0.01%	0.001%
36	6.635	1734	1740	1742	rBV2	427	409	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
 Data File : VV020527.D
 Acq On : 11 Mar 2021 11:22
 Operator : SY/MD
 Sample : M1610-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
 Title : VOC Analysis

37	6.709	1760	1763	1768	rVB2	247	186	0.01%	0.001%
38	6.796	1787	1790	1799	rVB2	181	189	0.01%	0.001%
39	6.841	1799	1804	1807	rBV2	206	180	0.01%	0.001%
40	6.989	1839	1850	1876	rBV	192410	350036	20.57%	2.553%
41	7.320	1938	1953	1983	rBV	821685	1421398	83.54%	10.368%
42	7.587	2032	2036	2037	rBV3	403	201	0.01%	0.001%
43	7.625	2038	2048	2077	rVV	133874	237991	13.99%	1.736%
44	7.780	2093	2096	2099	rVV3	323	245	0.01%	0.002%
45	7.841	2113	2115	2120	rVB2	286	164	0.01%	0.001%
46	7.873	2120	2125	2131	rVB3	320	368	0.02%	0.003%
47	7.982	2156	2159	2160	rBV2	344	189	0.01%	0.001%
48	8.059	2178	2183	2184	rBV2	325	161	0.01%	0.001%
49	8.095	2184	2194	2236	rBV2	349548	731004	42.96%	5.332%
50	8.304	2257	2259	2261	rBV	396	191	0.01%	0.001%
51	8.355	2271	2275	2278	rVB3	317	235	0.01%	0.002%
52	8.381	2281	2283	2287	rBV2	265	172	0.01%	0.001%
53	8.484	2312	2315	2323	rVB	270	334	0.02%	0.002%
54	8.526	2323	2328	2331	rBV2	548	372	0.02%	0.003%
55	8.857	2419	2431	2473	rVV	889852	1448163	85.11%	10.563%
56	9.146	2515	2521	2526	rBV3	562	590	0.03%	0.004%
57	9.201	2537	2538	2541	rVB	432	210	0.01%	0.002%
58	9.220	2541	2544	2547	rBV2	244	191	0.01%	0.001%
59	9.558	2645	2649	2653	rVB3	311	216	0.01%	0.002%
60	9.641	2672	2675	2678	rVB2	307	186	0.01%	0.001%
61	9.673	2678	2685	2688	rBV2	219	264	0.02%	0.002%
62	9.773	2714	2716	2722	rVB2	286	196	0.01%	0.001%
63	9.873	2744	2747	2753	rVB2	150	155	0.01%	0.001%
64	9.960	2771	2774	2776	rBV2	238	184	0.01%	0.001%
65	10.091	2809	2815	2819	rBV2	297	399	0.02%	0.003%
66	10.223	2843	2856	2875	rVV	482748	756499	44.46%	5.518%
67	10.548	2953	2957	2959	rBV2	257	170	0.01%	0.001%
68	10.686	2997	3000	3005	rBV2	244	267	0.02%	0.002%
69	11.053	3111	3114	3118	rBV2	161	155	0.01%	0.001%
70	11.152	3140	3145	3148	rBV2	366	329	0.02%	0.002%
71	11.188	3154	3156	3162	rBV3	272	323	0.02%	0.002%
72	11.255	3165	3177	3195	rBV	957087	1455137	85.52%	10.614%
73	11.484	3243	3248	3249	rBV2	364	262	0.02%	0.002%
74	11.632	3280	3294	3315	rBV	936122	1451781	85.32%	10.590%
75	11.757	3329	3333	3336	rVV3	441	344	0.02%	0.003%
76	11.786	3339	3342	3345	rVB2	395	246	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
 Data File : VV020527.D
 Acq On : 11 Mar 2021 11:22
 Operator : SY/MD
 Sample : M1610-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M

Title : VOC Analysis

77	11.911	3379	3381	3386	rVB2	288	177	0.01%	0.001%
78	12.075	3429	3432	3439	rVB2	295	317	0.02%	0.002%
79	12.117	3443	3445	3448	rVV	237	178	0.01%	0.001%
80	12.149	3452	3455	3460	rBV2	227	206	0.01%	0.002%
81	12.194	3467	3469	3474	rVB	245	165	0.01%	0.001%
82	12.513	3565	3568	3572	rBV	359	313	0.02%	0.002%
83	12.583	3587	3590	3596	rVB2	311	327	0.02%	0.002%
84	12.667	3608	3616	3622	rBV5	611	1029	0.06%	0.008%
85	12.693	3622	3624	3628	rVB2	305	180	0.01%	0.001%
86	12.747	3637	3641	3643	rBV2	254	196	0.01%	0.001%
87	12.927	3694	3697	3700	rBV2	309	157	0.01%	0.001%
88	13.078	3741	3744	3749	rBV2	198	184	0.01%	0.001%
89	13.114	3752	3755	3758	rBV	217	169	0.01%	0.001%
90	13.230	3787	3791	3794	rBV2	256	192	0.01%	0.001%
91	13.426	3849	3852	3856	rBV	437	343	0.02%	0.003%
92	13.676	3928	3930	3935	rBV2	251	227	0.01%	0.002%
93	13.712	3935	3941	3944	rBV3	402	463	0.03%	0.003%
94	13.754	3951	3954	3955	rBV2	571	332	0.02%	0.002%
95	14.210	4093	4096	4098	rBV	436	289	0.02%	0.002%
96	14.323	4129	4131	4138	rVB2	472	281	0.02%	0.002%
97	14.438	4163	4167	4174	rBV3	505	649	0.04%	0.005%
98	14.487	4179	4182	4186	rVV	443	313	0.02%	0.002%
99	14.847	4291	4294	4295	rBV2	417	226	0.01%	0.002%
100	15.554	4512	4514	4516	rBV2	541	201	0.01%	0.001%




Sum of corrected areas: 13709400

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
Data File : VV020527.D
Acq On : 11 Mar 2021 11:22
Operator : SY/MD
Sample : M1610-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

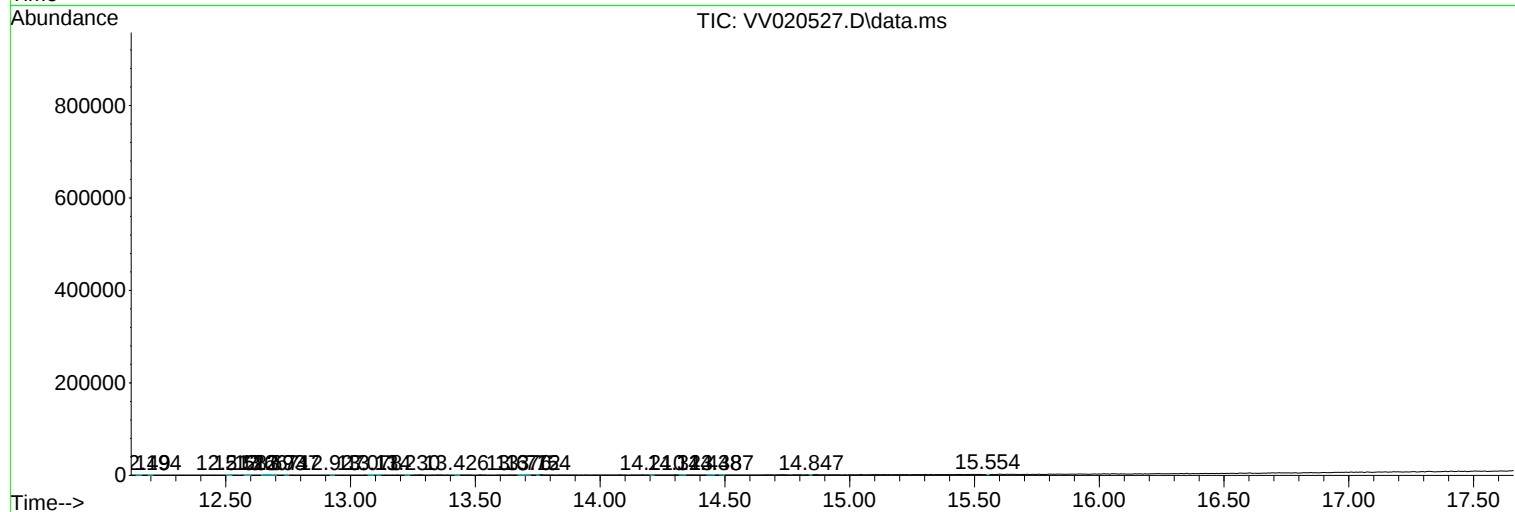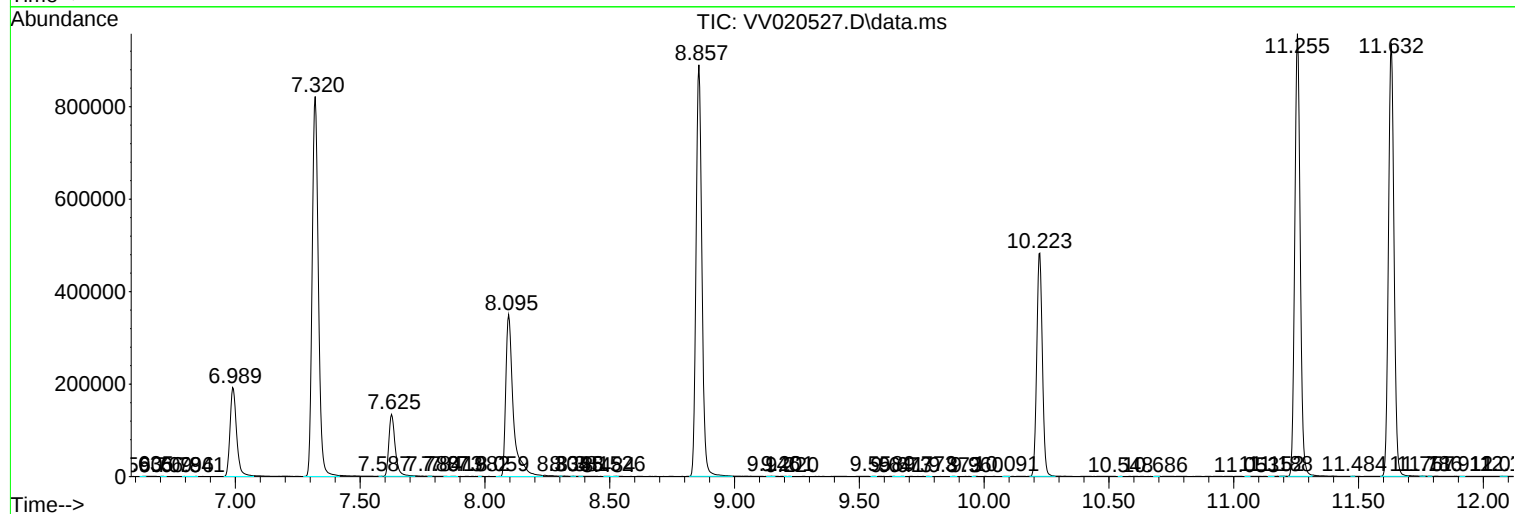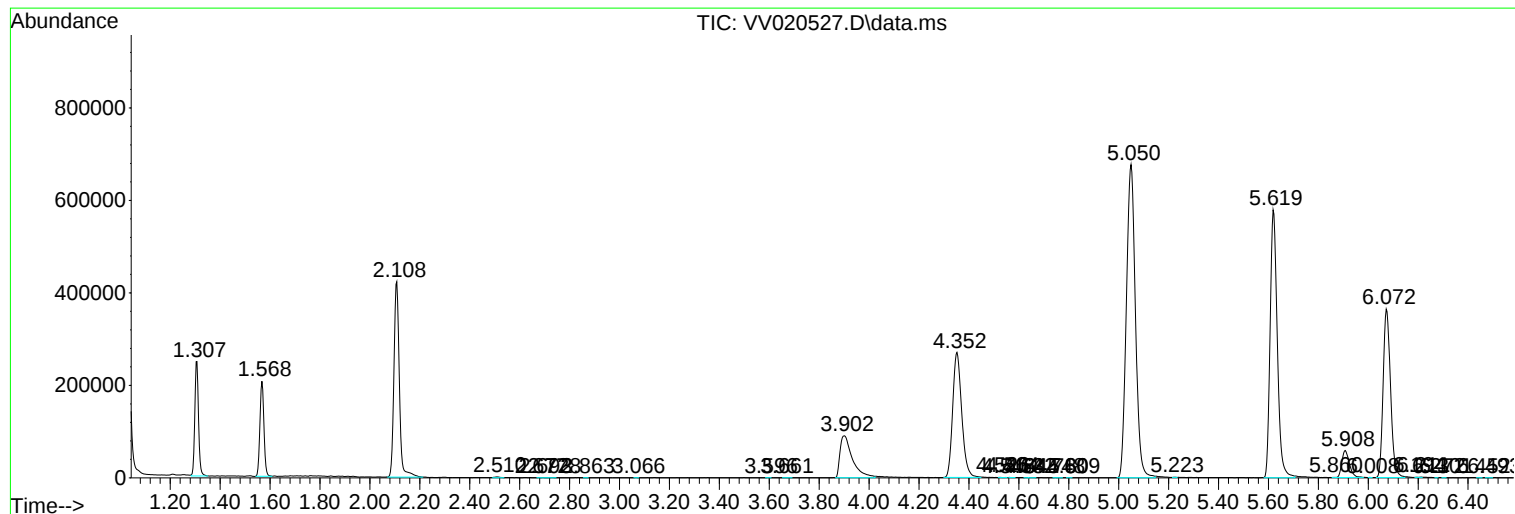

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
Data File : VV020527.D
Acq On : 11 Mar 2021 11:22
Operator : SY/MD
Sample : M1610-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
Data File : VV020527.D
Acq On : 11 Mar 2021 11:22
Operator : SY/MD
Sample : M1610-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
