

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
 Data File : VV020528.D
 Acq On : 11 Mar 2021 11:46
 Operator : SY/MD
 Sample : M1632-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B66

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M

Title : VOC Analysis

Signal : TIC: VV020528.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	101	rVB	305289	307269	16.22%	2.104%
2	1.568	157	164	177	rVB	226594	255890	13.50%	1.752%
3	2.108	321	332	366	rBV	491787	737866	38.94%	5.053%
4	2.262	377	380	383	rVB2	369	211	0.01%	0.001%
5	2.301	384	392	399	rVB3	673	1127	0.06%	0.008%
6	2.359	407	410	412	rBV2	304	245	0.01%	0.002%
7	2.455	436	440	442	rBV2	455	319	0.02%	0.002%
8	2.510	451	457	463	rVB6	990	1310	0.07%	0.009%
9	2.587	478	481	483	rBV2	213	154	0.01%	0.001%
10	2.880	569	572	579	rBV2	200	223	0.01%	0.002%
11	3.163	655	660	662	rBV	207	179	0.01%	0.001%
12	3.195	664	670	675	rBV2	206	268	0.01%	0.002%
13	3.288	695	699	708	rVB2	257	305	0.02%	0.002%
14	3.478	756	758	762	rVV	234	146	0.01%	0.001%
15	3.574	784	788	793	rVB2	216	221	0.01%	0.002%
16	3.603	793	797	800	rBV	215	160	0.01%	0.001%
17	3.780	849	852	855	rVB2	230	164	0.01%	0.001%
18	3.899	878	889	936	rBV	102088	344268	18.17%	2.358%
19	4.169	971	973	980	rVB4	410	385	0.02%	0.003%
20	4.352	1013	1030	1061	rBV	300864	755593	39.88%	5.175%
21	4.574	1096	1099	1102	rBV3	283	212	0.01%	0.001%
22	4.597	1104	1106	1108	rBV2	318	158	0.01%	0.001%
23	4.703	1136	1139	1144	rBV3	307	259	0.01%	0.002%
24	4.728	1144	1147	1151	rVB4	321	198	0.01%	0.001%
25	4.802	1167	1170	1175	rBV3	265	215	0.01%	0.001%
26	4.873	1188	1192	1198	rVB2	252	232	0.01%	0.002%
27	5.050	1226	1247	1286	rBV2	744532	1894811	100.00%	12.977%
28	5.426	1361	1364	1367	rBV2	285	166	0.01%	0.001%
29	5.481	1379	1381	1385	rVV2	529	284	0.01%	0.002%
30	5.503	1385	1388	1391	rVV3	268	175	0.01%	0.001%
31	5.619	1412	1424	1453	rBV	555049	1115811	58.89%	7.642%
32	5.786	1474	1476	1483	rVB3	550	334	0.02%	0.002%
33	5.857	1495	1498	1500	rBV2	309	208	0.01%	0.001%
34	5.912	1502	1515	1539	rVV4	72106	165443	8.73%	1.133%
35	6.072	1551	1565	1597	rBV	395998	810741	42.79%	5.552%
36	6.217	1605	1610	1612	rBV4	797	839	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
 Data File : VV020528.D
 Acq On : 11 Mar 2021 11:46
 Operator : SY/MD
 Sample : M1632-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B66

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
 Title : VOC Analysis

37	6.333	1643	1646	1648	rBV	318	160	0.01%	0.001%
38	6.606	1727	1731	1737	rBV2	170	246	0.01%	0.002%
39	6.642	1737	1742	1744	rBV2	170	146	0.01%	0.001%
40	6.703	1757	1761	1764	rBV2	272	230	0.01%	0.002%
41	6.989	1837	1850	1879	rBV	205980	376428	19.87%	2.578%
42	7.230	1922	1925	1929	rBV2	212	206	0.01%	0.001%
43	7.262	1933	1935	1937	rVB	325	152	0.01%	0.001%
44	7.320	1937	1953	1983	rBV	938686	1611906	85.07%	11.039%
45	7.625	2037	2048	2074	rBV	148226	254359	13.42%	1.742%
46	7.822	2104	2109	2114	rBV3	223	188	0.01%	0.001%
47	7.863	2120	2122	2128	rVB	378	208	0.01%	0.001%
48	7.892	2128	2131	2136	rBV2	281	250	0.01%	0.002%
49	7.944	2138	2147	2150	rBV3	1273	1650	0.09%	0.011%
50	7.989	2157	2161	2164	rVB3	621	517	0.03%	0.004%
51	8.095	2183	2194	2235	rBV2	387919	782625	41.30%	5.360%
52	8.436	2298	2300	2305	rVB2	246	178	0.01%	0.001%
53	8.461	2305	2308	2313	rBV3	191	192	0.01%	0.001%
54	8.661	2368	2370	2376	rVB2	228	145	0.01%	0.001%
55	8.719	2382	2388	2390	rBV	186	170	0.01%	0.001%
56	8.857	2419	2431	2463	rBV	849206	1391044	73.41%	9.527%
57	9.066	2494	2496	2501	rVB3	201	147	0.01%	0.001%
58	9.121	2508	2513	2515	rBV2	398	326	0.02%	0.002%
59	9.239	2545	2550	2555	rVV2	181	203	0.01%	0.001%
60	9.268	2555	2559	2562	rVV2	163	162	0.01%	0.001%
61	9.551	2642	2647	2648	rBV	277	220	0.01%	0.002%
62	9.564	2649	2651	2655	rVB2	346	189	0.01%	0.001%
63	9.686	2683	2689	2691	rBV	219	230	0.01%	0.002%
64	9.735	2702	2704	2710	rVB2	239	207	0.01%	0.001%
65	9.789	2717	2721	2724	rBV2	293	246	0.01%	0.002%
66	9.809	2724	2727	2730	rVB	238	164	0.01%	0.001%
67	10.220	2843	2855	2883	rBV	530054	826185	43.60%	5.658%
68	10.387	2897	2907	2918	rBV3	1976	3436	0.18%	0.024%
69	10.583	2962	2968	2973	rBV2	239	348	0.02%	0.002%
70	10.609	2973	2976	2981	rVB2	214	171	0.01%	0.001%
71	10.699	3001	3004	3011	rBV2	212	258	0.01%	0.002%
72	10.735	3011	3015	3019	rBV2	193	170	0.01%	0.001%
73	10.831	3043	3045	3052	rVB2	239	213	0.01%	0.001%
74	11.198	3156	3159	3165	rVB4	314	279	0.01%	0.002%
75	11.255	3165	3177	3205	rBV	888487	1365961	72.09%	9.355%
76	11.442	3232	3235	3238	rBV2	384	220	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
 Data File : VV020528.D
 Acq On : 11 Mar 2021 11:46
 Operator : SY/MD
 Sample : M1632-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B66

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M

Title : VOC Analysis

77	11.461	3239	3241	3246	rVB3	496	319	0.02%	0.002%
78	11.490	3246	3250	3252	rBV2	326	261	0.01%	0.002%
79	11.632	3280	3294	3311	rBV	1016483	1578178	83.29%	10.808%
80	11.754	3329	3332	3336	rVB3	513	334	0.02%	0.002%
81	11.796	3343	3345	3348	rVB2	410	182	0.01%	0.001%
82	12.320	3505	3508	3510	rBV	229	143	0.01%	0.001%
83	12.397	3529	3532	3538	rVB2	306	309	0.02%	0.002%
84	12.529	3570	3573	3580	rVV	292	292	0.02%	0.002%
85	12.558	3580	3582	3588	rVB	265	181	0.01%	0.001%
86	12.670	3610	3617	3620	rBV3	652	663	0.03%	0.005%
87	12.706	3625	3628	3633	rBV	313	282	0.01%	0.002%
88	12.776	3647	3650	3654	rBV2	296	160	0.01%	0.001%
89	12.799	3655	3657	3663	rVB2	225	212	0.01%	0.001%
90	12.866	3675	3678	3682	rBV2	296	312	0.02%	0.002%
91	13.162	3766	3770	3773	rBV2	277	254	0.01%	0.002%
92	13.278	3802	3806	3812	rVB3	750	767	0.04%	0.005%
93	13.304	3812	3814	3817	rBV2	261	181	0.01%	0.001%
94	13.358	3828	3831	3835	rVB2	415	294	0.02%	0.002%
95	13.564	3893	3895	3898	rBV3	254	171	0.01%	0.001%
96	13.680	3928	3931	3933	rBV2	286	208	0.01%	0.001%
97	13.725	3942	3945	3946	rBV	339	196	0.01%	0.001%
98	14.066	4048	4051	4055	rBV	413	286	0.02%	0.002%
99	15.152	4387	4389	4394	rBV2	505	287	0.02%	0.002%
100	15.400	4464	4466	4468	rBV2	465	252	0.01%	0.002%




Sum of corrected areas: 14601448

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
Data File : VV020528.D
Acq On : 11 Mar 2021 11:46
Operator : SY/MD
Sample : M1632-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B66

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

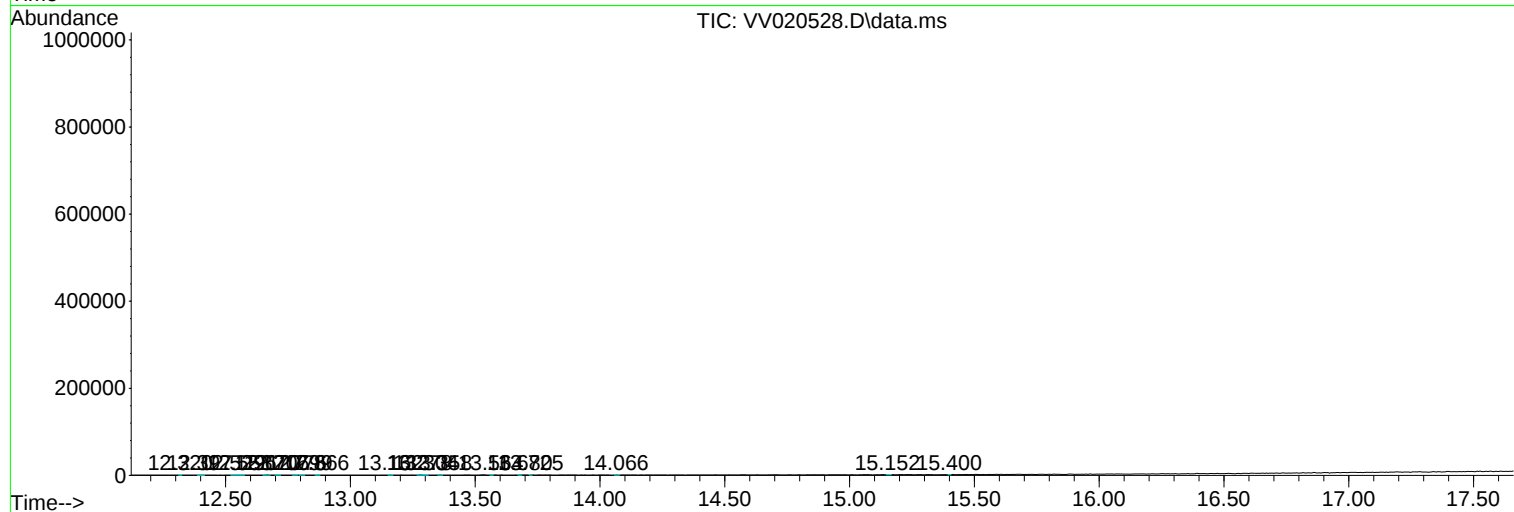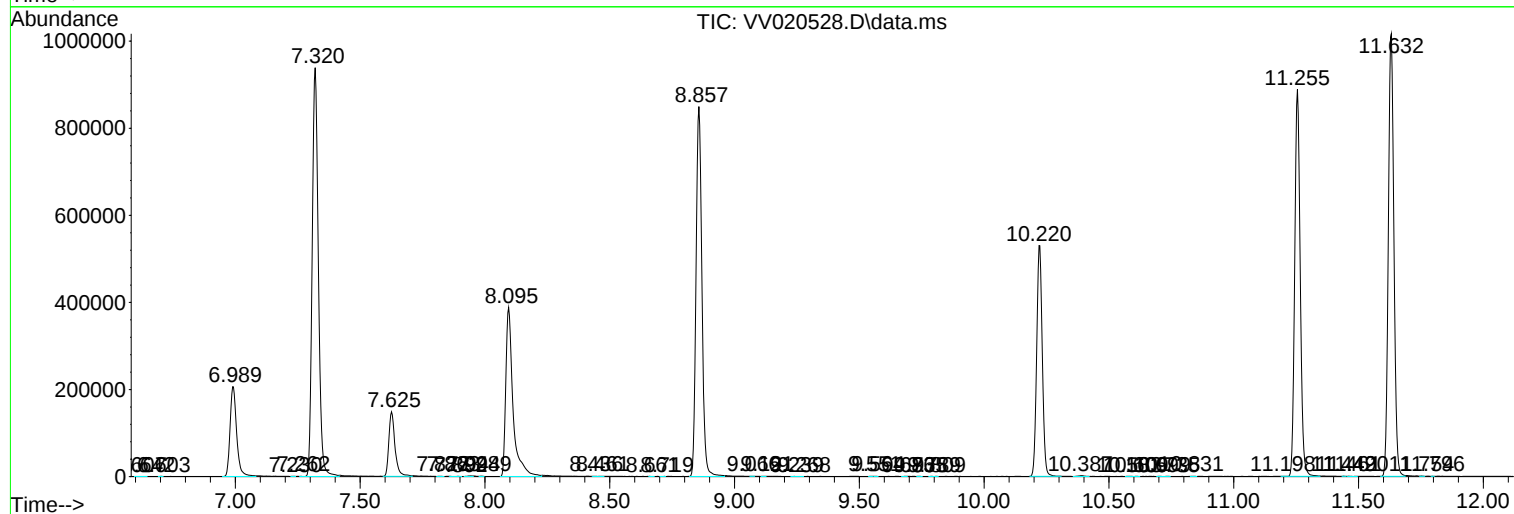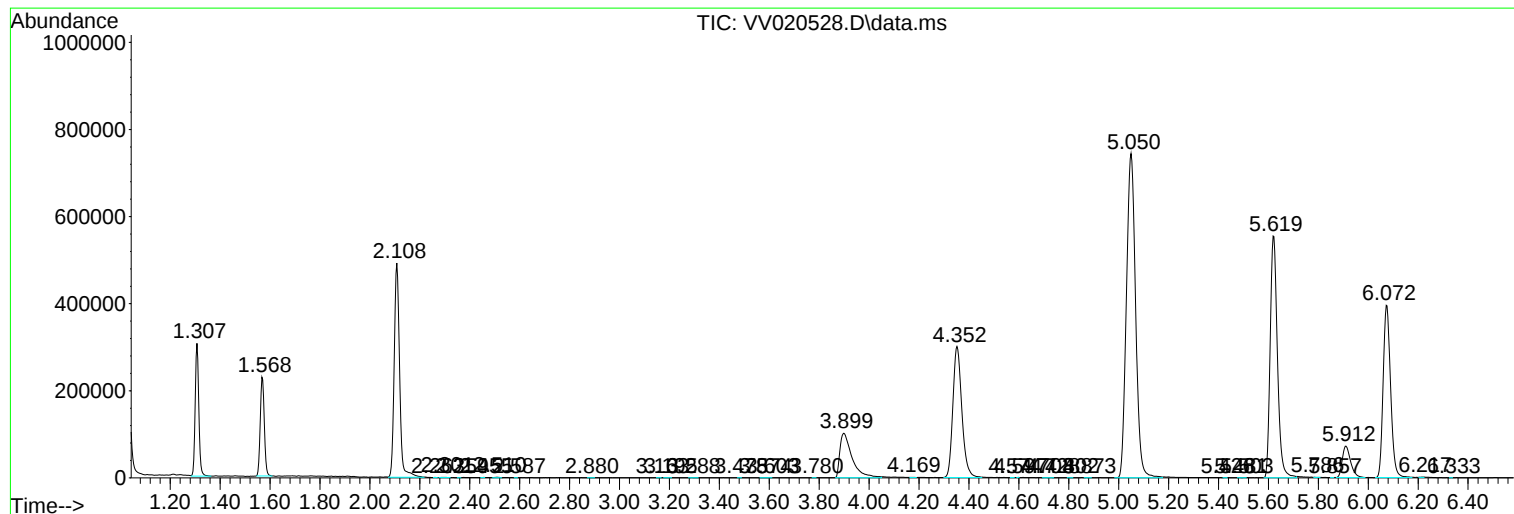

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
Data File : VV020528.D
Acq On : 11 Mar 2021 11:46
Operator : SY/MD
Sample : M1632-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B66

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
Data File : VV020528.D
Acq On : 11 Mar 2021 11:46
Operator : SY/MD
Sample : M1632-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B66

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
