

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
 Data File : VV020529.D
 Acq On : 11 Mar 2021 12:09
 Operator : SY/MD
 Sample : M1632-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B67

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M

Title : VOC Analysis

Signal : TIC: VV020529.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	98	rVB	292322	292953	16.03%	2.061%
2	1.571	157	165	176	rVB	223087	250750	13.72%	1.764%
3	2.108	321	332	345	rBV	477042	687853	37.64%	4.840%
4	2.298	384	391	396	rBV4	620	979	0.05%	0.007%
5	2.320	396	398	404	rVB2	349	256	0.01%	0.002%
6	2.356	404	409	413	rVB3	407	265	0.01%	0.002%
7	2.378	413	416	420	rBV3	374	367	0.02%	0.003%
8	2.404	421	424	429	rVV	378	319	0.02%	0.002%
9	2.455	438	440	443	rBV2	338	196	0.01%	0.001%
10	2.510	451	457	470	rVB6	834	1384	0.08%	0.010%
11	2.603	484	486	489	rBV3	241	157	0.01%	0.001%
12	2.622	489	492	496	rVB2	445	307	0.02%	0.002%
13	2.651	500	501	503	rVB	494	153	0.01%	0.001%
14	2.674	503	508	512	rBV2	185	160	0.01%	0.001%
15	2.892	574	576	581	rVB2	239	138	0.01%	0.001%
16	3.011	609	613	618	rVB2	237	232	0.01%	0.002%
17	3.037	618	621	625	rBV2	154	149	0.01%	0.001%
18	3.407	732	736	739	rBV2	194	164	0.01%	0.001%
19	3.455	746	751	755	rBV2	345	412	0.02%	0.003%
20	3.532	772	775	779	rVV2	215	145	0.01%	0.001%
21	3.741	837	840	844	rVB2	202	151	0.01%	0.001%
22	3.831	864	868	871	rVB	226	149	0.01%	0.001%
23	3.902	878	890	940	rBV2	97773	350175	19.16%	2.464%
24	4.352	1013	1030	1066	rBV	286363	721878	39.50%	5.079%
25	4.581	1100	1101	1108	rVB3	363	196	0.01%	0.001%
26	4.613	1108	1111	1113	rBV	372	222	0.01%	0.002%
27	4.654	1121	1124	1127	rBV3	303	234	0.01%	0.002%
28	4.683	1131	1133	1135	rVV	319	166	0.01%	0.001%
29	4.709	1138	1141	1144	rVV3	456	314	0.02%	0.002%
30	4.745	1148	1152	1158	rVV	266	238	0.01%	0.002%
31	4.831	1176	1179	1184	rVV	255	178	0.01%	0.001%
32	4.883	1194	1195	1200	rVB	356	162	0.01%	0.001%
33	4.931	1207	1210	1216	rVB2	302	223	0.01%	0.002%
34	5.050	1229	1247	1281	rBV2	724964	1827636	100.00%	12.859%
35	5.375	1346	1348	1352	rVB	352	198	0.01%	0.001%
36	5.423	1361	1363	1367	rVB3	305	165	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
 Data File : VV020529.D
 Acq On : 11 Mar 2021 12:09
 Operator : SY/MD
 Sample : M1632-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B67

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
 Title : VOC Analysis

37	5.462	1373	1375	1378	rVB3	346	153	0.01%	0.001%
38	5.484	1378	1382	1385	rBV	567	396	0.02%	0.003%
39	5.500	1385	1387	1390	rVV2	260	162	0.01%	0.001%
40	5.519	1390	1393	1398	rVB3	354	289	0.02%	0.002%

41	5.622	1412	1425	1453	rBV	549966	1104075	60.41%	7.768%
42	5.844	1493	1494	1500	rVB2	464	242	0.01%	0.002%
43	5.908	1500	1514	1541	rVB3	66393	148515	8.13%	1.045%
44	6.072	1548	1565	1587	rBV	384771	781888	42.78%	5.501%
45	6.224	1605	1612	1616	rBV4	801	1097	0.06%	0.008%

46	6.243	1616	1618	1622	rVB4	458	360	0.02%	0.003%
47	6.310	1637	1639	1642	rVB2	362	227	0.01%	0.002%
48	6.330	1642	1645	1647	rBV2	432	246	0.01%	0.002%
49	6.757	1773	1778	1781	rVB2	361	351	0.02%	0.002%
50	6.841	1801	1804	1808	rBV2	138	138	0.01%	0.001%

51	6.989	1839	1850	1871	rBV	197630	360398	19.72%	2.536%
52	7.153	1898	1901	1903	rVB3	340	152	0.01%	0.001%
53	7.217	1917	1921	1925	rBV3	623	605	0.03%	0.004%
54	7.320	1940	1953	1977	rBV	912517	1552923	84.97%	10.926%
55	7.625	2037	2048	2076	rBV	142003	247234	13.53%	1.740%

56	7.754	2086	2088	2092	rVB2	394	236	0.01%	0.002%
57	7.805	2102	2104	2106	rBV	316	170	0.01%	0.001%
58	7.850	2116	2118	2121	rVB2	462	233	0.01%	0.002%
59	7.941	2143	2146	2147	rBV3	654	279	0.02%	0.002%
60	7.989	2157	2161	2164	rVB3	444	352	0.02%	0.002%

61	8.011	2164	2168	2171	rBV2	204	142	0.01%	0.001%
62	8.040	2174	2177	2181	rVB2	367	295	0.02%	0.002%
63	8.095	2184	2194	2227	rBV2	386496	781365	42.75%	5.498%
64	8.577	2341	2344	2348	rBV	319	247	0.01%	0.002%
65	8.680	2373	2376	2383	rBV2	123	142	0.01%	0.001%

66	8.712	2383	2386	2390	rVB	311	194	0.01%	0.001%
67	8.731	2390	2392	2395	rBV2	251	179	0.01%	0.001%
68	8.789	2406	2410	2412	rVB2	256	188	0.01%	0.001%
69	8.857	2418	2431	2463	rBV	859446	1374754	75.22%	9.673%
70	9.056	2490	2493	2494	rBV2	226	149	0.01%	0.001%

71	9.143	2517	2520	2523	rBV2	590	349	0.02%	0.002%
72	9.194	2529	2536	2538	rBV2	248	254	0.01%	0.002%
73	9.214	2538	2542	2544	rBV2	244	158	0.01%	0.001%
74	9.278	2559	2562	2568	rBV2	185	203	0.01%	0.001%
75	9.371	2586	2591	2593	rBV2	242	236	0.01%	0.002%

76	9.545	2642	2645	2650	rBV2	197	151	0.01%	0.001%
----	-------	------	------	------	------	-----	-----	-------	--------

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
 Data File : VV020529.D
 Acq On : 11 Mar 2021 12:09
 Operator : SY/MD
 Sample : M1632-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B67

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
 Title : VOC Analysis

77	9.834	2732	2735	2740	rVB2	165	159	0.01%	0.001%
78	10.223	2842	2856	2878	rBV	514004	808153	44.22%	5.686%
79	10.381	2901	2905	2906	rBV2	833	575	0.03%	0.004%
80	11.021	3100	3104	3106	rVB2	262	177	0.01%	0.001%
81	11.162	3144	3148	3150	rBV3	362	286	0.02%	0.002%
82	11.178	3150	3153	3161	rVB4	549	641	0.04%	0.005%
83	11.255	3165	3177	3205	rBV	897376	1361350	74.49%	9.578%
84	11.426	3227	3230	3231	rBV3	293	184	0.01%	0.001%
85	11.632	3279	3294	3320	rBV	996719	1537094	84.10%	10.815%
86	11.831	3354	3356	3358	rBV2	374	238	0.01%	0.002%
87	11.924	3381	3385	3389	rBV3	303	263	0.01%	0.002%
88	12.265	3487	3491	3493	rBV2	393	249	0.01%	0.002%
89	12.661	3611	3614	3616	rBV	405	175	0.01%	0.001%
90	13.030	3727	3729	3731	rBV2	224	145	0.01%	0.001%
91	13.165	3763	3771	3772	rBV2	382	544	0.03%	0.004%
92	13.278	3802	3806	3808	rBV	498	309	0.02%	0.002%
93	13.567	3893	3896	3898	rVB2	426	236	0.01%	0.002%
94	13.644	3917	3920	3924	rBV3	361	368	0.02%	0.003%
95	13.677	3928	3930	3934	rVB2	377	252	0.01%	0.002%
96	13.744	3948	3951	3952	rBV	335	179	0.01%	0.001%
97	13.837	3977	3980	3983	rBV	339	257	0.01%	0.002%
98	15.101	4369	4373	4380	rBV4	554	518	0.03%	0.004%
99	15.310	4436	4438	4440	rBV2	542	241	0.01%	0.002%
100	15.378	4455	4459	4462	rBV3	1239	932	0.05%	0.007%


Sum of corrected areas: 14212876

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
Data File : VV020529.D
Acq On : 11 Mar 2021 12:09
Operator : SY/MD
Sample : M1632-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B67

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

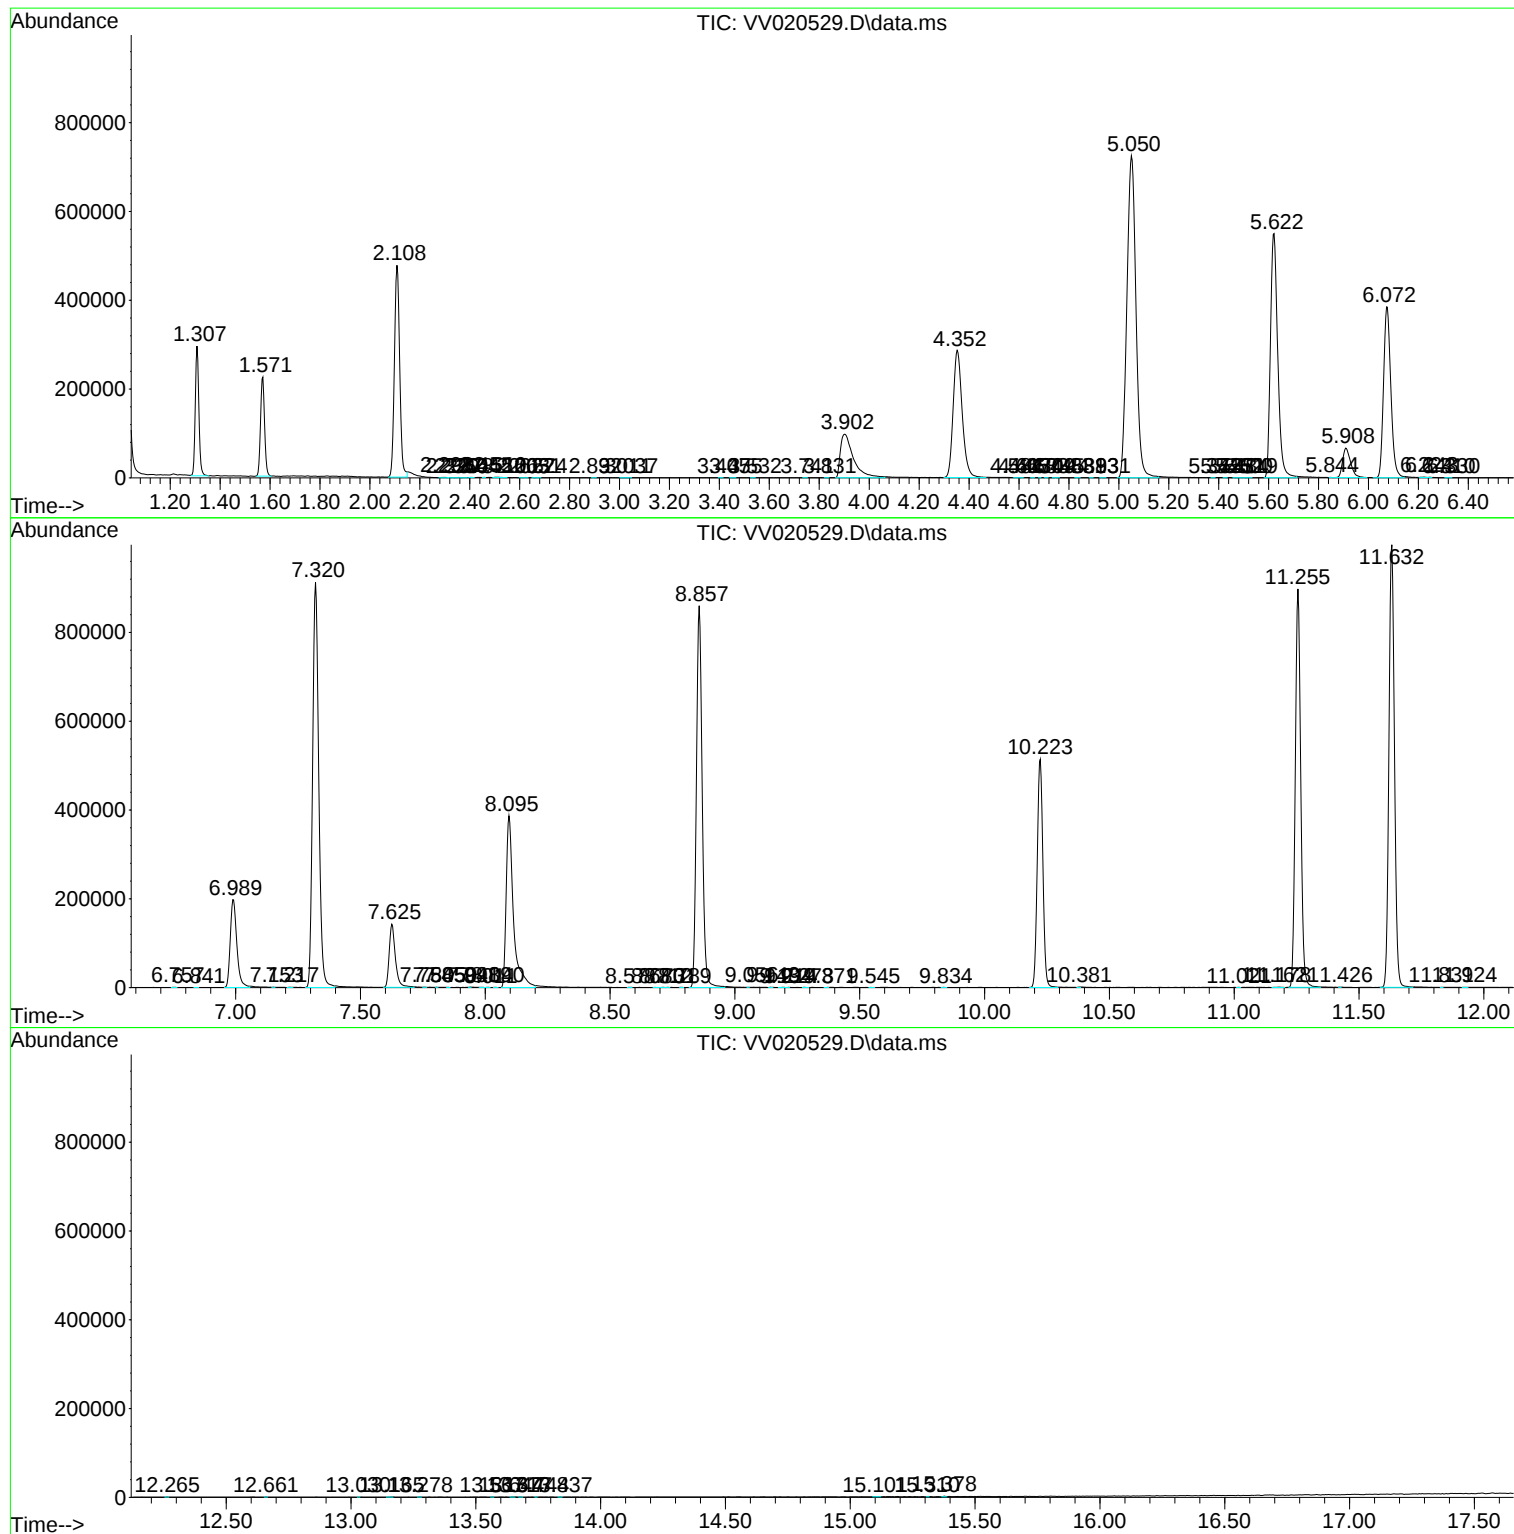

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
Data File : VV020529.D
Acq On : 11 Mar 2021 12:09
Operator : SY/MD
Sample : M1632-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B67

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
Data File : VV020529.D
Acq On : 11 Mar 2021 12:09
Operator : SY/MD
Sample : M1632-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B67

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
