

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
 Data File : VV020531.D
 Acq On : 11 Mar 2021 12:57
 Operator : SY/MD
 Sample : VIBLK70
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK70

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M

Title : VOC Analysis

Signal : TIC: VV020531.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	97	rVB	303177	295656	15.82%	2.014%
2	1.568	156	164	178	rBV	226105	257185	13.76%	1.752%
3	1.992	294	296	299	rVB3	788	378	0.02%	0.003%
4	2.108	321	332	364	rVB	483099	719110	38.48%	4.899%
5	2.294	388	390	395	rVB2	706	505	0.03%	0.003%
6	2.352	405	408	410	rBV	217	142	0.01%	0.001%
7	2.375	412	415	419	rVB	325	211	0.01%	0.001%
8	2.407	421	425	428	rBV2	306	253	0.01%	0.002%
9	2.510	450	457	465	rBV4	2077	3011	0.16%	0.021%
10	2.664	501	505	507	rBV	341	232	0.01%	0.002%
11	2.774	534	539	545	rVB2	208	225	0.01%	0.002%
12	2.844	559	561	565	rVB2	252	153	0.01%	0.001%
13	2.918	582	584	589	rVB	232	150	0.01%	0.001%
14	3.018	612	615	620	rBV	163	140	0.01%	0.001%
15	3.134	647	651	654	rVV2	241	165	0.01%	0.001%
16	3.208	668	674	678	rBV	231	255	0.01%	0.002%
17	3.259	687	690	695	rVB2	182	157	0.01%	0.001%
18	3.536	770	776	780	rBV2	305	453	0.02%	0.003%
19	3.587	789	792	796	rVV2	207	139	0.01%	0.001%
20	3.751	841	843	848	rVB2	474	275	0.01%	0.002%
21	3.780	848	852	854	rBV	319	230	0.01%	0.002%
22	3.899	877	889	932	rBV	108106	355293	19.01%	2.420%
23	4.352	1013	1030	1062	rBV	294659	746407	39.95%	5.085%
24	4.619	1111	1113	1116	rVB2	397	230	0.01%	0.002%
25	4.638	1116	1119	1122	rBV2	412	305	0.02%	0.002%
26	5.050	1229	1247	1272	rBV2	737871	1868561	100.00%	12.730%
27	5.417	1354	1361	1363	rBV3	433	421	0.02%	0.003%
28	5.439	1365	1368	1373	rBV4	288	229	0.01%	0.002%
29	5.510	1387	1390	1392	rVV2	282	163	0.01%	0.001%
30	5.619	1411	1424	1456	rBV	558316	1130622	60.51%	7.702%
31	5.863	1497	1500	1502	rBV3	243	138	0.01%	0.001%
32	5.908	1502	1514	1539	rVV	63059	128945	6.90%	0.878%
33	6.072	1552	1565	1597	rBV	398376	811044	43.40%	5.525%
34	6.227	1606	1613	1617	rBV7	737	1151	0.06%	0.008%
35	6.445	1676	1681	1684	rBV2	251	225	0.01%	0.002%
36	6.513	1698	1702	1705	rBV	172	148	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
 Data File : VV020531.D
 Acq On : 11 Mar 2021 12:57
 Operator : SY/MD
 Sample : VIBLK70
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK70

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
 Title : VOC Analysis

37	6.603	1727	1730	1733	rBV2	277	204	0.01%	0.001%
38	6.670	1750	1751	1755	rVV2	277	140	0.01%	0.001%
39	6.892	1815	1820	1824	rBV2	186	176	0.01%	0.001%
40	6.989	1838	1850	1880	rBV	215267	391829	20.97%	2.669%
41	7.224	1919	1923	1929	rVB3	212	241	0.01%	0.002%
42	7.252	1929	1932	1939	rBV2	319	327	0.02%	0.002%
43	7.320	1939	1953	1979	rBV	937954	1604279	85.86%	10.929%
44	7.625	2037	2048	2073	rBV	153936	267139	14.30%	1.820%
45	7.786	2095	2098	2099	rBV	311	203	0.01%	0.001%
46	7.825	2108	2110	2116	rVB2	314	248	0.01%	0.002%
47	7.857	2116	2120	2129	rVB4	569	586	0.03%	0.004%
48	7.960	2148	2152	2154	rBV2	299	269	0.01%	0.002%
49	7.989	2154	2161	2166	rVV3	1450	1822	0.10%	0.012%
50	8.031	2171	2174	2178	rVB2	230	144	0.01%	0.001%
51	8.053	2178	2181	2183	rBV2	235	152	0.01%	0.001%
52	8.095	2183	2194	2237	rBV2	399874	815763	43.66%	5.557%
53	8.330	2264	2267	2270	rBV3	407	301	0.02%	0.002%
54	8.690	2374	2379	2383	rBV2	145	173	0.01%	0.001%
55	8.731	2388	2392	2395	rVV2	266	205	0.01%	0.001%
56	8.857	2419	2431	2459	rBV	872525	1413805	75.66%	9.632%
57	9.198	2534	2537	2541	rBV2	219	174	0.01%	0.001%
58	9.243	2547	2551	2553	rBV2	252	186	0.01%	0.001%
59	9.349	2581	2584	2592	rVB	272	307	0.02%	0.002%
60	9.397	2592	2599	2603	rBV2	398	430	0.02%	0.003%
61	9.458	2614	2618	2623	rVB2	226	211	0.01%	0.001%
62	9.497	2627	2630	2640	rVB	191	260	0.01%	0.002%
63	9.590	2655	2659	2664	rBV2	195	184	0.01%	0.001%
64	9.841	2734	2737	2741	rBV	246	207	0.01%	0.001%
65	9.921	2758	2762	2764	rBV2	232	188	0.01%	0.001%
66	10.223	2843	2856	2880	rBV	531240	825316	44.17%	5.623%
67	10.378	2902	2904	2910	rBV2	215	142	0.01%	0.001%
68	10.558	2957	2960	2963	rVB3	237	157	0.01%	0.001%
69	10.593	2968	2971	2975	rVV2	224	160	0.01%	0.001%
70	10.616	2976	2978	2982	rVB2	220	151	0.01%	0.001%
71	10.744	3015	3018	3024	rVB2	387	427	0.02%	0.003%
72	10.931	3074	3076	3083	rVB2	228	214	0.01%	0.001%
73	10.966	3083	3087	3092	rBV	284	262	0.01%	0.002%
74	11.075	3118	3121	3129	rVB2	241	261	0.01%	0.002%
75	11.111	3129	3132	3134	rBV2	248	179	0.01%	0.001%
76	11.255	3165	3177	3208	rBV	919786	1421114	76.05%	9.681%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
 Data File : VV020531.D
 Acq On : 11 Mar 2021 12:57
 Operator : SY/MD
 Sample : VIBLK70
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK70

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M

Title : VOC Analysis

77	11.474	3242	3245	3248	rBV2	407	244	0.01%	0.002%
78	11.632	3281	3294	3313	rBV	1037114	1601875	85.73%	10.913%
79	11.854	3361	3363	3367	rBV2	228	172	0.01%	0.001%
80	11.911	3377	3381	3384	rBV3	221	164	0.01%	0.001%
81	11.937	3386	3389	3393	rVV2	193	172	0.01%	0.001%
82	12.091	3435	3437	3439	rVB	437	167	0.01%	0.001%
83	12.140	3449	3452	3457	rVB2	207	145	0.01%	0.001%
84	12.278	3492	3495	3498	rBV	329	245	0.01%	0.002%
85	12.529	3570	3573	3576	rBV	197	150	0.01%	0.001%
86	12.551	3577	3580	3585	rVB2	434	332	0.02%	0.002%
87	12.645	3606	3609	3611	rBV	217	159	0.01%	0.001%
88	12.664	3611	3615	3619	rVV3	620	552	0.03%	0.004%
89	12.738	3636	3638	3641	rVB2	360	153	0.01%	0.001%
90	12.763	3641	3646	3647	rBV	275	196	0.01%	0.001%
91	12.918	3691	3694	3701	rVB3	309	309	0.02%	0.002%
92	12.972	3709	3711	3716	rVB2	317	193	0.01%	0.001%
93	13.001	3716	3720	3723	rBV2	306	260	0.01%	0.002%
94	13.101	3748	3751	3758	rVV3	394	447	0.02%	0.003%
95	13.362	3830	3832	3837	rBV3	208	158	0.01%	0.001%
96	13.513	3876	3879	3882	rVB2	416	244	0.01%	0.002%
97	13.628	3912	3915	3917	rBV	271	171	0.01%	0.001%
98	13.834	3976	3979	3981	rBV2	256	151	0.01%	0.001%
99	14.702	4248	4249	4252	rBV	312	181	0.01%	0.001%
100	15.146	4384	4387	4389	rBV3	606	452	0.02%	0.003%




Sum of corrected areas: 14678735

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
Data File : VV020531.D
Acq On : 11 Mar 2021 12:57
Operator : SY/MD
Sample : VIBLK70
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK70

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

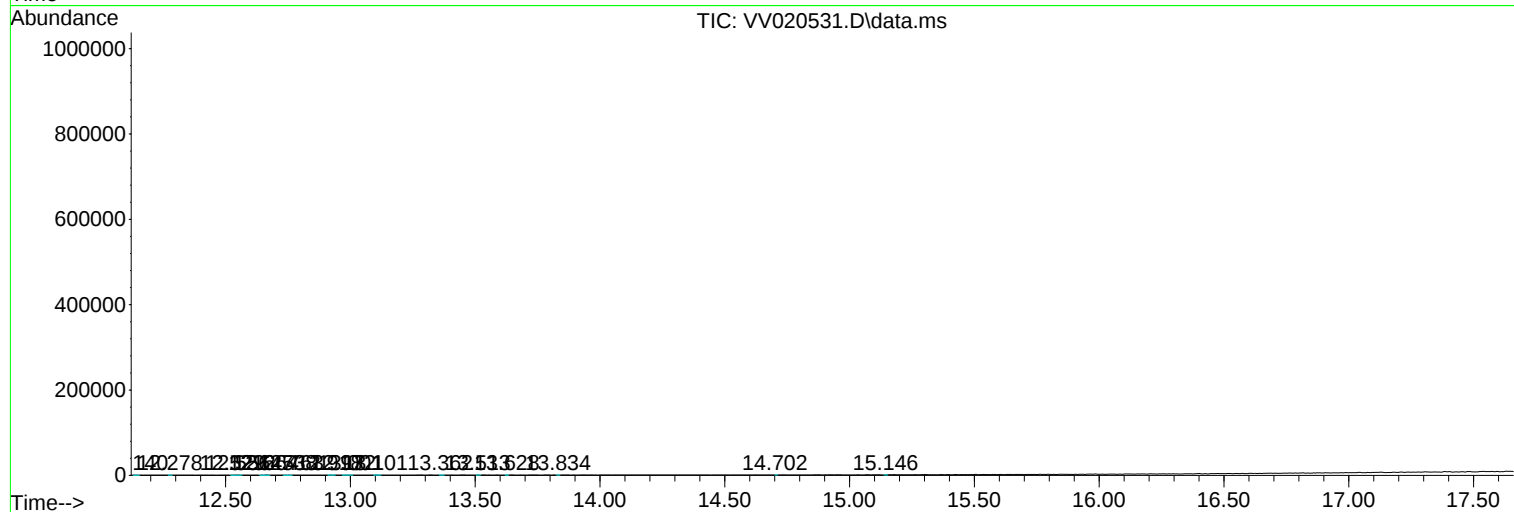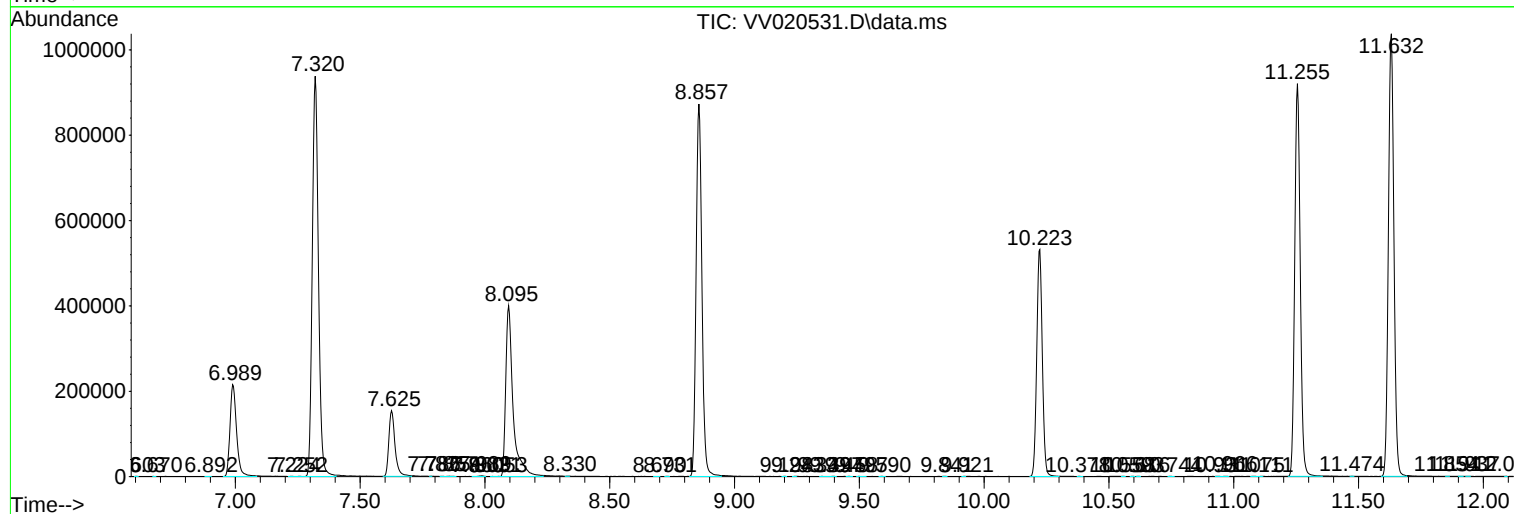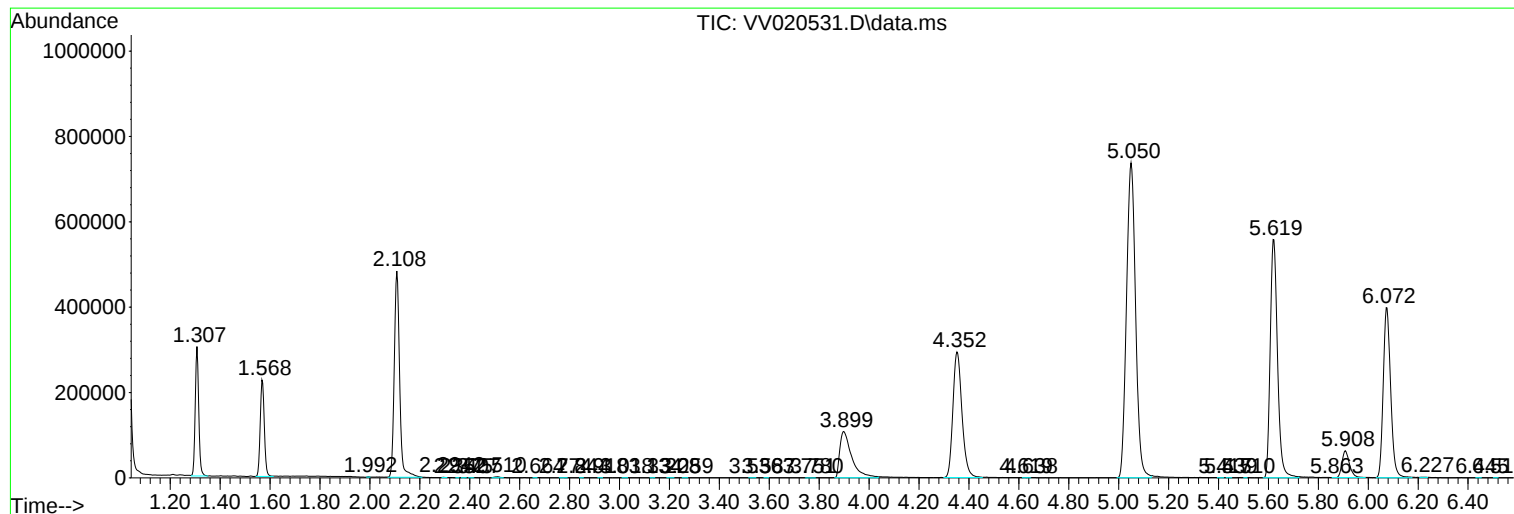

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
Data File : VV020531.D
Acq On : 11 Mar 2021 12:57
Operator : SY/MD
Sample : VIBLK70
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK70

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
Data File : VV020531.D
Acq On : 11 Mar 2021 12:57
Operator : SY/MD
Sample : VIBLK70
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK70

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
