

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
 Data File : VV020541.D
 Acq On : 11 Mar 2021 16:52
 Operator : SY/MD
 Sample : VIBLK72
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK72

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M

Title : VOC Analysis

Signal : TIC: VV020541.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	99	rVB	249096	252225	14.76%	1.787%
2	1.571	157	165	179	rVB	203253	231165	13.53%	1.638%
3	2.108	321	332	374	rVB	423079	641756	37.55%	4.547%
4	2.513	450	458	465	rVV5	1618	2581	0.15%	0.018%
5	2.555	467	471	474	rBV2	276	240	0.01%	0.002%
6	2.728	522	525	527	rBV2	175	131	0.01%	0.001%
7	2.744	528	530	533	rVB2	327	140	0.01%	0.001%
8	2.799	544	547	549	rBV2	331	186	0.01%	0.001%
9	2.867	566	568	571	rBV	252	196	0.01%	0.001%
10	2.969	596	600	604	rBV	223	151	0.01%	0.001%
11	2.992	604	607	612	rVB2	208	150	0.01%	0.001%
12	3.018	612	615	620	rBV	185	192	0.01%	0.001%
13	3.214	673	676	684	rBV2	249	268	0.02%	0.002%
14	3.262	686	691	696	rVV2	205	197	0.01%	0.001%
15	3.336	712	714	718	rVB	227	172	0.01%	0.001%
16	3.445	745	748	751	rBV2	281	267	0.02%	0.002%
17	3.686	820	823	825	rBV	180	146	0.01%	0.001%
18	3.709	825	830	834	rVB2	163	167	0.01%	0.001%
19	3.767	845	848	851	rVB2	250	168	0.01%	0.001%
20	3.828	861	867	874	rVB2	401	541	0.03%	0.004%
21	3.902	879	890	938	rBV	86803	311596	18.23%	2.208%
22	4.352	1012	1030	1066	rBV	270632	684292	40.04%	4.848%
23	4.661	1121	1126	1131	rVB3	452	383	0.02%	0.003%
24	4.699	1135	1138	1142	rVB3	248	179	0.01%	0.001%
25	4.725	1142	1146	1147	rBV3	227	139	0.01%	0.001%
26	5.050	1230	1247	1273	rBV2	681489	1709030	100.00%	12.109%
27	5.384	1349	1351	1354	rVB2	281	136	0.01%	0.001%
28	5.413	1356	1360	1366	rVV4	407	434	0.03%	0.003%
29	5.487	1379	1383	1384	rBV	219	174	0.01%	0.001%
30	5.519	1389	1393	1396	rBV2	236	216	0.01%	0.002%
31	5.622	1408	1425	1454	rBV	615402	1233996	72.20%	8.743%
32	5.908	1501	1514	1541	rVV2	61505	128779	7.54%	0.912%
33	6.072	1552	1565	1590	rBV	364934	741412	43.38%	5.253%
34	6.275	1625	1628	1633	rVB3	498	340	0.02%	0.002%
35	6.297	1633	1635	1637	rVV2	281	164	0.01%	0.001%
36	6.323	1639	1643	1652	rVB3	267	333	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW031221\
 Data File : VW020541.D
 Acq On : 11 Mar 2021 16:52
 Operator : SY/MD
 Sample : VIBLK72
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK72

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
 Title : VOC Analysis

37	6.403	1664	1668	1673	rVB2	256	308	0.02%	0.002%
38	6.429	1673	1676	1680	rVB	251	192	0.01%	0.001%
39	6.452	1680	1683	1686	rBV2	224	212	0.01%	0.002%
40	6.500	1692	1698	1701	rBV2	293	302	0.02%	0.002%
41	6.551	1708	1714	1717	rBV	148	142	0.01%	0.001%
42	6.641	1735	1742	1744	rBV3	844	868	0.05%	0.006%
43	6.709	1760	1763	1765	rBV	222	167	0.01%	0.001%
44	6.847	1803	1806	1812	rBV2	102	134	0.01%	0.001%
45	6.989	1839	1850	1878	rBV	189057	344220	20.14%	2.439%
46	7.191	1909	1913	1914	rBV3	269	178	0.01%	0.001%
47	7.246	1928	1930	1938	rVB3	536	609	0.04%	0.004%
48	7.320	1938	1953	1978	rBV	837959	1445142	84.56%	10.239%
49	7.625	2038	2048	2068	rBV	130773	228859	13.39%	1.622%
50	7.770	2091	2093	2097	rBV2	387	211	0.01%	0.001%
51	7.924	2137	2141	2143	rBV	160	127	0.01%	0.001%
52	7.985	2149	2160	2175	rVB2	14685	25336	1.48%	0.180%
53	8.046	2175	2179	2183	rBV	363	285	0.02%	0.002%
54	8.095	2183	2194	2241	rBV2	344189	712259	41.68%	5.047%
55	8.394	2282	2287	2288	rBV3	319	272	0.02%	0.002%
56	8.448	2301	2304	2307	rVV3	248	183	0.01%	0.001%
57	8.558	2336	2338	2340	rBV	232	131	0.01%	0.001%
58	8.857	2418	2431	2459	rBV	957710	1547203	90.53%	10.963%
59	9.326	2573	2577	2581	rBV2	208	157	0.01%	0.001%
60	9.545	2642	2645	2651	rVV	176	195	0.01%	0.001%
61	9.921	2760	2762	2765	rVB2	258	133	0.01%	0.001%
62	10.124	2822	2825	2828	rVV	198	143	0.01%	0.001%
63	10.223	2843	2856	2878	rBV	486809	755356	44.20%	5.352%
64	10.394	2906	2909	2912	rBV	211	159	0.01%	0.001%
65	10.439	2917	2923	2925	rBV	292	321	0.02%	0.002%
66	10.455	2925	2928	2932	rVB2	288	260	0.02%	0.002%
67	10.490	2932	2939	2944	rBV2	268	438	0.03%	0.003%
68	10.574	2962	2965	2969	rBV2	235	216	0.01%	0.002%
69	10.754	3016	3021	3023	rBV	354	228	0.01%	0.002%
70	10.796	3031	3034	3037	rVB2	290	184	0.01%	0.001%
71	11.075	3118	3121	3127	rVB2	257	235	0.01%	0.002%
72	11.146	3138	3143	3146	rBV2	268	277	0.02%	0.002%
73	11.168	3146	3150	3153	rVV3	444	413	0.02%	0.003%
74	11.181	3153	3154	3160	rVB	473	270	0.02%	0.002%
75	11.255	3165	3177	3200	rBV	1027076	1596294	93.40%	11.310%
76	11.464	3240	3242	3245	rVB3	276	131	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
 Data File : VV020541.D
 Acq On : 11 Mar 2021 16:52
 Operator : SY/MD
 Sample : VIBLK72
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK72

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M

Title : VOC Analysis

77	11.631	3281	3294	3317	rBV	982555	1502923	87.94%	10.649%
78	11.837	3356	3358	3360	rBV	326	142	0.01%	0.001%
79	12.001	3407	3409	3411	rBV	343	165	0.01%	0.001%
80	12.033	3417	3419	3423	rVB2	260	192	0.01%	0.001%
81	12.059	3424	3427	3430	rBV2	231	164	0.01%	0.001%
82	12.156	3454	3457	3459	rBV2	187	143	0.01%	0.001%
83	12.220	3474	3477	3481	rBV	366	193	0.01%	0.001%
84	12.310	3501	3505	3508	rVB	206	127	0.01%	0.001%
85	12.365	3519	3522	3524	rBV2	245	195	0.01%	0.001%
86	12.406	3532	3535	3538	rVB2	370	167	0.01%	0.001%
87	12.519	3568	3570	3575	rVV2	233	184	0.01%	0.001%
88	12.541	3575	3577	3580	rVB	290	149	0.01%	0.001%
89	12.741	3636	3639	3642	rBV2	235	132	0.01%	0.001%
90	12.824	3661	3665	3668	rBV2	272	211	0.01%	0.001%
91	12.869	3676	3679	3682	rVV2	242	151	0.01%	0.001%
92	12.889	3682	3685	3689	rVB2	375	285	0.02%	0.002%
93	12.985	3711	3715	3716	rBV2	317	236	0.01%	0.002%
94	13.056	3733	3737	3739	rBV	309	230	0.01%	0.002%
95	13.252	3795	3798	3803	rVV2	348	253	0.01%	0.002%
96	13.287	3807	3809	3813	rVV	501	386	0.02%	0.003%
97	13.355	3827	3830	3833	rBV3	366	254	0.01%	0.002%
98	13.400	3842	3844	3846	rBV2	262	129	0.01%	0.001%
99	14.548	4198	4201	4205	rBV2	576	441	0.03%	0.003%
100	14.934	4318	4321	4325	rBV4	857	651	0.04%	0.005%


Sum of corrected areas: 14113495

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
Data File : VV020541.D
Acq On : 11 Mar 2021 16:52
Operator : SY/MD
Sample : VIBLK72
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK72

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

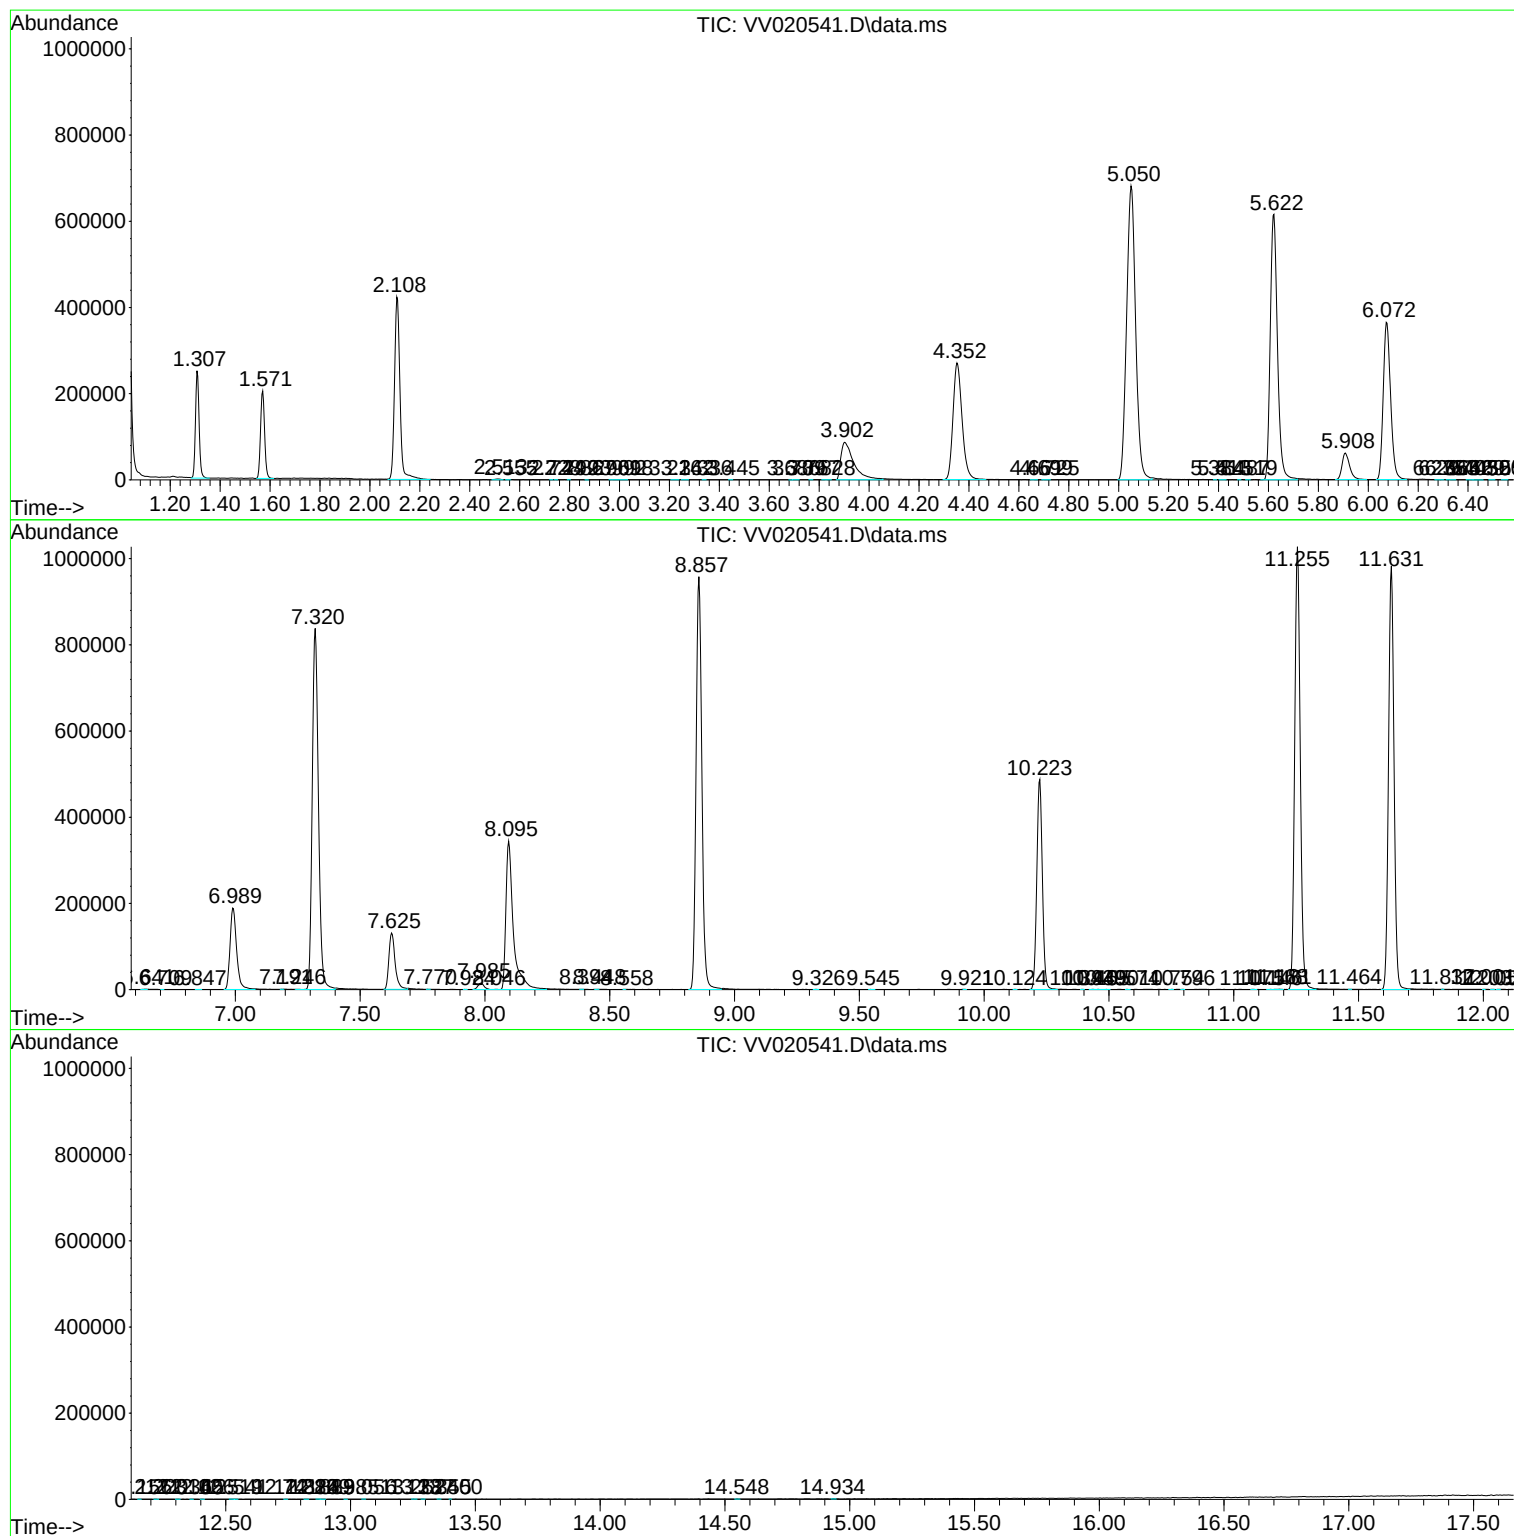

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
Data File : VV020541.D
Acq On : 11 Mar 2021 16:52
Operator : SY/MD
Sample : VIBLK72
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK72

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
Data File : VV020541.D
Acq On : 11 Mar 2021 16:52
Operator : SY/MD
Sample : VIBLK72
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK72

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
