

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
 Data File : VV020543.D
 Acq On : 11 Mar 2021 17:39
 Operator : SY/MD
 Sample : VIBLK73
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK73

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M

Title : VOC Analysis

Signal : TIC: VV020543.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	97	rVB	249627	251589	14.57%	1.802%
2	1.571	157	165	179	rBV	203235	230496	13.35%	1.651%
3	2.056	314	316	320	rBV4	673	359	0.02%	0.003%
4	2.108	321	332	346	rBV	430594	625140	36.19%	4.478%
5	2.356	406	409	412	rVB2	310	207	0.01%	0.001%
6	2.510	451	457	465	rBV4	1297	1883	0.11%	0.013%
7	2.616	488	490	493	rVB2	333	166	0.01%	0.001%
8	2.642	493	498	501	rBV2	200	209	0.01%	0.001%
9	2.664	501	505	508	rVV2	250	207	0.01%	0.001%
10	2.690	508	513	516	rVV2	158	138	0.01%	0.001%
11	2.735	523	527	528	rBV2	263	198	0.01%	0.001%
12	2.773	536	539	542	rBV	231	164	0.01%	0.001%
13	2.883	569	573	576	rVV2	243	253	0.01%	0.002%
14	2.909	579	581	587	rVB2	348	250	0.01%	0.002%
15	2.982	602	604	609	rVB2	208	170	0.01%	0.001%
16	3.011	609	613	614	rBV	149	135	0.01%	0.001%
17	3.227	676	680	683	rBV	315	282	0.02%	0.002%
18	3.269	690	693	702	rVB2	211	238	0.01%	0.002%
19	3.654	809	813	816	rVV	147	138	0.01%	0.001%
20	3.908	879	892	940	rBV2	86374	331737	19.21%	2.376%
21	4.246	994	997	1000	rBV2	265	198	0.01%	0.001%
22	4.352	1013	1030	1060	rBV	272348	690924	40.00%	4.950%
23	4.564	1094	1096	1100	rVB2	365	243	0.01%	0.002%
24	4.587	1100	1103	1107	rBV2	544	352	0.02%	0.003%
25	4.667	1125	1128	1135	rVB3	533	501	0.03%	0.004%
26	4.744	1150	1152	1156	rBV	230	146	0.01%	0.001%
27	4.863	1187	1189	1192	rVB2	301	195	0.01%	0.001%
28	4.883	1192	1195	1198	rVB	314	231	0.01%	0.002%
29	4.905	1198	1202	1203	rBV	345	229	0.01%	0.002%
30	5.050	1230	1247	1278	rBV2	681472	1727208	100.00%	12.373%
31	5.400	1353	1356	1366	rVB3	608	743	0.04%	0.005%
32	5.458	1369	1374	1377	rVB2	346	297	0.02%	0.002%
33	5.484	1378	1382	1384	rBV2	181	134	0.01%	0.001%
34	5.500	1384	1387	1390	rVV2	262	217	0.01%	0.002%
35	5.622	1411	1425	1455	rBV	574705	1152970	66.75%	8.260%
36	5.908	1502	1514	1534	rBV	62594	126491	7.32%	0.906%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW031221\
 Data File : VW020543.D
 Acq On : 11 Mar 2021 17:39
 Operator : SY/MD
 Sample : VIBLK73
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK73

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
 Title : VOC Analysis

37	6.008	1542	1545	1547	rBV3	388	276	0.02%	0.002%
38	6.072	1552	1565	1589	rBV	367650	750779	43.47%	5.378%
39	6.217	1608	1610	1617	rBV5	441	453	0.03%	0.003%
40	6.310	1636	1639	1646	rVB2	321	254	0.01%	0.002%
41	6.648	1740	1744	1752	rVB5	670	1013	0.06%	0.007%
42	6.715	1762	1765	1768	rVB2	268	215	0.01%	0.002%
43	6.831	1798	1801	1809	rVB2	178	174	0.01%	0.001%
44	6.934	1831	1833	1836	rBV2	292	241	0.01%	0.002%
45	6.989	1839	1850	1881	rBV	186591	344725	19.96%	2.470%
46	7.162	1901	1904	1905	rBV	259	153	0.01%	0.001%
47	7.320	1941	1953	1987	rVV	839114	1456671	84.34%	10.435%
48	7.625	2037	2048	2076	rBV	133879	235998	13.66%	1.691%
49	7.857	2117	2120	2122	rBV	203	135	0.01%	0.001%
50	7.876	2123	2126	2129	rVB2	441	278	0.02%	0.002%
51	7.982	2152	2159	2170	rVB3	3707	5552	0.32%	0.040%
52	8.095	2183	2194	2239	rBV2	367618	761730	44.10%	5.457%
53	8.339	2268	2270	2273	rVB3	389	245	0.01%	0.002%
54	8.439	2298	2301	2303	rBV	187	138	0.01%	0.001%
55	8.629	2358	2360	2365	rVB3	334	253	0.01%	0.002%
56	8.722	2386	2389	2392	rBV	271	195	0.01%	0.001%
57	8.783	2405	2408	2411	rVB2	211	138	0.01%	0.001%
58	8.857	2419	2431	2462	rBV	895136	1449391	83.92%	10.383%
59	9.153	2520	2523	2524	rBV	254	149	0.01%	0.001%
60	9.256	2552	2555	2558	rBV2	245	142	0.01%	0.001%
61	9.294	2564	2567	2571	rBV2	200	172	0.01%	0.001%
62	9.403	2598	2601	2603	rBV	229	132	0.01%	0.001%
63	9.445	2611	2614	2617	rBV2	160	140	0.01%	0.001%
64	9.632	2669	2672	2674	rBV2	215	150	0.01%	0.001%
65	9.680	2684	2687	2689	rBV	237	176	0.01%	0.001%
66	9.792	2720	2722	2731	rVB2	314	335	0.02%	0.002%
67	9.860	2740	2743	2747	rVB2	263	163	0.01%	0.001%
68	9.899	2752	2755	2760	rVB2	169	156	0.01%	0.001%
69	9.924	2760	2763	2767	rBV2	237	185	0.01%	0.001%
70	10.220	2843	2855	2878	rBV	504970	790332	45.76%	5.662%
71	10.374	2901	2903	2907	rBV2	304	249	0.01%	0.002%
72	10.776	3025	3028	3033	rBV2	163	160	0.01%	0.001%
73	10.847	3048	3050	3052	rBV	256	181	0.01%	0.001%
74	11.050	3109	3113	3114	rBV	268	217	0.01%	0.002%
75	11.153	3142	3145	3149	rBV2	326	239	0.01%	0.002%
76	11.172	3149	3151	3152	rBV	405	189	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
 Data File : VV020543.D
 Acq On : 11 Mar 2021 17:39
 Operator : SY/MD
 Sample : VIBLK73
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK73

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M

Title : VOC Analysis

77	11.255	3164	3177	3202	rBV	965421	1487616	86.13%	10.657%
78	11.481	3245	3247	3250	rBV	286	160	0.01%	0.001%
79	11.632	3281	3294	3317	rBV	970801	1518155	87.90%	10.876%
80	11.805	3346	3348	3350	rBV2	352	140	0.01%	0.001%
81	11.847	3358	3361	3362	rBV2	275	160	0.01%	0.001%
82	11.857	3362	3364	3367	rVB2	301	172	0.01%	0.001%
83	12.091	3434	3437	3441	rBV2	382	269	0.02%	0.002%
84	12.243	3481	3484	3490	rBV2	255	282	0.02%	0.002%
85	12.394	3527	3531	3537	rBV3	272	258	0.01%	0.002%
86	12.435	3541	3544	3547	rBV2	297	184	0.01%	0.001%
87	12.545	3575	3578	3581	rBV	270	207	0.01%	0.001%
88	12.561	3581	3583	3588	rVV2	291	184	0.01%	0.001%
89	12.847	3669	3672	3676	rBV2	252	176	0.01%	0.001%
90	13.085	3743	3746	3750	rVB	279	156	0.01%	0.001%
91	13.188	3775	3778	3782	rBV3	283	230	0.01%	0.002%
92	13.275	3802	3805	3807	rBV	348	251	0.01%	0.002%
93	13.355	3826	3830	3832	rBV2	267	214	0.01%	0.002%
94	13.445	3852	3858	3861	rBV2	313	397	0.02%	0.003%
95	13.673	3927	3929	3935	rBV3	247	149	0.01%	0.001%
96	14.741	4259	4261	4264	rBV2	456	265	0.02%	0.002%
97	14.767	4266	4269	4271	rBV2	706	433	0.03%	0.003%
98	15.085	4366	4368	4371	rBV2	566	378	0.02%	0.003%
99	15.619	4532	4534	4537	rBV2	838	473	0.03%	0.003%
100	15.635	4537	4539	4543	rBV2	874	733	0.04%	0.005%


Sum of corrected areas: 13959154

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
Data File : VV020543.D
Acq On : 11 Mar 2021 17:39
Operator : SY/MD
Sample : VIBLK73
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK73

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

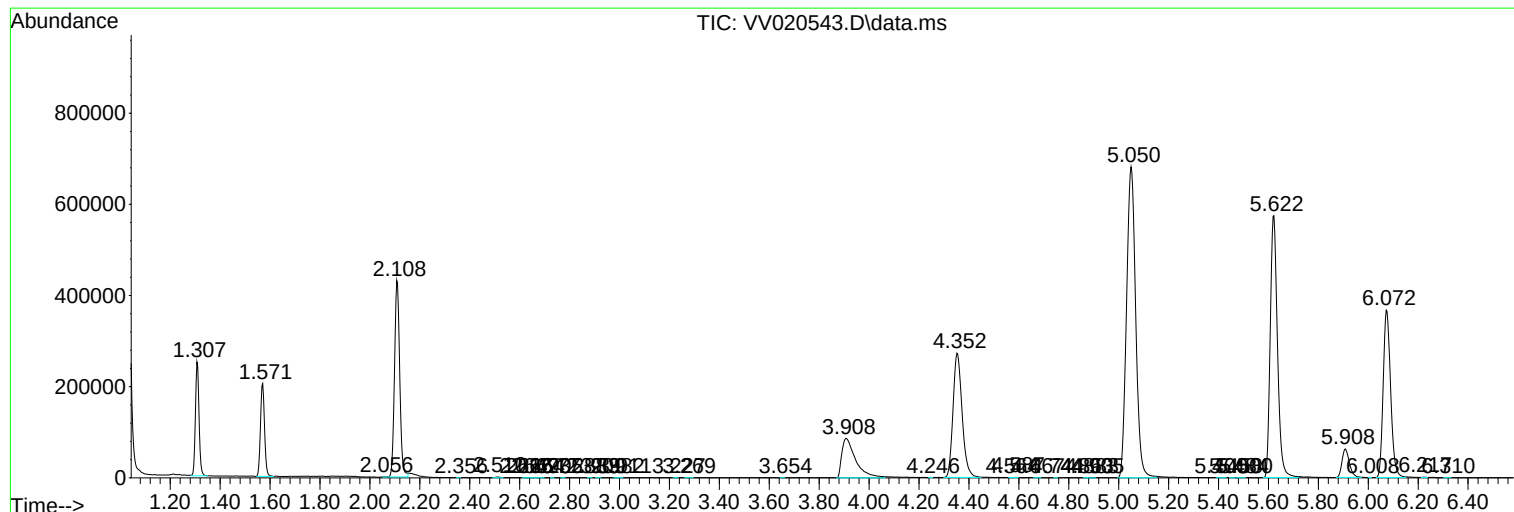

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
Data File : VV020543.D
Acq On : 11 Mar 2021 17:39
Operator : SY/MD
Sample : VIBLK73
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK73

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
Data File : VV020543.D
Acq On : 11 Mar 2021 17:39
Operator : SY/MD
Sample : VIBLK73
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK73

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
