

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
 Data File : VV020545.D
 Acq On : 11 Mar 2021 18:26
 Operator : SY/MD
 Sample : VIBLK74
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK74

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M

Title : VOC Analysis

Signal : TIC: VV020545.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	104	rVB	250887	254617	14.71%	1.826%
2	1.571	157	165	179	rBV	207118	234957	13.57%	1.685%
3	2.108	321	332	345	rBV	432746	625728	36.15%	4.488%
4	2.513	450	458	464	rBV5	1391	2180	0.13%	0.016%
5	2.580	475	479	482	rBV2	183	160	0.01%	0.001%
6	2.613	486	489	497	rVB	258	261	0.02%	0.002%
7	2.683	507	511	515	rBV2	275	158	0.01%	0.001%
8	2.706	515	518	520	rVB2	358	179	0.01%	0.001%
9	2.722	520	523	526	rBV2	286	244	0.01%	0.002%
10	2.889	571	575	579	rBV2	197	156	0.01%	0.001%
11	2.957	593	596	602	rBV2	146	161	0.01%	0.001%
12	3.413	735	738	743	rBV	221	181	0.01%	0.001%
13	3.516	766	770	771	rBV2	232	178	0.01%	0.001%
14	3.638	804	808	812	rVB	256	192	0.01%	0.001%
15	3.777	846	851	853	rBV	202	213	0.01%	0.002%
16	3.809	858	861	865	rVB2	275	225	0.01%	0.002%
17	3.831	865	868	873	rBV2	165	179	0.01%	0.001%
18	3.912	879	893	938	rBV2	81264	320647	18.52%	2.300%
19	4.352	1013	1030	1056	rBV	275657	693430	40.06%	4.973%
20	4.590	1101	1104	1107	rVB3	439	214	0.01%	0.002%
21	4.632	1113	1117	1118	rBV2	239	167	0.01%	0.001%
22	4.712	1139	1142	1145	rVB3	277	193	0.01%	0.001%
23	4.828	1175	1178	1183	rVB3	196	159	0.01%	0.001%
24	4.957	1214	1218	1221	rVV2	218	164	0.01%	0.001%
25	5.050	1227	1247	1280	rBV2	686330	1730938	100.00%	12.415%
26	5.275	1314	1317	1321	rBV3	344	296	0.02%	0.002%
27	5.294	1321	1323	1332	rVB4	378	388	0.02%	0.003%
28	5.368	1343	1346	1349	rBV2	522	314	0.02%	0.002%
29	5.455	1370	1373	1374	rBV	291	161	0.01%	0.001%
30	5.506	1386	1389	1398	rVB3	328	307	0.02%	0.002%
31	5.622	1411	1425	1460	rBV	572977	1144781	66.14%	8.211%
32	5.908	1503	1514	1539	rBV	62154	128802	7.44%	0.924%
33	6.075	1552	1566	1593	rBV	372020	755924	43.67%	5.422%
34	6.227	1603	1613	1614	rBV7	722	1070	0.06%	0.008%
35	6.262	1623	1624	1629	rVB2	490	228	0.01%	0.002%
36	6.310	1637	1639	1644	rBV	223	165	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
 Data File : VV020545.D
 Acq On : 11 Mar 2021 18:26
 Operator : SY/MD
 Sample : VIBLK74
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK74

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
 Title : VOC Analysis

37	6.442	1677	1680	1684	rBV2	219	192	0.01%	0.001%
38	6.654	1736	1746	1754	rBV4	868	1761	0.10%	0.013%
39	6.776	1778	1784	1788	rBV	285	313	0.02%	0.002%
40	6.989	1838	1850	1876	rBV	192079	350963	20.28%	2.517%
41	7.111	1886	1888	1891	rVB3	638	304	0.02%	0.002%
42	7.146	1896	1899	1905	rVB4	380	416	0.02%	0.003%
43	7.175	1905	1908	1912	rBV2	683	480	0.03%	0.003%
44	7.204	1915	1917	1927	rVV4	742	672	0.04%	0.005%
45	7.320	1940	1953	1985	rBV	849444	1467610	84.79%	10.526%
46	7.474	1998	2001	2003	rBV	638	362	0.02%	0.003%
47	7.625	2035	2048	2068	rBV	136153	236803	13.68%	1.698%
48	7.805	2101	2104	2106	rBV2	251	158	0.01%	0.001%
49	7.937	2142	2145	2152	rVB2	244	224	0.01%	0.002%
50	7.982	2152	2159	2168	rBV4	2076	3496	0.20%	0.025%
51	8.095	2184	2194	2244	rBV2	358816	750374	43.35%	5.382%
52	8.394	2283	2287	2288	rBV	245	168	0.01%	0.001%
53	8.497	2317	2319	2325	rVB2	252	196	0.01%	0.001%
54	8.526	2325	2328	2332	rVB	260	165	0.01%	0.001%
55	8.561	2335	2339	2342	rBV	238	176	0.01%	0.001%
56	8.799	2411	2413	2418	rBV	178	155	0.01%	0.001%
57	8.857	2418	2431	2478	rVV	892626	1448323	83.67%	10.388%
58	9.111	2504	2510	2513	rBV3	347	458	0.03%	0.003%
59	9.149	2518	2522	2524	rVV2	269	157	0.01%	0.001%
60	9.259	2553	2556	2563	rVV2	177	198	0.01%	0.001%
61	9.310	2568	2572	2575	rBV2	194	170	0.01%	0.001%
62	9.448	2612	2615	2620	rVB2	183	157	0.01%	0.001%
63	9.808	2724	2727	2732	rBV2	235	193	0.01%	0.001%
64	9.989	2779	2783	2786	rVB2	259	229	0.01%	0.002%
65	10.021	2792	2793	2799	rVB2	246	191	0.01%	0.001%
66	10.072	2804	2809	2811	rBV	178	159	0.01%	0.001%
67	10.223	2843	2856	2878	rBV	496517	780086	45.07%	5.595%
68	10.464	2928	2931	2934	rBV	210	182	0.01%	0.001%
69	10.603	2969	2974	2976	rBV2	228	210	0.01%	0.002%
70	10.657	2986	2991	2998	rBV2	323	420	0.02%	0.003%
71	10.844	3045	3049	3052	rBV2	208	166	0.01%	0.001%
72	10.915	3067	3071	3075	rBV	280	315	0.02%	0.002%
73	10.988	3090	3094	3099	rBV2	157	188	0.01%	0.001%
74	11.178	3149	3153	3155	rBV4	382	299	0.02%	0.002%
75	11.255	3164	3177	3199	rBV	949424	1472338	85.06%	10.560%
76	11.500	3250	3253	3255	rBV	439	215	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW031221\
 Data File : VW020545.D
 Acq On : 11 Mar 2021 18:26
 Operator : SY/MD
 Sample : VIBLK74
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK74

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M

Title : VOC Analysis

77	11.567	3267	3274	3280	rVB2	478	615	0.04%	0.004%
78	11.632	3280	3294	3318	rBV	971960	1517990	87.70%	10.887%
79	11.789	3341	3343	3347	rVB2	368	181	0.01%	0.001%
80	11.812	3347	3350	3355	rVV2	299	263	0.02%	0.002%
81	11.982	3400	3403	3407	rVB2	360	243	0.01%	0.002%
82	12.085	3431	3435	3438	rBV	300	311	0.02%	0.002%
83	12.477	3554	3557	3559	rVV	274	197	0.01%	0.001%
84	12.532	3571	3574	3579	rVB2	311	242	0.01%	0.002%
85	12.644	3605	3609	3612	rBV3	295	240	0.01%	0.002%
86	12.760	3643	3645	3648	rVB	322	162	0.01%	0.001%
87	12.789	3648	3654	3657	rBV3	453	482	0.03%	0.003%
88	12.908	3687	3691	3692	rBV	301	201	0.01%	0.001%
89	12.947	3699	3703	3706	rBV2	273	262	0.02%	0.002%
90	13.050	3732	3735	3739	rBV2	295	292	0.02%	0.002%
91	13.111	3749	3754	3764	rBV3	459	871	0.05%	0.006%
92	13.162	3764	3770	3773	rBV3	410	457	0.03%	0.003%
93	13.226	3788	3790	3794	rVB2	317	162	0.01%	0.001%
94	13.255	3795	3799	3800	rBV2	293	210	0.01%	0.002%
95	13.529	3882	3884	3887	rVB2	421	248	0.01%	0.002%
96	13.789	3961	3965	3966	rBV2	280	210	0.01%	0.002%
97	14.429	4160	4164	4166	rBV2	344	310	0.02%	0.002%
98	14.586	4210	4213	4215	rBV2	335	235	0.01%	0.002%
99	14.702	4245	4249	4252	rBV3	409	270	0.02%	0.002%
100	15.127	4379	4381	4383	rBV2	438	195	0.01%	0.001%




Sum of corrected areas: 13942808

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
Data File : VV020545.D
Acq On : 11 Mar 2021 18:26
Operator : SY/MD
Sample : VIBLK74
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK74

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

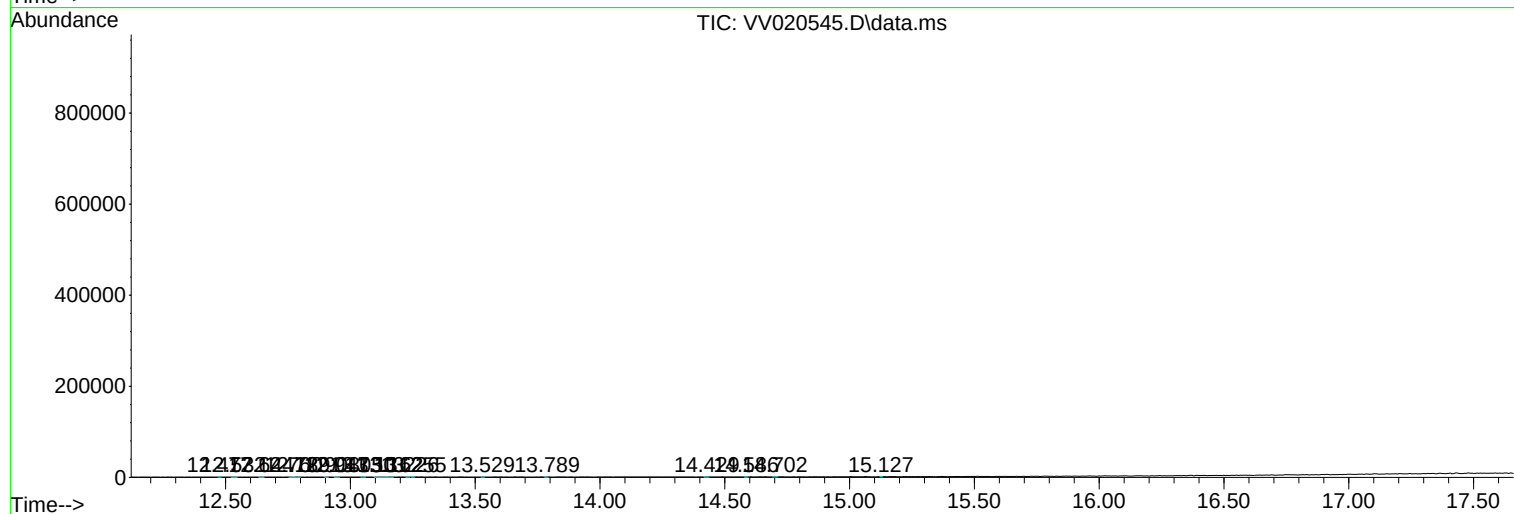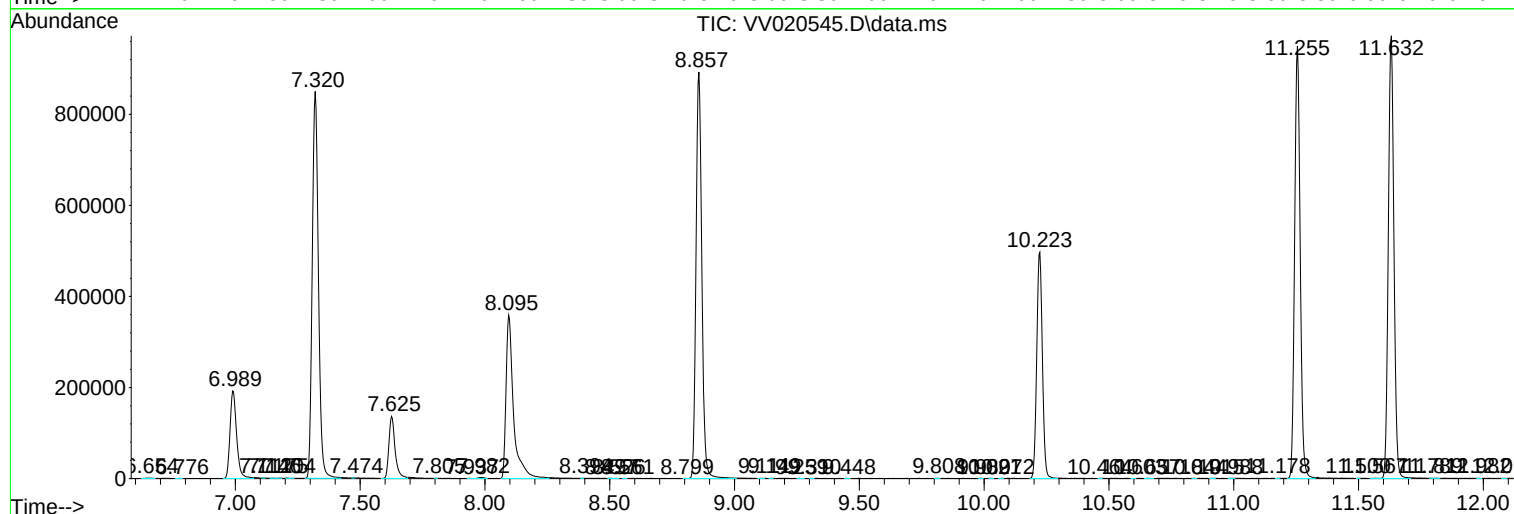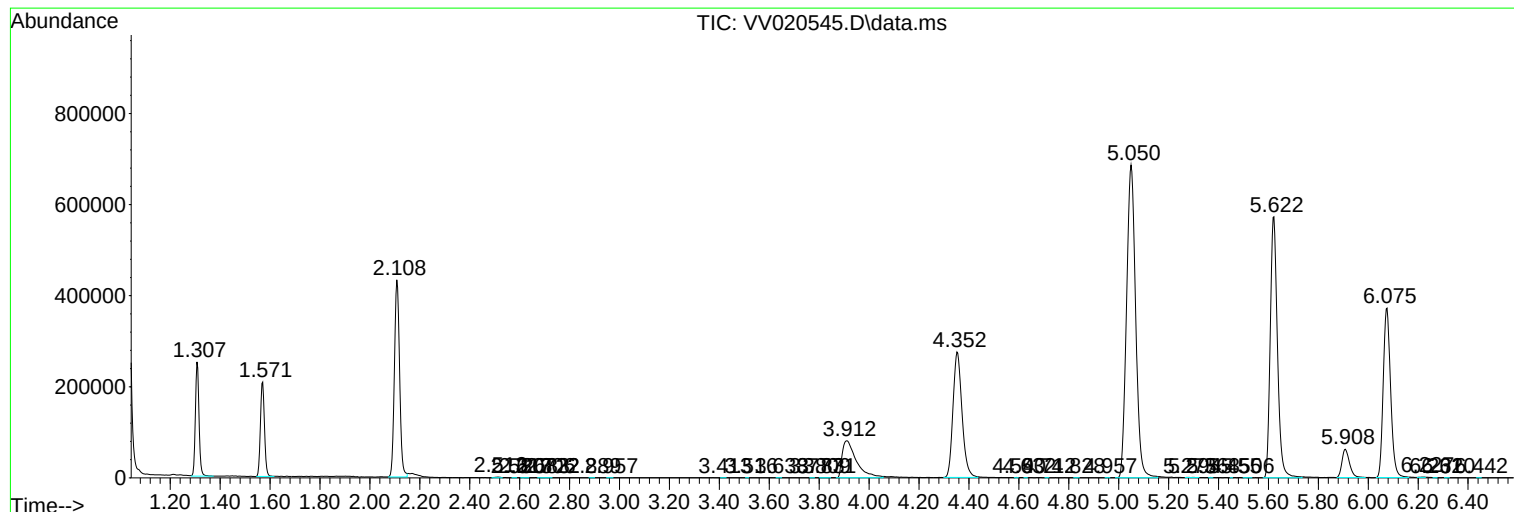

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
Data File : VV020545.D
Acq On : 11 Mar 2021 18:26
Operator : SY/MD
Sample : VIBLK74
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK74

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
Data File : VV020545.D
Acq On : 11 Mar 2021 18:26
Operator : SY/MD
Sample : VIBLK74
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK74

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
