

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
 Data File : VV020547.D
 Acq On : 11 Mar 2021 20:01
 Operator : SY/MD
 Sample : VV0312WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK65

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M

Title : VOC Analysis

Signal : TIC: VV020547.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	98	rVB	240808	245713	14.29%	1.780%
2	1.571	157	165	180	rVB	202318	229793	13.36%	1.665%
3	2.108	321	332	345	rBV	412680	604906	35.18%	4.383%
4	2.294	382	390	399	rVB3	1472	2153	0.13%	0.016%
5	2.365	410	412	418	rVB	339	285	0.02%	0.002%
6	2.513	451	458	468	rVB2	2772	3983	0.23%	0.029%
7	2.561	469	473	475	rBV2	274	217	0.01%	0.002%
8	2.590	480	482	485	rVB	356	185	0.01%	0.001%
9	2.648	498	500	507	rVB2	437	432	0.03%	0.003%
10	2.683	507	511	515	rBV2	433	452	0.03%	0.003%
11	2.812	546	551	553	rBV	245	209	0.01%	0.002%
12	2.857	562	565	568	rBV	234	201	0.01%	0.001%
13	2.873	568	570	574	rVV2	255	222	0.01%	0.002%
14	3.146	652	655	662	rVB2	166	160	0.01%	0.001%
15	3.198	668	671	673	rBV2	247	166	0.01%	0.001%
16	3.423	736	741	745	rBV	242	245	0.01%	0.002%
17	3.452	745	750	754	rVV3	262	214	0.01%	0.002%
18	3.600	793	796	798	rVB	334	171	0.01%	0.001%
19	3.864	874	878	880	rBV2	203	185	0.01%	0.001%
20	3.905	880	891	927	rBV	86686	315600	18.35%	2.287%
21	4.352	1013	1030	1060	rBV2	272828	696276	40.49%	5.045%
22	4.571	1096	1098	1101	rVV3	380	263	0.02%	0.002%
23	4.613	1109	1111	1116	rVB2	309	199	0.01%	0.001%
24	4.638	1116	1119	1123	rBV2	306	282	0.02%	0.002%
25	4.674	1127	1130	1134	rBV3	427	314	0.02%	0.002%
26	4.876	1189	1193	1196	rBV2	202	163	0.01%	0.001%
27	4.921	1201	1207	1210	rBV2	239	256	0.01%	0.002%
28	4.973	1221	1223	1228	rVB2	311	206	0.01%	0.001%
29	5.050	1228	1247	1275	rBV2	674998	1719575	100.00%	12.460%
30	5.365	1342	1345	1347	rBV	293	177	0.01%	0.001%
31	5.513	1387	1391	1396	rBV2	367	305	0.02%	0.002%
32	5.561	1403	1406	1410	rBV3	232	159	0.01%	0.001%
33	5.619	1412	1424	1454	rBV	565837	1136649	66.10%	8.236%
34	5.908	1502	1514	1533	rBV2	58665	120265	6.99%	0.871%
35	6.072	1551	1565	1590	rBV	369834	753429	43.81%	5.459%
36	6.574	1718	1721	1725	rVB2	219	160	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
 Data File : VV020547.D
 Acq On : 11 Mar 2021 20:01
 Operator : SY/MD
 Sample : VV0312WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK65

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
 Title : VOC Analysis

37	6.642	1740	1742	1745	rBV	276	166	0.01%	0.001%
38	6.664	1746	1749	1752	rVB3	473	321	0.02%	0.002%
39	6.728	1767	1769	1771	rVB	317	162	0.01%	0.001%
40	6.918	1824	1828	1833	rVB2	210	192	0.01%	0.001%
41	6.989	1839	1850	1878	rBV	193709	354711	20.63%	2.570%
42	7.320	1941	1953	1980	rBV	824347	1431496	83.25%	10.372%
43	7.625	2038	2048	2076	rBV	138073	243270	14.15%	1.763%
44	7.741	2082	2084	2093	rVB4	702	693	0.04%	0.005%
45	7.796	2099	2101	2105	rVB2	397	260	0.02%	0.002%
46	7.815	2105	2107	2112	rVB2	415	332	0.02%	0.002%
47	7.982	2152	2159	2169	rBV4	1838	2676	0.16%	0.019%
48	8.095	2183	2194	2241	rBV2	353765	734944	42.74%	5.325%
49	8.278	2249	2251	2254	rVB2	844	361	0.02%	0.003%
50	8.410	2287	2292	2295	rBV3	448	393	0.02%	0.003%
51	8.436	2295	2300	2303	rVV3	343	317	0.02%	0.002%
52	8.494	2312	2318	2320	rBV3	230	233	0.01%	0.002%
53	8.535	2328	2331	2335	rBV	190	157	0.01%	0.001%
54	8.619	2355	2357	2365	rVB2	339	256	0.01%	0.002%
55	8.735	2390	2393	2395	rVB2	303	162	0.01%	0.001%
56	8.857	2418	2431	2462	rBV	879005	1419061	82.52%	10.282%
57	9.075	2495	2499	2503	rBV2	327	309	0.02%	0.002%
58	9.104	2506	2508	2515	rBV2	451	572	0.03%	0.004%
59	9.153	2520	2523	2526	rBV2	243	233	0.01%	0.002%
60	9.310	2567	2572	2574	rBV2	321	220	0.01%	0.002%
61	9.423	2602	2607	2610	rBV2	277	273	0.02%	0.002%
62	9.439	2610	2612	2618	rVV2	245	231	0.01%	0.002%
63	9.600	2658	2662	2666	rBV2	264	210	0.01%	0.002%
64	9.725	2699	2701	2709	rBV	313	315	0.02%	0.002%
65	9.815	2724	2729	2735	rBV2	245	294	0.02%	0.002%
66	9.953	2761	2772	2776	rBV3	459	724	0.04%	0.005%
67	10.223	2843	2856	2878	rBV	498374	786943	45.76%	5.702%
68	10.329	2888	2889	2894	rVB	357	154	0.01%	0.001%
69	10.397	2907	2910	2914	rVB3	390	289	0.02%	0.002%
70	10.477	2932	2935	2938	rBV2	272	192	0.01%	0.001%
71	10.548	2952	2957	2960	rBV3	568	594	0.03%	0.004%
72	10.725	3007	3012	3015	rBV2	302	362	0.02%	0.003%
73	10.847	3047	3050	3053	rBV	251	244	0.01%	0.002%
74	10.873	3055	3058	3060	rVV	273	221	0.01%	0.002%
75	10.928	3071	3075	3082	rBV4	635	744	0.04%	0.005%
76	11.034	3104	3108	3115	rVB2	295	338	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
 Data File : VV020547.D
 Acq On : 11 Mar 2021 20:01
 Operator : SY/MD
 Sample : VV0312WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK65

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M

Title : VOC Analysis

77	11.169	3146	3150	3152	rBV3	460	411	0.02%	0.003%
78	11.194	3153	3158	3162	rVV3	1023	989	0.06%	0.007%
79	11.255	3165	3177	3202	rBV	943765	1457667	84.77%	10.562%
80	11.628	3281	3293	3316	rBV	972171	1508741	87.74%	10.932%
81	11.857	3361	3364	3368	rVB4	454	398	0.02%	0.003%
82	11.895	3373	3376	3380	rVB3	436	315	0.02%	0.002%
83	11.918	3380	3383	3386	rBV2	327	282	0.02%	0.002%
84	12.509	3564	3567	3569	rBV	268	166	0.01%	0.001%
85	12.657	3606	3613	3614	rBV3	1567	1422	0.08%	0.010%
86	12.735	3632	3637	3640	rBV3	232	224	0.01%	0.002%
87	12.799	3654	3657	3659	rBV	350	210	0.01%	0.002%
88	12.895	3684	3687	3691	rBV3	253	222	0.01%	0.002%
89	12.972	3708	3711	3718	rBV2	271	305	0.02%	0.002%
90	13.072	3739	3742	3749	rVB2	403	404	0.02%	0.003%
91	13.101	3749	3751	3754	rBV2	355	252	0.01%	0.002%
92	13.146	3762	3765	3770	rBV3	265	244	0.01%	0.002%
93	13.281	3798	3807	3814	rBV6	2060	3264	0.19%	0.024%
94	13.345	3826	3827	3831	rBV2	286	152	0.01%	0.001%
95	13.426	3848	3852	3856	rVB	361	301	0.02%	0.002%
96	13.519	3876	3881	3890	rVB2	2278	2976	0.17%	0.022%
97	13.757	3948	3955	3962	rVB4	2926	3735	0.22%	0.027%
98	14.361	4142	4143	4146	rVB2	462	179	0.01%	0.001%
99	14.683	4240	4243	4246	rBV2	590	356	0.02%	0.003%
100	14.712	4250	4252	4255	rVB	422	190	0.01%	0.001%




Sum of corrected areas: 13801200

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
Data File : VV020547.D
Acq On : 11 Mar 2021 20:01
Operator : SY/MD
Sample : VV0312WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK65

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

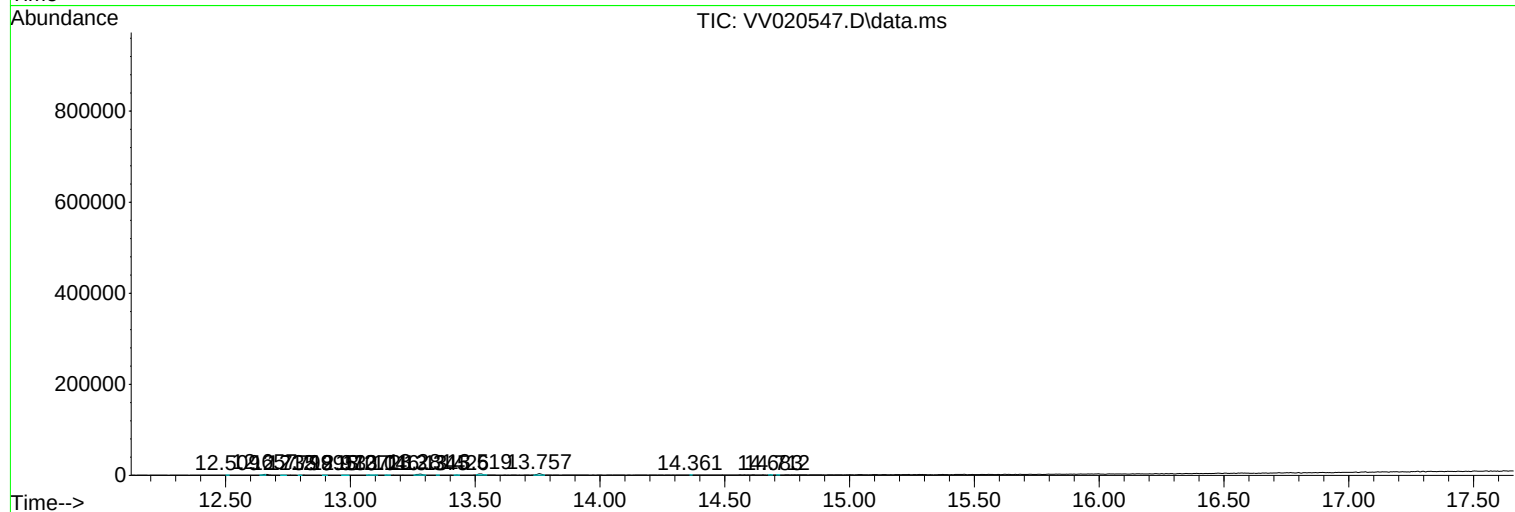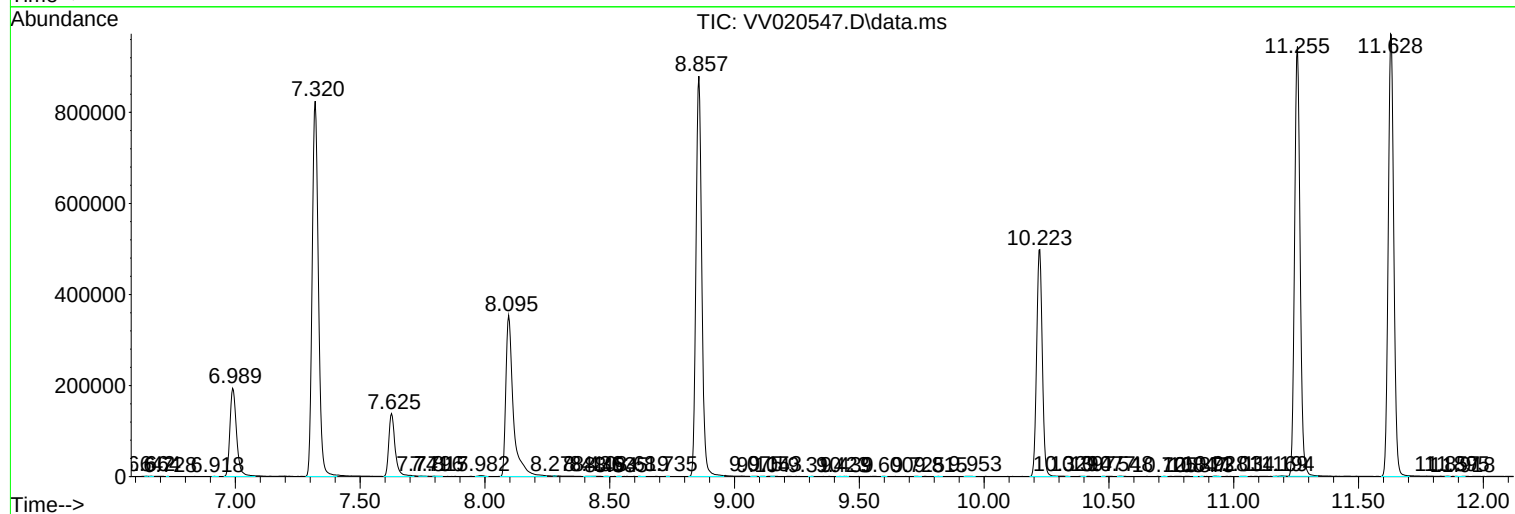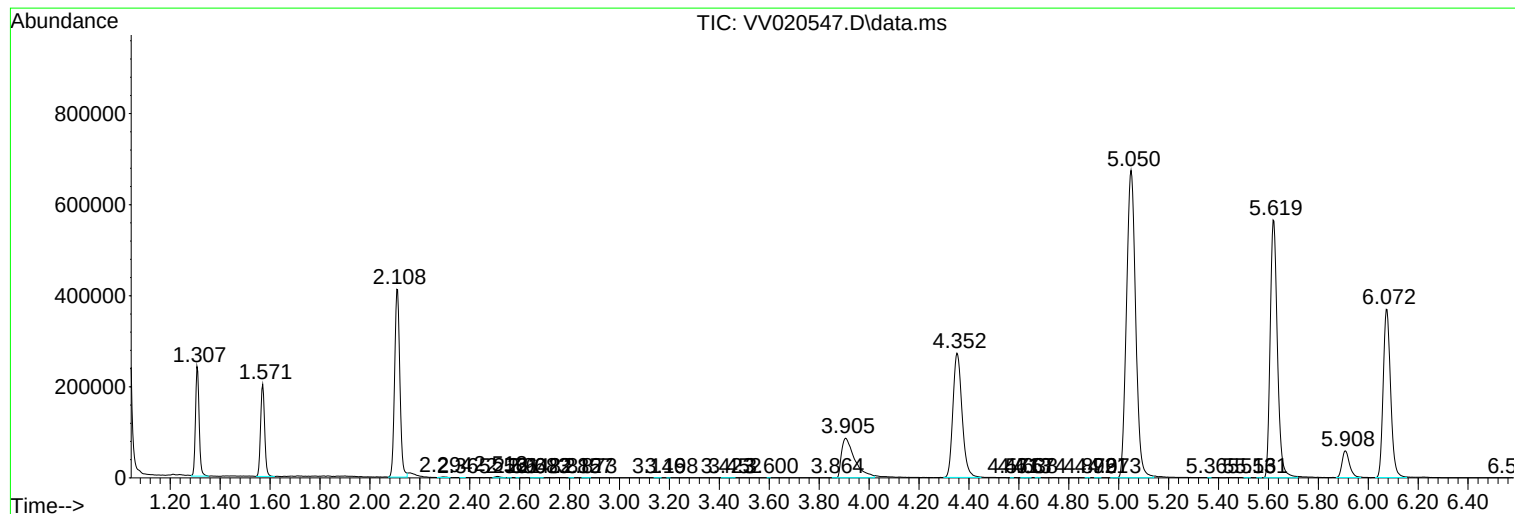

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
Data File : VV020547.D
Acq On : 11 Mar 2021 20:01
Operator : SY/MD
Sample : VV0312WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK65

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
Data File : VV020547.D
Acq On : 11 Mar 2021 20:01
Operator : SY/MD
Sample : VV0312WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK65

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
