

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
 Data File : VV020548.D
 Acq On : 11 Mar 2021 20:24
 Operator : SY/MD
 Sample : M1632-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M

Title : VOC Analysis

Signal : TIC: VV020548.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	101	rVB	240658	246572	14.26%	1.758%
2	1.571	157	165	179	rVB	200237	228404	13.20%	1.628%
3	2.108	321	332	366	rBV	418852	637556	36.86%	4.546%
4	2.246	373	375	377	rBV2	280	169	0.01%	0.001%
5	2.298	385	391	398	rVB3	937	1322	0.08%	0.009%
6	2.359	408	410	415	rVB	298	141	0.01%	0.001%
7	2.388	417	419	426	rVV	218	311	0.02%	0.002%
8	2.510	450	457	469	rVB4	1679	3019	0.17%	0.022%
9	2.558	469	472	474	rBV2	250	194	0.01%	0.001%
10	2.593	480	483	487	rVB2	268	200	0.01%	0.001%
11	2.757	531	534	536	rBV2	215	158	0.01%	0.001%
12	2.815	545	552	555	rBV2	233	270	0.02%	0.002%
13	2.944	588	592	594	rBV2	222	177	0.01%	0.001%
14	3.037	618	621	624	rVB2	345	266	0.02%	0.002%
15	3.056	624	627	630	rBV2	246	235	0.01%	0.002%
16	3.179	661	665	668	rBV	198	175	0.01%	0.001%
17	3.252	684	688	689	rBV	255	171	0.01%	0.001%
18	3.484	755	760	763	rBV2	173	194	0.01%	0.001%
19	3.571	782	787	791	rVB2	272	276	0.02%	0.002%
20	3.596	791	795	796	rBV	204	159	0.01%	0.001%
21	3.661	814	815	819	rVB	229	142	0.01%	0.001%
22	3.780	848	852	858	rVB2	154	176	0.01%	0.001%
23	3.828	864	867	871	rBV2	165	148	0.01%	0.001%
24	3.905	879	891	939	rBV2	90191	326265	18.86%	2.326%
25	4.352	1013	1030	1061	rBV	275660	701390	40.55%	5.001%
26	4.535	1083	1087	1096	rVB4	552	736	0.04%	0.005%
27	4.584	1096	1102	1104	rBV2	363	419	0.02%	0.003%
28	4.613	1107	1111	1112	rBV2	321	269	0.02%	0.002%
29	4.638	1116	1119	1121	rBV	491	304	0.02%	0.002%
30	4.680	1127	1132	1135	rVB3	426	377	0.02%	0.003%
31	4.728	1141	1147	1150	rVB4	524	606	0.04%	0.004%
32	4.744	1150	1152	1153	rBV4	259	133	0.01%	0.001%
33	4.876	1189	1193	1199	rBV	289	339	0.02%	0.002%
34	4.944	1208	1214	1216	rBV2	217	230	0.01%	0.002%
35	5.050	1229	1247	1280	rBV2	680809	1729720	100.00%	12.332%
36	5.407	1355	1358	1362	rBV2	345	298	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
 Data File : VV020548.D
 Acq On : 11 Mar 2021 20:24
 Operator : SY/MD
 Sample : M1632-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
 Title : VOC Analysis

37	5.439	1366	1368	1377	rVB3	418	435	0.03%	0.003%
38	5.477	1377	1380	1383	rBV	357	244	0.01%	0.002%
39	5.500	1383	1387	1393	rVB3	275	291	0.02%	0.002%
40	5.539	1395	1399	1402	rBV3	222	193	0.01%	0.001%

41	5.619	1411	1424	1458	rBV	571882	1151171	66.55%	8.207%
42	5.908	1502	1514	1531	rBV	58756	122002	7.05%	0.870%
43	6.072	1552	1565	1597	rBV	374922	753032	43.53%	5.369%
44	6.474	1685	1690	1691	rBV	190	139	0.01%	0.001%
45	6.513	1698	1702	1707	rVB2	192	178	0.01%	0.001%

46	6.632	1736	1739	1740	rBV	406	151	0.01%	0.001%
47	6.651	1740	1745	1749	rVV3	436	531	0.03%	0.004%
48	6.902	1818	1823	1827	rBV2	193	212	0.01%	0.002%
49	6.989	1839	1850	1879	rBV	191519	354406	20.49%	2.527%
50	7.262	1931	1935	1940	rVB4	455	422	0.02%	0.003%

51	7.320	1940	1953	1979	rBV	851686	1467495	84.84%	10.463%
52	7.625	2037	2048	2074	rBV	136630	239697	13.86%	1.709%
53	7.947	2145	2148	2151	rVB	266	181	0.01%	0.001%
54	7.982	2154	2159	2167	rBV6	1579	2141	0.12%	0.015%
55	8.037	2171	2176	2180	rBV2	219	197	0.01%	0.001%

56	8.095	2184	2194	2233	rBV2	369839	745163	43.08%	5.313%
57	8.516	2322	2325	2328	rBV3	266	214	0.01%	0.002%
58	8.722	2387	2389	2393	rVB2	393	251	0.01%	0.002%
59	8.760	2395	2401	2404	rVB	267	297	0.02%	0.002%
60	8.796	2404	2412	2415	rBV2	323	445	0.03%	0.003%

61	8.857	2416	2431	2462	rBV	908320	1452422	83.97%	10.355%
62	9.079	2496	2500	2503	rBV3	442	398	0.02%	0.003%
63	9.130	2514	2516	2519	rVB2	275	152	0.01%	0.001%
64	9.149	2519	2522	2523	rBV	426	235	0.01%	0.002%
65	9.493	2623	2629	2632	rBV	230	292	0.02%	0.002%

66	9.538	2640	2643	2645	rBV	310	250	0.01%	0.002%
67	9.718	2696	2699	2700	rBV2	225	149	0.01%	0.001%
68	9.751	2705	2709	2712	rVV2	218	210	0.01%	0.001%
69	9.940	2763	2768	2770	rBV2	316	292	0.02%	0.002%
70	10.027	2788	2795	2801	rVB2	282	437	0.03%	0.003%

71	10.062	2801	2806	2814	rBV2	261	453	0.03%	0.003%
72	10.220	2843	2855	2880	rBV	506215	795032	45.96%	5.668%
73	10.432	2916	2921	2925	rBV2	192	250	0.01%	0.002%
74	10.548	2954	2957	2961	rBV	341	250	0.01%	0.002%
75	10.619	2975	2979	2981	rBV2	253	234	0.01%	0.002%

76	10.927	3071	3075	3077	rBV	334	247	0.01%	0.002%
----	--------	------	------	------	-----	-----	-----	-------	--------

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW031221\
 Data File : VW020548.D
 Acq On : 11 Mar 2021 20:24
 Operator : SY/MD
 Sample : M1632-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M

Title : VOC Analysis

77	11.255	3165	3177	3202	rBV	972405	1493535	86.35%	10.648%
78	11.632	3280	3294	3321	rBV	982073	1550697	89.65%	11.056%
79	11.812	3347	3350	3358	rVB4	472	446	0.03%	0.003%
80	11.914	3379	3382	3383	rBV	281	134	0.01%	0.001%
81	11.927	3383	3386	3389	rBV	230	132	0.01%	0.001%
82	12.040	3418	3421	3423	rBV	264	187	0.01%	0.001%
83	12.149	3453	3455	3459	rBV3	266	170	0.01%	0.001%
84	12.329	3510	3511	3521	rVB3	299	296	0.02%	0.002%
85	12.554	3578	3581	3584	rBV	287	255	0.01%	0.002%
86	12.654	3607	3612	3613	rBV2	617	524	0.03%	0.004%
87	12.699	3625	3626	3629	rVB	250	124	0.01%	0.001%
88	12.783	3649	3652	3656	rVB2	290	176	0.01%	0.001%
89	12.818	3658	3663	3668	rVB2	488	461	0.03%	0.003%
90	12.943	3698	3702	3703	rBV2	640	412	0.02%	0.003%
91	13.037	3728	3731	3734	rVB2	317	194	0.01%	0.001%
92	13.120	3751	3757	3763	rBV2	390	604	0.03%	0.004%
93	13.275	3798	3805	3814	rBV5	1111	1869	0.11%	0.013%
94	13.525	3876	3883	3888	rBV2	833	1422	0.08%	0.010%
95	13.570	3894	3897	3902	rBV2	203	178	0.01%	0.001%
96	13.622	3905	3913	3918	rBV3	502	731	0.04%	0.005%
97	13.754	3952	3954	3957	rBV	556	355	0.02%	0.003%
98	13.844	3979	3982	3984	rBV	341	225	0.01%	0.002%
99	13.937	4008	4011	4014	rVV2	366	302	0.02%	0.002%
100	14.178	4083	4086	4089	rBV2	418	317	0.02%	0.002%




Sum of corrected areas: 14026058

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
Data File : VV020548.D
Acq On : 11 Mar 2021 20:24
Operator : SY/MD
Sample : M1632-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

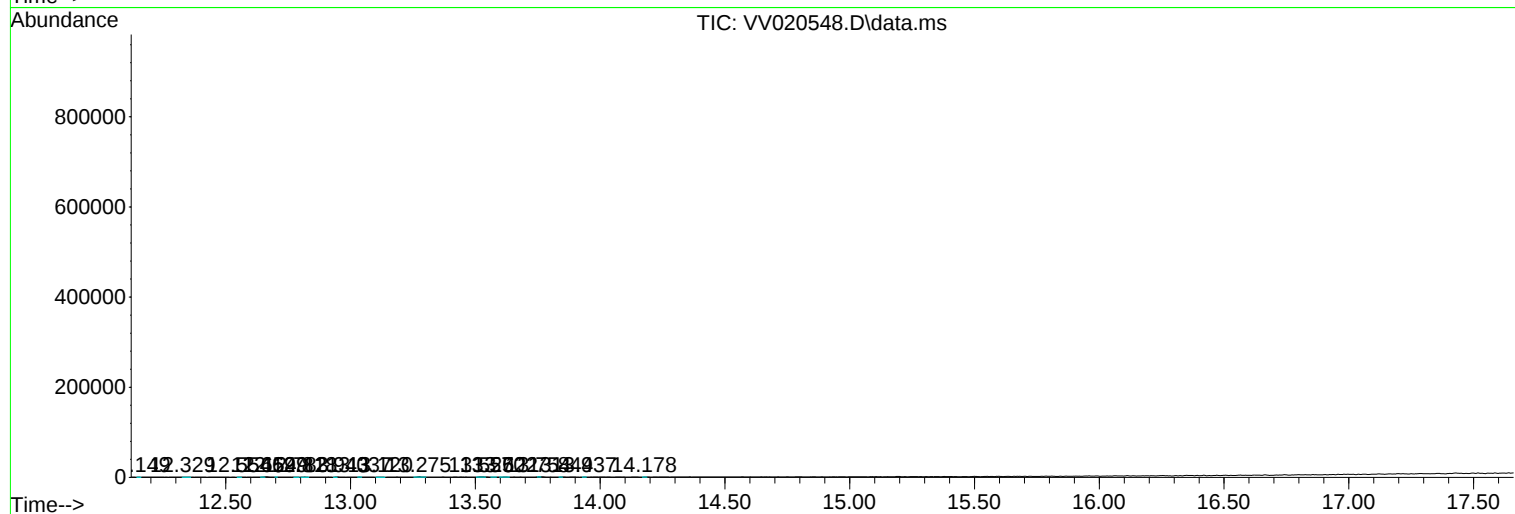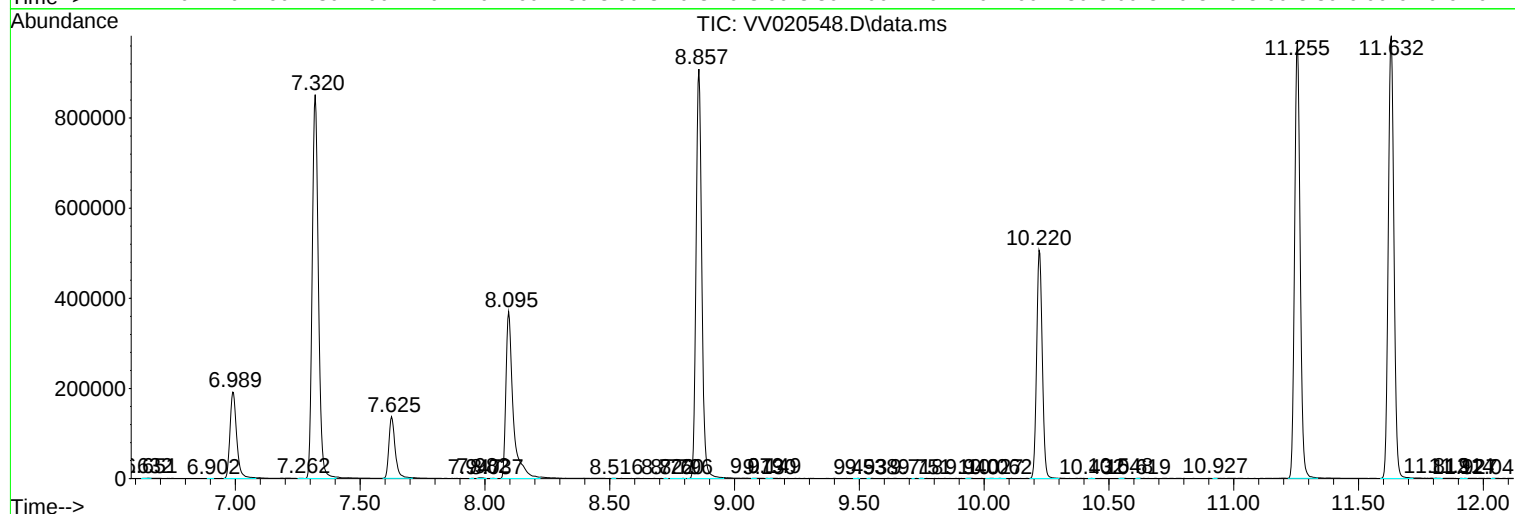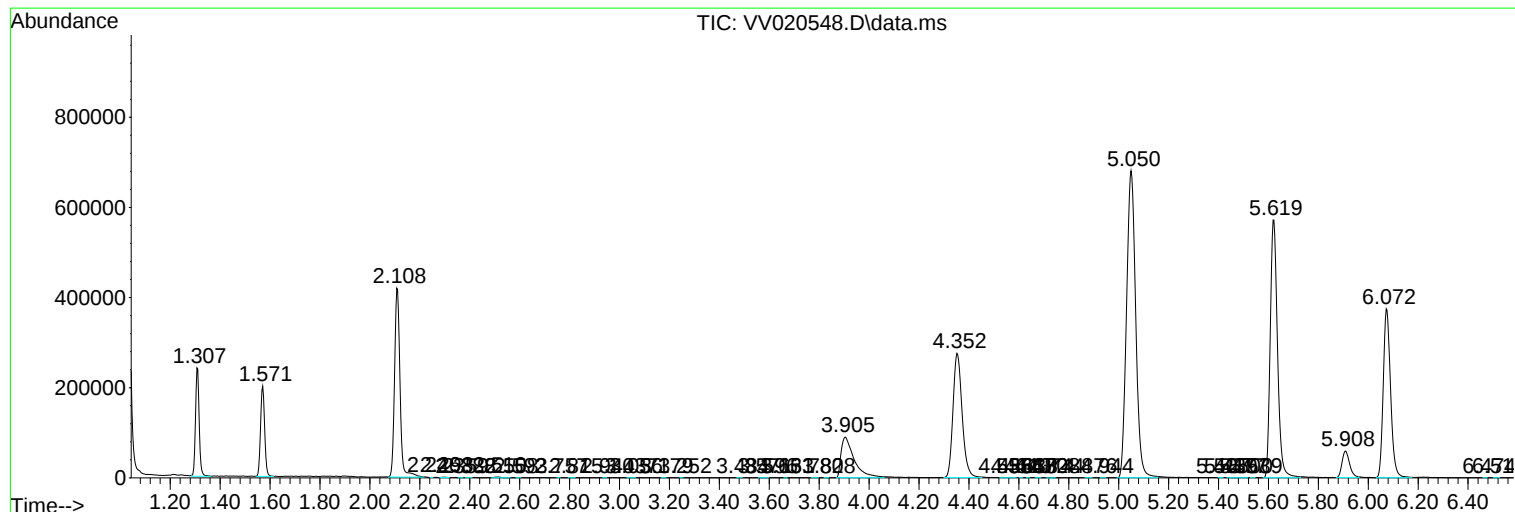

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
Data File : VV020548.D
Acq On : 11 Mar 2021 20:24
Operator : SY/MD
Sample : M1632-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
Data File : VV020548.D
Acq On : 11 Mar 2021 20:24
Operator : SY/MD
Sample : M1632-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
