

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
 Data File : VV020549.D
 Acq On : 11 Mar 2021 20:53
 Operator : SY/MD
 Sample : M1633-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B68

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M

Title : VOC Analysis

Signal : TIC: VV020549.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	100	rVB	273491	277721	15.32%	1.910%
2	1.571	157	165	178	rVB	212430	243342	13.42%	1.673%
3	2.108	321	332	346	rBV	463461	677266	37.35%	4.658%
4	2.294	384	390	397	rBV2	698	947	0.05%	0.007%
5	2.510	451	457	463	rVB4	962	1428	0.08%	0.010%
6	2.596	480	484	487	rBV3	385	333	0.02%	0.002%
7	2.767	535	537	543	rVB2	213	184	0.01%	0.001%
8	2.818	549	553	560	rVV3	288	353	0.02%	0.002%
9	2.950	588	594	597	rBV2	217	282	0.02%	0.002%
10	3.018	612	615	618	rBV	259	195	0.01%	0.001%
11	3.095	636	639	642	rVB2	226	164	0.01%	0.001%
12	3.130	646	650	655	rVV2	175	212	0.01%	0.001%
13	3.268	684	693	694	rBV	317	416	0.02%	0.003%
14	3.391	727	731	736	rVB2	188	180	0.01%	0.001%
15	3.481	756	759	765	rBV	322	384	0.02%	0.003%
16	3.587	788	792	794	rBV	229	201	0.01%	0.001%
17	3.635	805	807	810	rBV2	236	165	0.01%	0.001%
18	3.715	828	832	836	rBV2	254	252	0.01%	0.002%
19	3.741	836	840	846	rVB2	223	324	0.02%	0.002%
20	3.776	846	851	853	rBV	324	293	0.02%	0.002%
21	3.857	869	876	878	rBV2	257	296	0.02%	0.002%
22	3.902	878	890	935	rBV	86872	325265	17.94%	2.237%
23	4.265	1000	1003	1007	rVB2	370	238	0.01%	0.002%
24	4.349	1012	1029	1058	rBV	281382	717620	39.58%	4.935%
25	4.632	1113	1117	1122	rVB3	416	309	0.02%	0.002%
26	4.760	1155	1157	1160	rVV2	277	171	0.01%	0.001%
27	4.899	1195	1200	1203	rVB2	210	193	0.01%	0.001%
28	5.050	1229	1247	1278	rBV2	714876	1813089	100.00%	12.469%
29	5.407	1356	1358	1362	rVB3	484	333	0.02%	0.002%
30	5.432	1362	1366	1369	rBV3	475	371	0.02%	0.003%
31	5.445	1369	1370	1377	rVB	326	180	0.01%	0.001%
32	5.490	1377	1384	1385	rBV3	351	338	0.02%	0.002%
33	5.619	1411	1424	1453	rBV	590688	1174564	64.78%	8.078%
34	5.834	1489	1491	1495	rBV2	513	375	0.02%	0.003%
35	5.905	1501	1513	1544	rBV2	57389	119941	6.62%	0.825%
36	6.072	1551	1565	1598	rBV	383797	784154	43.25%	5.393%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
 Data File : VV020549.D
 Acq On : 11 Mar 2021 20:53
 Operator : SY/MD
 Sample : M1633-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B68

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
 Title : VOC Analysis

37	6.471	1685	1689	1691	rBV	253	190	0.01%	0.001%
38	6.503	1697	1699	1702	rVV	302	163	0.01%	0.001%
39	6.583	1717	1724	1729	rBV2	292	343	0.02%	0.002%
40	6.821	1792	1798	1800	rBV2	216	273	0.02%	0.002%
41	6.902	1815	1823	1826	rBV	186	263	0.01%	0.002%
42	6.989	1838	1850	1876	rBV	205827	378256	20.86%	2.601%
43	7.175	1905	1908	1910	rBV3	271	204	0.01%	0.001%
44	7.204	1913	1917	1921	rVB3	308	295	0.02%	0.002%
45	7.320	1939	1953	1978	rBV	905833	1571974	86.70%	10.811%
46	7.625	2037	2048	2084	rBV	145995	257853	14.22%	1.773%
47	7.857	2116	2120	2121	rBV	625	375	0.02%	0.003%
48	7.899	2129	2133	2136	rVB3	312	283	0.02%	0.002%
49	7.940	2139	2146	2155	rBV4	1410	2167	0.12%	0.015%
50	8.095	2184	2194	2232	rBV2	369697	747653	41.24%	5.142%
51	8.458	2302	2307	2310	rBV2	272	367	0.02%	0.003%
52	8.493	2315	2318	2321	rVB2	263	183	0.01%	0.001%
53	8.770	2399	2404	2408	rBV2	282	347	0.02%	0.002%
54	8.792	2409	2411	2415	rVB2	254	186	0.01%	0.001%
55	8.857	2417	2431	2461	rBV	915019	1479454	81.60%	10.174%
56	9.072	2495	2498	2502	rBV4	259	272	0.02%	0.002%
57	9.091	2502	2504	2506	rVV2	350	181	0.01%	0.001%
58	9.104	2506	2508	2513	rVV2	362	327	0.02%	0.002%
59	9.558	2645	2649	2652	rVB2	301	217	0.01%	0.001%
60	9.882	2748	2750	2759	rBV3	208	258	0.01%	0.002%
61	9.918	2759	2761	2766	rVV2	222	189	0.01%	0.001%
62	9.947	2768	2770	2776	rVB	418	290	0.02%	0.002%
63	10.014	2788	2791	2796	rVB2	227	207	0.01%	0.001%
64	10.050	2796	2802	2805	rBV2	386	419	0.02%	0.003%
65	10.220	2843	2855	2882	rBV	515550	820573	45.26%	5.643%
66	10.390	2898	2908	2917	rBV4	2382	3112	0.17%	0.021%
67	10.435	2918	2922	2926	rVB2	323	284	0.02%	0.002%
68	10.461	2926	2930	2933	rBV	288	230	0.01%	0.002%
69	10.580	2964	2967	2972	rVB2	221	208	0.01%	0.001%
70	10.622	2972	2980	2983	rBV2	323	470	0.03%	0.003%
71	10.731	3009	3014	3019	rBV2	274	310	0.02%	0.002%
72	10.773	3024	3027	3029	rBV2	214	181	0.01%	0.001%
73	10.860	3052	3054	3058	rVB2	448	296	0.02%	0.002%
74	10.937	3075	3078	3081	rVB2	342	222	0.01%	0.002%
75	11.011	3098	3101	3106	rVB2	269	249	0.01%	0.002%
76	11.101	3127	3129	3136	rVB2	338	264	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
 Data File : VV020549.D
 Acq On : 11 Mar 2021 20:53
 Operator : SY/MD
 Sample : M1633-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B68

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
 Title : VOC Analysis

77	11.175	3149	3152	3155	rBV3	305	294	0.02%	0.002%
78	11.255	3165	3177	3201	rBV	985410	1518794	83.77%	10.445%
79	11.554	3267	3270	3272	rBV	284	200	0.01%	0.001%
80	11.631	3280	3294	3317	rBV	1027801	1602321	88.38%	11.019%
81	11.837	3354	3358	3360	rBV3	379	209	0.01%	0.001%
82	11.895	3374	3376	3379	rBV	237	172	0.01%	0.001%
83	12.127	3444	3448	3451	rBV	349	292	0.02%	0.002%
84	12.252	3482	3487	3490	rBV2	274	292	0.02%	0.002%
85	12.368	3519	3523	3526	rVB2	273	240	0.01%	0.002%
86	12.590	3589	3592	3596	rBV2	329	239	0.01%	0.002%
87	12.654	3607	3612	3613	rBV2	636	506	0.03%	0.003%
88	12.815	3659	3662	3667	rVV2	208	209	0.01%	0.001%
89	12.905	3687	3690	3692	rBV2	418	341	0.02%	0.002%
90	13.101	3749	3751	3756	rVB2	412	354	0.02%	0.002%
91	13.133	3756	3761	3763	rBV	342	270	0.01%	0.002%
92	13.236	3788	3793	3798	rBV3	300	334	0.02%	0.002%
93	13.281	3801	3807	3814	rBV4	734	1226	0.07%	0.008%
94	13.445	3853	3858	3861	rBV2	564	512	0.03%	0.004%
95	13.522	3878	3882	3884	rBV	513	446	0.02%	0.003%
96	13.763	3950	3957	3960	rBV3	811	1023	0.06%	0.007%
97	13.892	3995	3997	4000	rVB2	381	211	0.01%	0.001%
98	14.860	4295	4298	4302	rBV2	536	391	0.02%	0.003%
99	15.004	4341	4343	4346	rVB3	604	329	0.02%	0.002%
100	15.561	4514	4516	4517	rBV2	590	268	0.01%	0.002%




Sum of corrected areas: 14541140

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
Data File : VV020549.D
Acq On : 11 Mar 2021 20:53
Operator : SY/MD
Sample : M1633-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B68

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

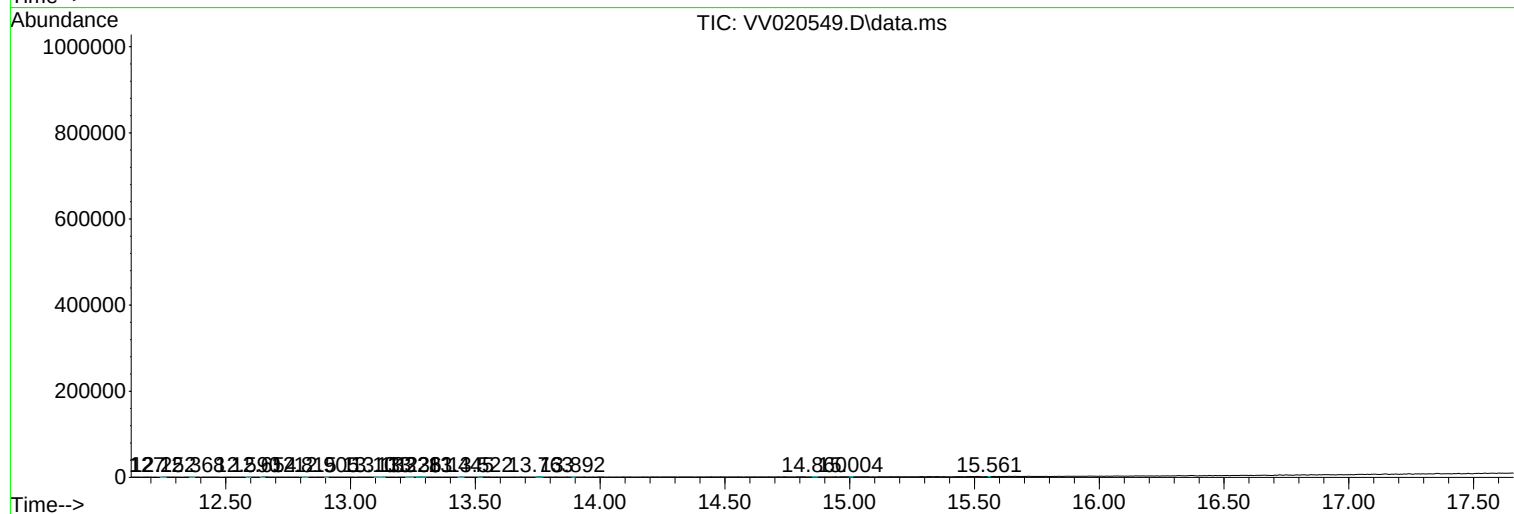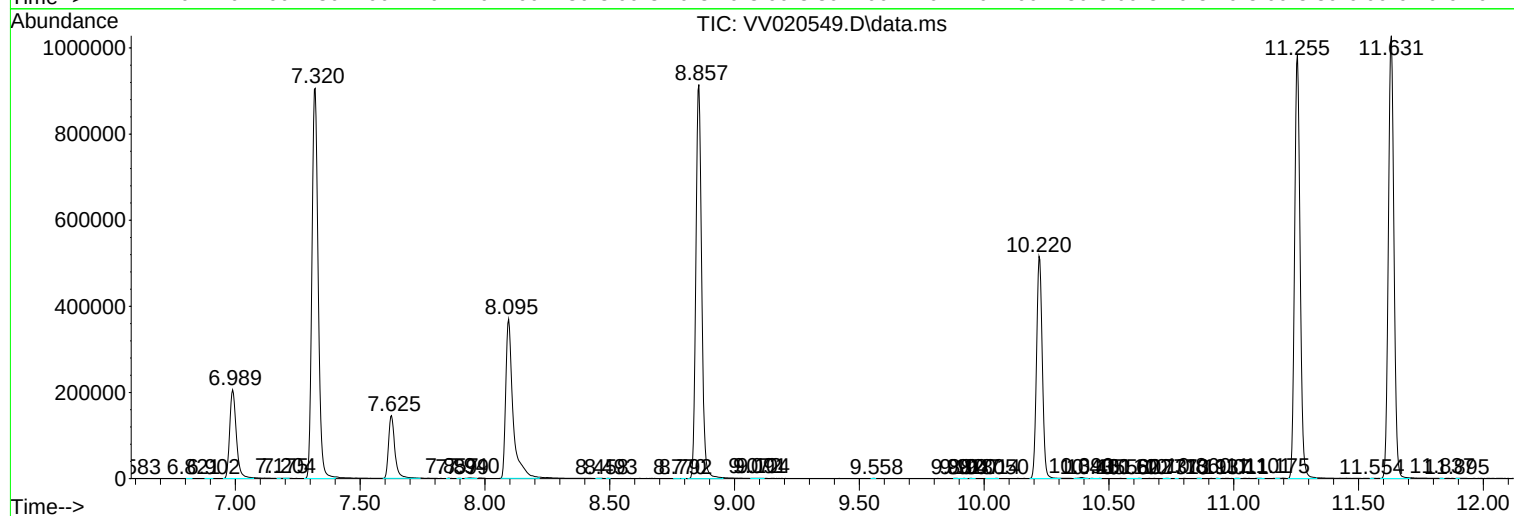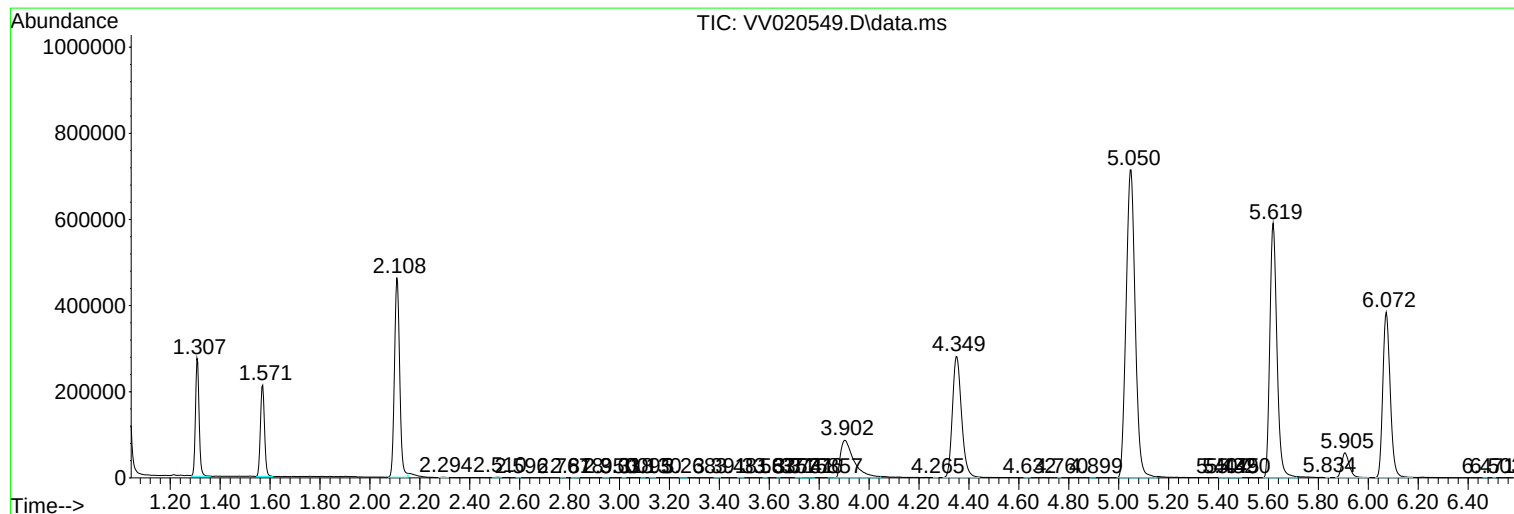

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
Data File : VV020549.D
Acq On : 11 Mar 2021 20:53
Operator : SY/MD
Sample : M1633-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B68

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
Data File : VV020549.D
Acq On : 11 Mar 2021 20:53
Operator : SY/MD
Sample : M1633-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B68

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
