

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
 Data File : VV020551.D
 Acq On : 11 Mar 2021 21:40
 Operator : SY/MD
 Sample : M1633-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B70

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M

Title : VOC Analysis

Signal : TIC: VV020551.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	104	rVB	263106	270848	15.26%	1.896%
2	1.571	157	165	177	rVB	211907	238951	13.46%	1.673%
3	2.108	322	332	346	rBV	446769	657075	37.01%	4.601%
4	2.298	387	391	399	rVB	1949	2107	0.12%	0.015%
5	2.355	403	409	410	rBV2	401	301	0.02%	0.002%
6	2.458	438	441	444	rBV2	336	207	0.01%	0.001%
7	2.510	452	457	465	rBV3	1072	1192	0.07%	0.008%
8	2.568	473	475	479	rBV2	354	240	0.01%	0.002%
9	2.616	486	490	494	rBV3	527	406	0.02%	0.003%
10	2.751	530	532	535	rVB	325	143	0.01%	0.001%
11	2.883	570	573	580	rVB2	293	311	0.02%	0.002%
12	2.966	596	599	601	rBV	219	156	0.01%	0.001%
13	3.060	623	628	632	rBV2	222	238	0.01%	0.002%
14	3.314	704	707	715	rBV2	303	409	0.02%	0.003%
15	3.359	717	721	726	rBV2	299	328	0.02%	0.002%
16	3.545	777	779	785	rBV2	156	191	0.01%	0.001%
17	3.593	785	794	798	rBV2	246	400	0.02%	0.003%
18	3.706	826	829	834	rBV2	242	275	0.02%	0.002%
19	3.902	879	890	932	rBV	90472	325513	18.33%	2.279%
20	4.133	959	962	970	rVB2	839	847	0.05%	0.006%
21	4.288	1008	1010	1013	rVB2	378	204	0.01%	0.001%
22	4.352	1013	1030	1060	rBV	276801	709635	39.97%	4.969%
23	4.539	1085	1088	1093	rBV3	492	530	0.03%	0.004%
24	4.596	1103	1106	1109	rVB3	412	283	0.02%	0.002%
25	4.616	1109	1112	1115	rVB2	323	253	0.01%	0.002%
26	4.638	1115	1119	1120	rBV2	234	174	0.01%	0.001%
27	4.677	1127	1131	1132	rBV2	312	186	0.01%	0.001%
28	4.712	1138	1142	1143	rBV	313	158	0.01%	0.001%
29	4.802	1167	1170	1178	rVB3	276	277	0.02%	0.002%
30	4.844	1178	1183	1186	rBV3	219	165	0.01%	0.001%
31	5.050	1229	1247	1273	rBV2	704102	1775426	100.00%	12.431%
32	5.301	1322	1325	1328	rVB2	294	174	0.01%	0.001%
33	5.420	1360	1362	1365	rVB2	353	224	0.01%	0.002%
34	5.439	1365	1368	1374	rBB3	233	258	0.01%	0.002%
35	5.465	1374	1376	1380	rVB3	216	168	0.01%	0.001%
36	5.497	1380	1386	1390	rBV3	411	462	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
 Data File : VV020551.D
 Acq On : 11 Mar 2021 21:40
 Operator : SY/MD
 Sample : M1633-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B70

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
 Title : VOC Analysis

37	5.622	1410	1425	1453	rBV	567285	1145836	64.54%	8.023%
38	5.850	1494	1496	1500	rVB2	373	159	0.01%	0.001%
39	5.912	1501	1515	1537	rBV6	85446	200525	11.29%	1.404%
40	6.072	1550	1565	1592	rBV	375524	768670	43.29%	5.382%
41	6.211	1605	1608	1610	rBV2	530	379	0.02%	0.003%
42	6.384	1658	1662	1666	rVV2	168	148	0.01%	0.001%
43	6.455	1682	1684	1687	rVB2	291	182	0.01%	0.001%
44	6.474	1687	1690	1694	rBV2	249	231	0.01%	0.002%
45	6.696	1756	1759	1766	rBV2	177	235	0.01%	0.002%
46	6.989	1839	1850	1882	rBV	200660	371831	20.94%	2.603%
47	7.243	1926	1929	1935	rVB3	337	406	0.02%	0.003%
48	7.272	1935	1938	1940	rBV2	242	185	0.01%	0.001%
49	7.320	1940	1953	1987	rBV	887717	1535686	86.50%	10.752%
50	7.555	2024	2026	2030	rVB	513	266	0.01%	0.002%
51	7.574	2030	2032	2035	rVB2	494	281	0.02%	0.002%
52	7.625	2035	2048	2075	rBV	144958	252542	14.22%	1.768%
53	7.895	2129	2132	2137	rBV2	286	226	0.01%	0.002%
54	7.944	2137	2147	2155	rBV3	1590	2267	0.13%	0.016%
55	7.989	2155	2161	2166	rBV5	968	1173	0.07%	0.008%
56	8.095	2182	2194	2228	rBV2	368450	732663	41.27%	5.130%
57	8.346	2271	2272	2276	rBV3	430	216	0.01%	0.002%
58	8.416	2291	2294	2298	rVB2	405	238	0.01%	0.002%
59	8.477	2310	2313	2314	rBV	227	149	0.01%	0.001%
60	8.619	2355	2357	2361	rVB2	209	145	0.01%	0.001%
61	8.796	2409	2412	2416	rVB2	241	179	0.01%	0.001%
62	8.857	2417	2431	2462	rBV	889855	1440760	81.15%	10.087%
63	9.162	2520	2526	2530	rVB3	258	306	0.02%	0.002%
64	9.210	2539	2541	2546	rVB	239	192	0.01%	0.001%
65	9.432	2605	2610	2615	rBV2	206	290	0.02%	0.002%
66	9.628	2667	2671	2673	rVV2	248	180	0.01%	0.001%
67	9.693	2687	2691	2694	rVB	244	169	0.01%	0.001%
68	9.731	2701	2703	2709	rVB2	262	197	0.01%	0.001%
69	9.763	2709	2713	2716	rBV	225	186	0.01%	0.001%
70	10.220	2843	2855	2881	rBV	511613	801297	45.13%	5.610%
71	10.355	2893	2897	2899	rBV	295	250	0.01%	0.002%
72	10.384	2899	2906	2917	rVB3	2461	3952	0.22%	0.028%
73	10.583	2962	2968	2970	rBV	217	199	0.01%	0.001%
74	10.628	2980	2982	2985	rVB2	264	168	0.01%	0.001%
75	10.651	2985	2989	2991	rBV	297	229	0.01%	0.002%
76	10.841	3045	3048	3053	rBV2	237	229	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
 Data File : VV020551.D
 Acq On : 11 Mar 2021 21:40
 Operator : SY/MD
 Sample : M1633-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B70

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M

Title : VOC Analysis

77	10.863	3053	3055	3059	rVV	318	172	0.01%	0.001%
78	11.053	3111	3114	3115	rBV	347	138	0.01%	0.001%
79	11.127	3134	3137	3139	rBV	385	279	0.02%	0.002%
80	11.255	3165	3177	3204	rBV	951855	1460911	82.29%	10.229%
81	11.497	3250	3252	3256	rVB	262	160	0.01%	0.001%
82	11.522	3256	3260	3265	rVB	482	396	0.02%	0.003%
83	11.632	3277	3294	3320	rBV	1006997	1563787	88.08%	10.949%
84	12.030	3415	3418	3419	rBV	276	167	0.01%	0.001%
85	12.114	3441	3444	3447	rBV	204	175	0.01%	0.001%
86	12.149	3451	3455	3459	rBV	329	270	0.02%	0.002%
87	12.259	3485	3489	3491	rBV2	279	242	0.01%	0.002%
88	12.455	3547	3550	3552	rBV3	242	184	0.01%	0.001%
89	12.660	3609	3614	3616	rBV2	314	280	0.02%	0.002%
90	12.773	3644	3649	3652	rBV2	283	285	0.02%	0.002%
91	12.792	3652	3655	3660	rVV	344	289	0.02%	0.002%
92	12.902	3685	3689	3692	rBV2	222	152	0.01%	0.001%
93	13.043	3730	3733	3735	rBV	259	155	0.01%	0.001%
94	13.152	3764	3767	3773	rVB	420	372	0.02%	0.003%
95	13.236	3789	3793	3797	rBV2	487	415	0.02%	0.003%
96	13.397	3838	3843	3846	rBV3	349	396	0.02%	0.003%
97	13.525	3881	3883	3889	rVB2	513	317	0.02%	0.002%
98	13.898	3996	3999	4005	rBV3	247	304	0.02%	0.002%
99	13.937	4009	4011	4014	rBV2	248	153	0.01%	0.001%
100	15.525	4501	4505	4507	rBV3	665	535	0.03%	0.004%




Sum of corrected areas: 14282671

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
Data File : VV020551.D
Acq On : 11 Mar 2021 21:40
Operator : SY/MD
Sample : M1633-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B70

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

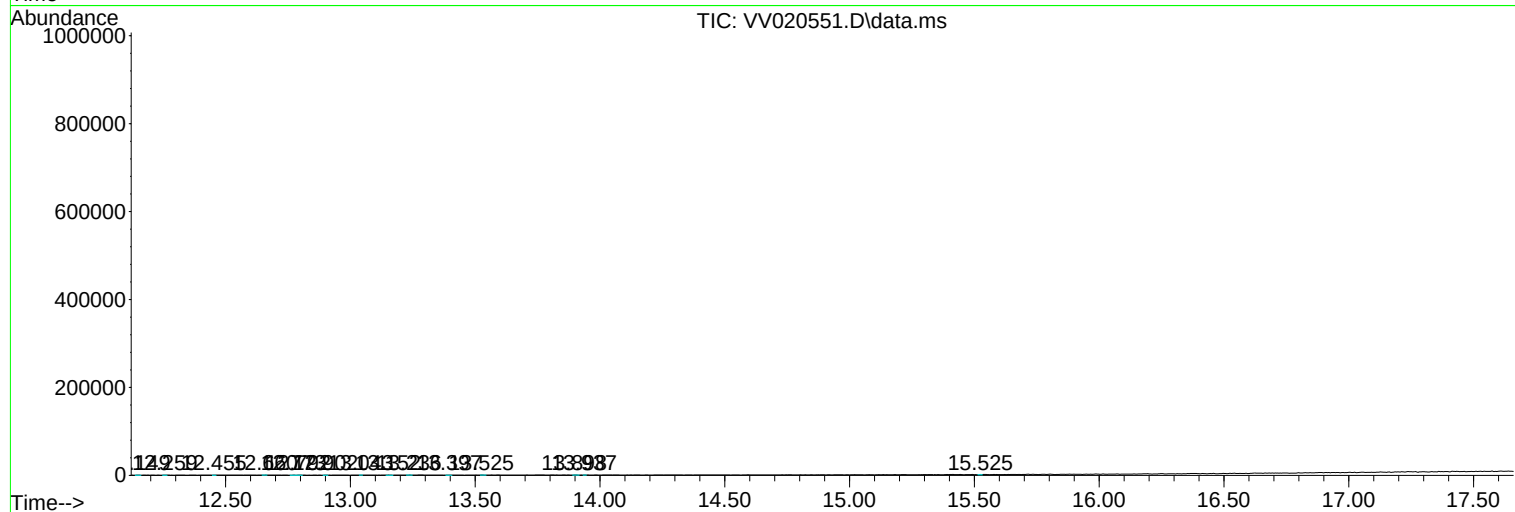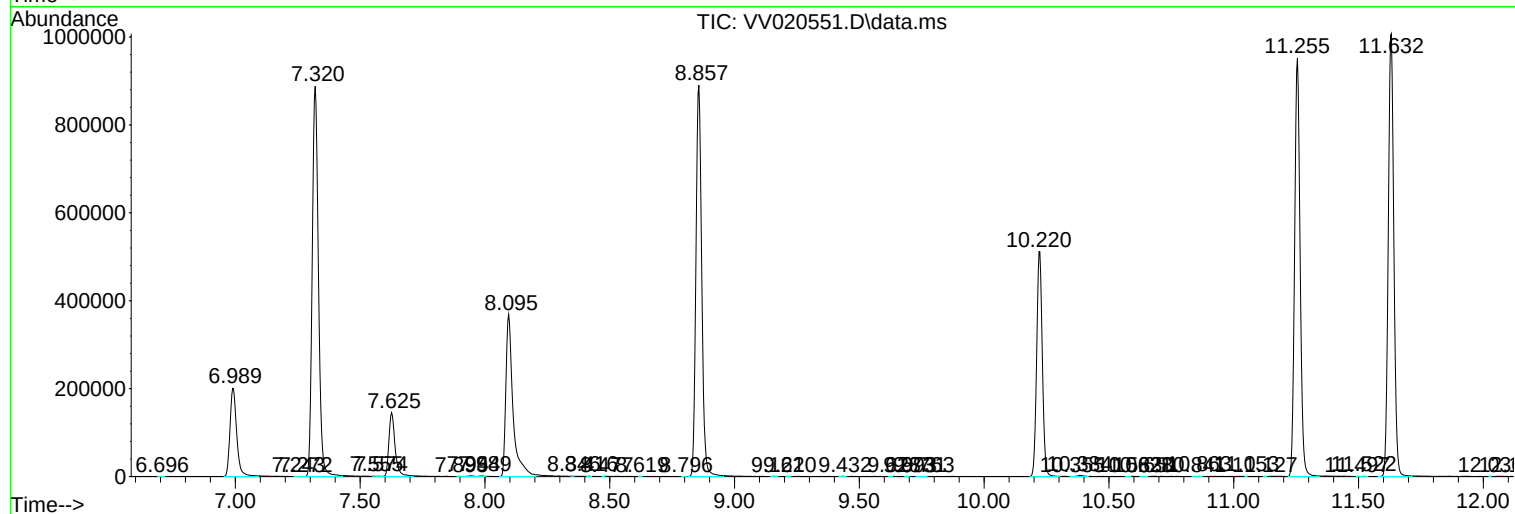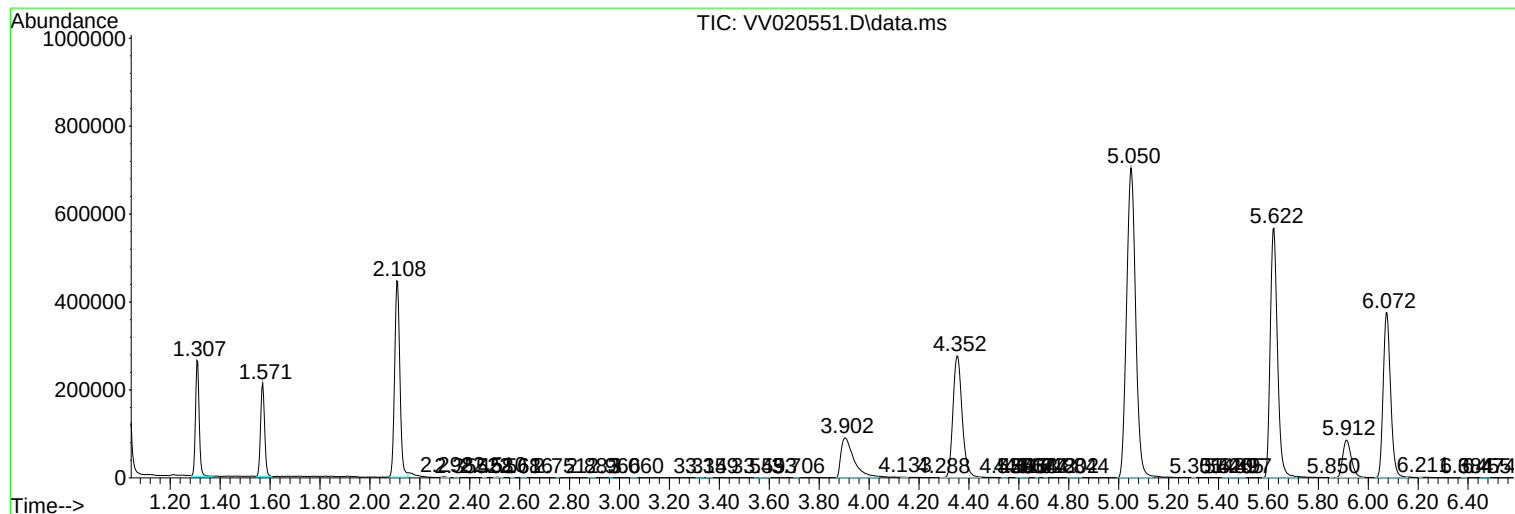

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
Data File : VV020551.D
Acq On : 11 Mar 2021 21:40
Operator : SY/MD
Sample : M1633-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B70

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
Data File : VV020551.D
Acq On : 11 Mar 2021 21:40
Operator : SY/MD
Sample : M1633-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B70

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
