

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
 Data File : VV020552.D
 Acq On : 11 Mar 2021 22:03
 Operator : SY/MD
 Sample : M1633-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B71

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M

Title : VOC Analysis

Signal : TIC: VV020552.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	96	rVB	264778	267991	14.75%	1.845%
2	1.571	157	165	177	rVB	210860	238954	13.15%	1.645%
3	2.047	311	313	316	rBV3	492	217	0.01%	0.001%
4	2.111	320	333	376	rVB	451467	687252	37.83%	4.732%
5	2.339	401	404	407	rBV2	383	278	0.02%	0.002%
6	2.359	407	410	412	rBV2	304	177	0.01%	0.001%
7	2.397	417	422	423	rBV2	399	309	0.02%	0.002%
8	2.506	453	456	467	rVB5	930	1324	0.07%	0.009%
9	2.687	509	512	516	rVB2	233	163	0.01%	0.001%
10	2.738	526	528	534	rBV2	228	222	0.01%	0.002%
11	3.191	663	669	671	rBV2	218	223	0.01%	0.002%
12	3.265	687	692	696	rVB2	180	203	0.01%	0.001%
13	3.330	709	712	716	rVB	225	170	0.01%	0.001%
14	3.445	741	748	750	rVB2	202	189	0.01%	0.001%
15	3.461	750	753	759	rBV2	216	311	0.02%	0.002%
16	3.548	777	780	787	rVB2	282	297	0.02%	0.002%
17	3.587	787	792	794	rBV2	227	213	0.01%	0.001%
18	3.629	801	805	808	rBV2	262	181	0.01%	0.001%
19	3.738	835	839	844	rBV	252	274	0.02%	0.002%
20	3.860	874	877	878	rBV	284	185	0.01%	0.001%
21	3.902	878	890	934	rBV2	93023	328119	18.06%	2.259%
22	4.207	982	985	993	rVB	426	350	0.02%	0.002%
23	4.352	1011	1030	1066	rBV	287719	727216	40.03%	5.007%
24	4.497	1073	1075	1079	rBB2	283	210	0.01%	0.001%
25	4.651	1121	1123	1127	rVV3	245	181	0.01%	0.001%
26	4.677	1127	1131	1135	rVV2	482	431	0.02%	0.003%
27	4.860	1184	1188	1191	rBV2	221	185	0.01%	0.001%
28	4.966	1218	1221	1226	rBV2	312	233	0.01%	0.002%
29	5.050	1230	1247	1291	rBV2	712346	1816520	100.00%	12.507%
30	5.394	1350	1354	1357	rBV3	316	333	0.02%	0.002%
31	5.439	1366	1368	1372	rBV3	207	173	0.01%	0.001%
32	5.619	1412	1424	1453	rBV	573215	1153204	63.48%	7.940%
33	5.911	1502	1515	1536	rBV4	83084	194467	10.71%	1.339%
34	6.072	1551	1565	1598	rBV	385900	784170	43.17%	5.399%
35	6.474	1686	1690	1698	rBV2	190	253	0.01%	0.002%
36	6.792	1786	1789	1794	rVB2	238	204	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
 Data File : VV020552.D
 Acq On : 11 Mar 2021 22:03
 Operator : SY/MD
 Sample : M1633-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B71

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M

Title : VOC Analysis

37	6.989	1839	1850	1877	rBV	206964	376015	20.70%	2.589%
38	7.320	1940	1953	1984	rBV	891617	1554010	85.55%	10.700%
39	7.580	2031	2034	2037	rBV3	240	202	0.01%	0.001%
40	7.625	2037	2048	2072	rBV2	146744	256196	14.10%	1.764%
41	7.812	2103	2106	2109	rVB2	526	314	0.02%	0.002%
42	7.940	2135	2146	2156	rBV3	2289	4328	0.24%	0.030%
43	7.989	2156	2161	2166	rVB4	1027	1225	0.07%	0.008%
44	8.095	2182	2194	2239	rBV2	382926	772740	42.54%	5.321%
45	8.339	2268	2270	2273	rBV	241	176	0.01%	0.001%
46	8.387	2283	2285	2288	rBV	255	168	0.01%	0.001%
47	8.413	2291	2293	2296	rVB2	521	241	0.01%	0.002%
48	8.487	2311	2316	2319	rVB2	206	211	0.01%	0.001%
49	8.513	2319	2324	2325	rBV2	215	221	0.01%	0.002%
50	8.857	2419	2431	2464	rBV	889114	1441512	79.36%	9.925%
51	9.027	2482	2484	2487	rVB2	504	280	0.02%	0.002%
52	9.053	2490	2492	2498	rVB3	308	232	0.01%	0.002%
53	9.165	2525	2527	2530	rVB	368	178	0.01%	0.001%
54	9.204	2537	2539	2541	rBV	516	204	0.01%	0.001%
55	9.297	2566	2568	2571	rBV	293	169	0.01%	0.001%
56	9.538	2638	2643	2647	rBV	367	325	0.02%	0.002%
57	9.612	2661	2666	2669	rBV2	208	227	0.01%	0.002%
58	9.879	2745	2749	2752	rBV	282	314	0.02%	0.002%
59	10.056	2798	2804	2808	rBV2	192	245	0.01%	0.002%
60	10.220	2843	2855	2876	rBV	522827	824490	45.39%	5.677%
61	10.336	2888	2891	2893	rBV2	244	178	0.01%	0.001%
62	10.390	2899	2908	2920	rVB2	3901	5503	0.30%	0.038%
63	10.451	2920	2927	2929	rBV	223	243	0.01%	0.002%
64	10.770	3024	3026	3028	rVV2	304	162	0.01%	0.001%
65	10.789	3029	3032	3038	rVB3	690	595	0.03%	0.004%
66	10.969	3085	3088	3095	rBV2	262	416	0.02%	0.003%
67	11.114	3127	3133	3134	rBV	157	165	0.01%	0.001%
68	11.175	3147	3152	3156	rBV4	353	313	0.02%	0.002%
69	11.255	3162	3177	3206	rBV	967426	1470536	80.95%	10.125%
70	11.468	3241	3243	3247	rVB2	350	213	0.01%	0.001%
71	11.554	3267	3270	3272	rBV2	373	255	0.01%	0.002%
72	11.632	3280	3294	3317	rBV	1030653	1597779	87.96%	11.001%
73	11.799	3343	3346	3350	rBV3	282	289	0.02%	0.002%
74	11.818	3350	3352	3355	rVB2	363	187	0.01%	0.001%
75	11.837	3355	3358	3363	rVB2	306	257	0.01%	0.002%
76	11.863	3363	3366	3368	rBV2	280	227	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
 Data File : VV020552.D
 Acq On : 11 Mar 2021 22:03
 Operator : SY/MD
 Sample : M1633-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B71

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
 Title : VOC Analysis

77	11.914	3377	3382	3383	rBV	252	174	0.01%	0.001%
78	11.927	3384	3386	3392	rVB2	316	248	0.01%	0.002%
79	11.988	3403	3405	3408	rVB2	339	178	0.01%	0.001%
80	12.140	3449	3452	3455	rVB	293	180	0.01%	0.001%
81	12.162	3455	3459	3462	rBV2	266	203	0.01%	0.001%
82	12.255	3483	3488	3492	rBV2	401	460	0.03%	0.003%
83	12.307	3502	3504	3508	rVB2	309	175	0.01%	0.001%
84	12.349	3513	3517	3518	rBV	275	201	0.01%	0.001%
85	12.657	3611	3613	3619	rBV2	412	249	0.01%	0.002%
86	12.731	3632	3636	3637	rBV	205	166	0.01%	0.001%
87	12.802	3655	3658	3660	rBV2	336	214	0.01%	0.001%
88	12.992	3714	3717	3721	rBV	280	319	0.02%	0.002%
89	13.207	3782	3784	3787	rVB	357	208	0.01%	0.001%
90	13.268	3800	3803	3804	rBV	396	172	0.01%	0.001%
91	13.313	3815	3817	3821	rVB2	329	176	0.01%	0.001%
92	13.439	3852	3856	3860	rBV2	300	299	0.02%	0.002%
93	13.606	3905	3908	3910	rBV2	527	281	0.02%	0.002%
94	13.754	3952	3954	3955	rBV2	453	190	0.01%	0.001%
95	14.326	4128	4132	4138	rVB3	936	880	0.05%	0.006%
96	14.413	4157	4159	4164	rVB2	453	296	0.02%	0.002%
97	14.705	4247	4250	4252	rVB2	623	292	0.02%	0.002%
98	15.323	4439	4442	4444	rBV3	509	410	0.02%	0.003%
99	15.336	4444	4446	4451	rVB2	720	544	0.03%	0.004%
100	15.377	4457	4459	4462	rBV2	608	259	0.01%	0.002%




Sum of corrected areas: 14523697

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
Data File : VV020552.D
Acq On : 11 Mar 2021 22:03
Operator : SY/MD
Sample : M1633-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B71

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

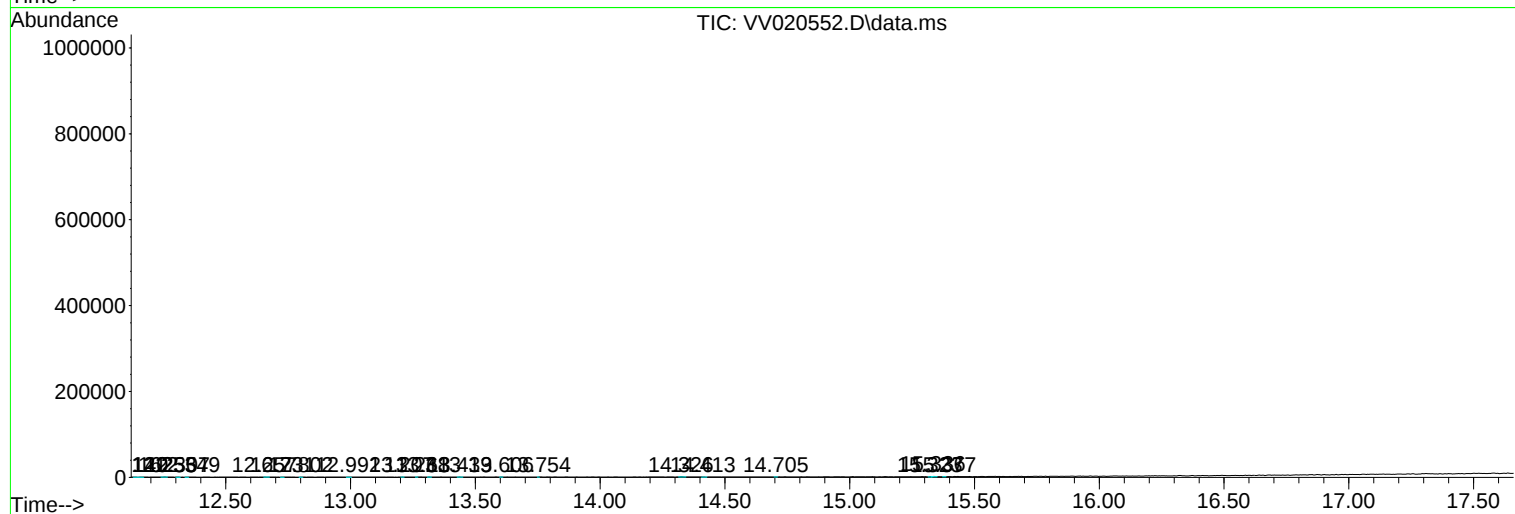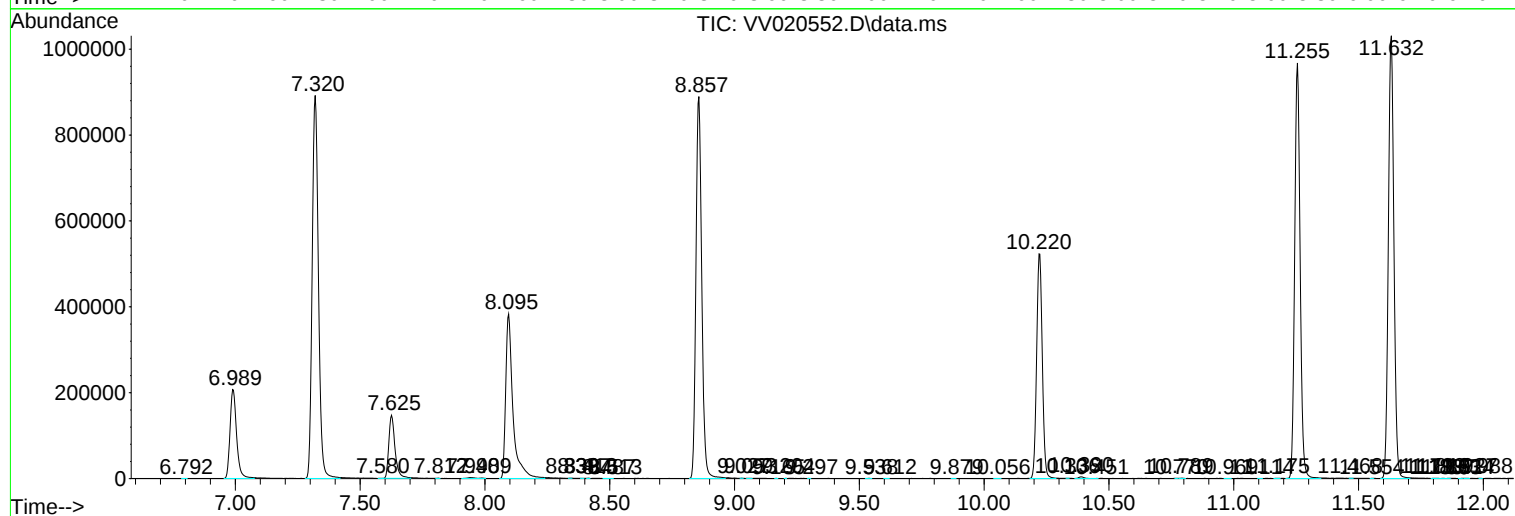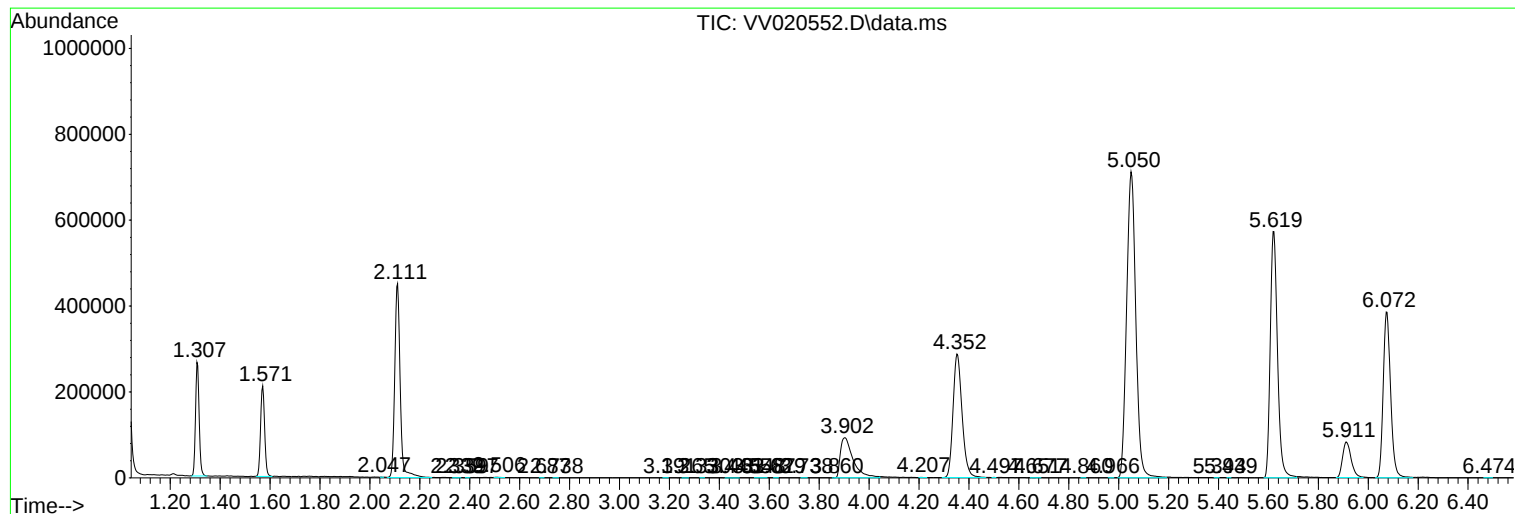

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
Data File : VV020552.D
Acq On : 11 Mar 2021 22:03
Operator : SY/MD
Sample : M1633-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B71

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
Data File : VV020552.D
Acq On : 11 Mar 2021 22:03
Operator : SY/MD
Sample : M1633-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B71

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
