

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
 Data File : VV020553.D
 Acq On : 11 Mar 2021 22:27
 Operator : SY/MD
 Sample : M1633-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B72

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M

Title : VOC Analysis

Signal : TIC: VV020553.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	50	55	68	rBV2	11475	11490	0.64%	0.081%
2	1.307	76	83	100	rVB	260627	267517	14.97%	1.885%
3	1.571	157	165	179	rBV	210894	238917	13.37%	1.683%
4	1.992	293	296	299	rBV4	950	535	0.03%	0.004%
5	2.111	322	333	346	rBV	440752	644909	36.08%	4.543%
6	2.625	489	493	496	rBV2	509	432	0.02%	0.003%
7	2.706	515	518	521	rBV3	298	157	0.01%	0.001%
8	2.757	530	534	536	rBV2	238	169	0.01%	0.001%
9	2.818	550	553	557	rVB2	259	226	0.01%	0.002%
10	2.876	568	571	574	rVV2	217	160	0.01%	0.001%
11	2.960	594	597	605	rVB5	770	890	0.05%	0.006%
12	3.047	619	624	627	rVB2	241	248	0.01%	0.002%
13	3.069	627	631	634	rBV	222	163	0.01%	0.001%
14	3.092	634	638	645	rBV2	232	243	0.01%	0.002%
15	3.130	645	650	655	rBV2	287	269	0.02%	0.002%
16	3.169	659	662	666	rVB	375	313	0.02%	0.002%
17	3.333	709	713	717	rVB	254	226	0.01%	0.002%
18	3.355	717	720	722	rBV2	187	159	0.01%	0.001%
19	3.699	820	827	832	rBV	275	326	0.02%	0.002%
20	3.809	855	861	864	rBV2	244	249	0.01%	0.002%
21	3.908	877	892	942	rBV2	89540	348925	19.52%	2.458%
22	4.240	993	995	999	rVB2	610	331	0.02%	0.002%
23	4.352	1013	1030	1062	rBV	279588	709713	39.71%	5.000%
24	4.542	1087	1089	1093	rVB	330	171	0.01%	0.001%
25	4.609	1106	1110	1112	rBV3	255	180	0.01%	0.001%
26	4.908	1200	1203	1206	rBV	264	209	0.01%	0.001%
27	4.928	1207	1209	1214	rVB2	211	180	0.01%	0.001%
28	5.050	1229	1247	1287	rBV2	695405	1787276	100.00%	12.591%
29	5.272	1313	1316	1317	rBV2	446	247	0.01%	0.002%
30	5.307	1324	1327	1333	rVB	522	405	0.02%	0.003%
31	5.333	1333	1335	1341	rVB3	474	235	0.01%	0.002%
32	5.487	1377	1383	1384	rBV2	261	226	0.01%	0.002%
33	5.497	1384	1386	1393	rVB2	251	258	0.01%	0.002%
34	5.551	1398	1403	1404	rBV2	409	277	0.02%	0.002%
35	5.622	1412	1425	1457	rBV	562590	1130778	63.27%	7.966%
36	5.908	1501	1514	1539	rBV	77471	158779	8.88%	1.119%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
 Data File : VV020553.D
 Acq On : 11 Mar 2021 22:27
 Operator : SY/MD
 Sample : M1633-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B72

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
 Title : VOC Analysis

37	6.075	1550	1566	1595	rBV	380107	772883	43.24%	5.445%
38	6.214	1604	1609	1610	rBV2	630	442	0.02%	0.003%
39	6.297	1632	1635	1637	rBV	263	198	0.01%	0.001%
40	6.333	1644	1646	1653	rVB2	493	356	0.02%	0.003%
41	6.455	1678	1684	1686	rBV2	187	259	0.01%	0.002%
42	6.545	1709	1712	1715	rVB2	306	165	0.01%	0.001%
43	6.821	1793	1798	1802	rBV2	206	242	0.01%	0.002%
44	6.908	1820	1825	1830	rVB2	204	235	0.01%	0.002%
45	6.944	1830	1836	1839	rBV2	145	162	0.01%	0.001%
46	6.989	1839	1850	1879	rBV	199442	369759	20.69%	2.605%
47	7.162	1900	1904	1910	rVB3	515	558	0.03%	0.004%
48	7.204	1915	1917	1922	rBV2	366	236	0.01%	0.002%
49	7.272	1935	1938	1941	rVB2	427	272	0.02%	0.002%
50	7.320	1941	1953	1978	rBV	890157	1533126	85.78%	10.801%
51	7.625	2038	2048	2077	rBV	144756	250936	14.04%	1.768%
52	7.882	2122	2128	2134	rBV2	212	311	0.02%	0.002%
53	7.940	2144	2146	2155	rVV2	1050	1251	0.07%	0.009%
54	7.982	2155	2159	2170	rVB5	873	1358	0.08%	0.010%
55	8.095	2184	2194	2236	rBV2	363080	766775	42.90%	5.402%
56	8.429	2294	2298	2299	rBV2	234	154	0.01%	0.001%
57	8.445	2299	2303	2306	rVB2	495	394	0.02%	0.003%
58	8.481	2311	2314	2316	rBV2	282	192	0.01%	0.001%
59	8.519	2323	2326	2331	rBV4	326	214	0.01%	0.002%
60	8.567	2337	2341	2346	rBV2	323	265	0.01%	0.002%
61	8.593	2346	2349	2352	rBV	225	152	0.01%	0.001%
62	8.857	2419	2431	2458	rBV	870619	1414667	79.15%	9.966%
63	9.066	2493	2496	2499	rBV	505	309	0.02%	0.002%
64	9.085	2499	2502	2505	rVV3	225	179	0.01%	0.001%
65	9.156	2521	2524	2529	rVV2	607	501	0.03%	0.004%
66	9.374	2591	2592	2597	rVB	227	155	0.01%	0.001%
67	9.445	2609	2614	2618	rBV	283	295	0.02%	0.002%
68	9.542	2641	2644	2648	rBV2	255	270	0.02%	0.002%
69	9.580	2648	2656	2667	rVV3	2966	5324	0.30%	0.038%
70	9.638	2671	2674	2676	rBV	277	177	0.01%	0.001%
71	9.696	2687	2692	2695	rBV2	245	221	0.01%	0.002%
72	9.853	2737	2741	2744	rBV2	304	281	0.02%	0.002%
73	10.220	2843	2855	2881	rVV	481971	761815	42.62%	5.367%
74	10.381	2897	2905	2917	rBV3	1147	2022	0.11%	0.014%
75	10.587	2967	2969	2971	rBV	250	165	0.01%	0.001%
76	10.911	3066	3070	3075	rVB	315	246	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
 Data File : VV020553.D
 Acq On : 11 Mar 2021 22:27
 Operator : SY/MD
 Sample : M1633-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B72

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M

Title : VOC Analysis

77	10.937	3075	3078	3081	rBV3	308	267	0.01%	0.002%
78	10.966	3084	3087	3089	rBV	341	250	0.01%	0.002%
79	11.255	3163	3177	3201	rBV	933272	1434509	80.26%	10.106%
80	11.423	3226	3229	3232	rBV3	428	301	0.02%	0.002%
81	11.484	3246	3248	3251	rBV	251	165	0.01%	0.001%
82	11.506	3252	3255	3257	rVB3	291	176	0.01%	0.001%
83	11.574	3273	3276	3280	rBV3	250	196	0.01%	0.001%
84	11.632	3280	3294	3314	rBV	1015899	1560969	87.34%	10.997%
85	11.767	3334	3336	3339	rVB2	318	155	0.01%	0.001%
86	11.982	3401	3403	3409	rVB2	287	196	0.01%	0.001%
87	12.123	3445	3447	3451	rVB2	314	158	0.01%	0.001%
88	12.657	3610	3613	3617	rBV2	312	267	0.01%	0.002%
89	12.786	3650	3653	3656	rBV2	228	189	0.01%	0.001%
90	12.937	3695	3700	3703	rBV3	263	279	0.02%	0.002%
91	13.114	3752	3755	3759	rBV2	360	322	0.02%	0.002%
92	13.197	3778	3781	3784	rBV3	264	216	0.01%	0.002%
93	13.281	3805	3807	3810	rVB2	464	270	0.02%	0.002%
94	13.503	3870	3876	3879	rBV2	319	376	0.02%	0.003%
95	13.905	3998	4001	4003	rBV2	334	247	0.01%	0.002%
96	14.094	4057	4060	4066	rBV	412	433	0.02%	0.003%
97	15.088	4366	4369	4374	rBV2	415	459	0.03%	0.003%
98	15.120	4376	4379	4382	rVB3	595	483	0.03%	0.003%
99	15.303	4434	4436	4440	rVB3	749	532	0.03%	0.004%
100	15.323	4440	4442	4443	rBV2	500	222	0.01%	0.002%




Sum of corrected areas: 14194947

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
Data File : VV020553.D
Acq On : 11 Mar 2021 22:27
Operator : SY/MD
Sample : M1633-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B72

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

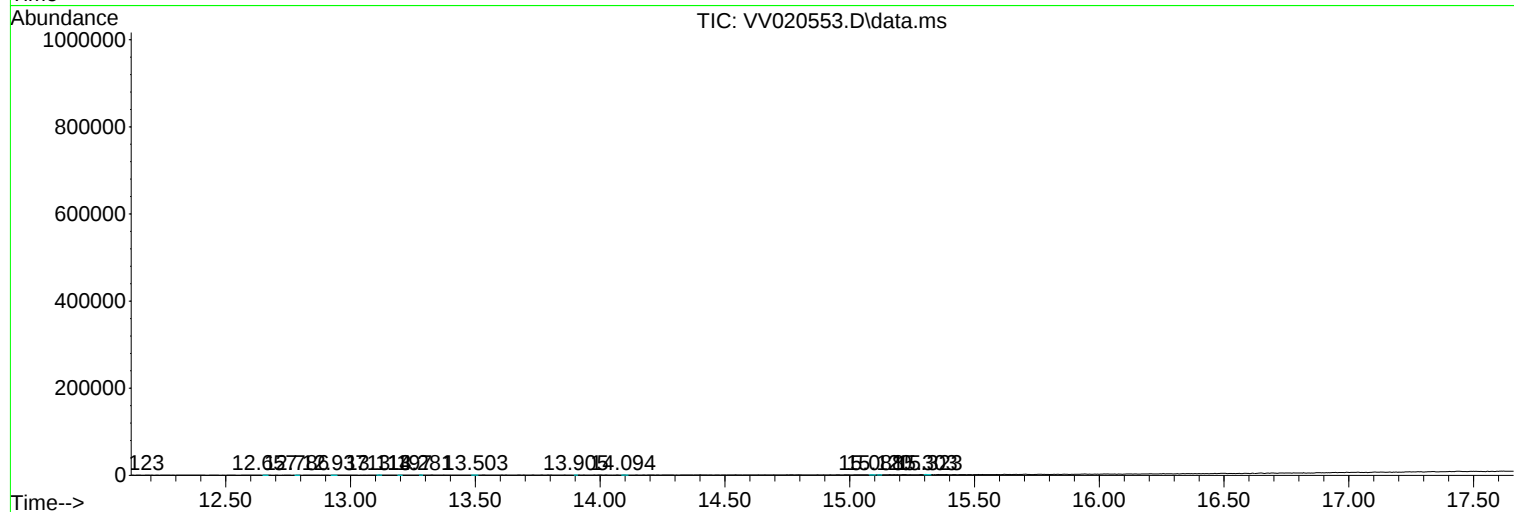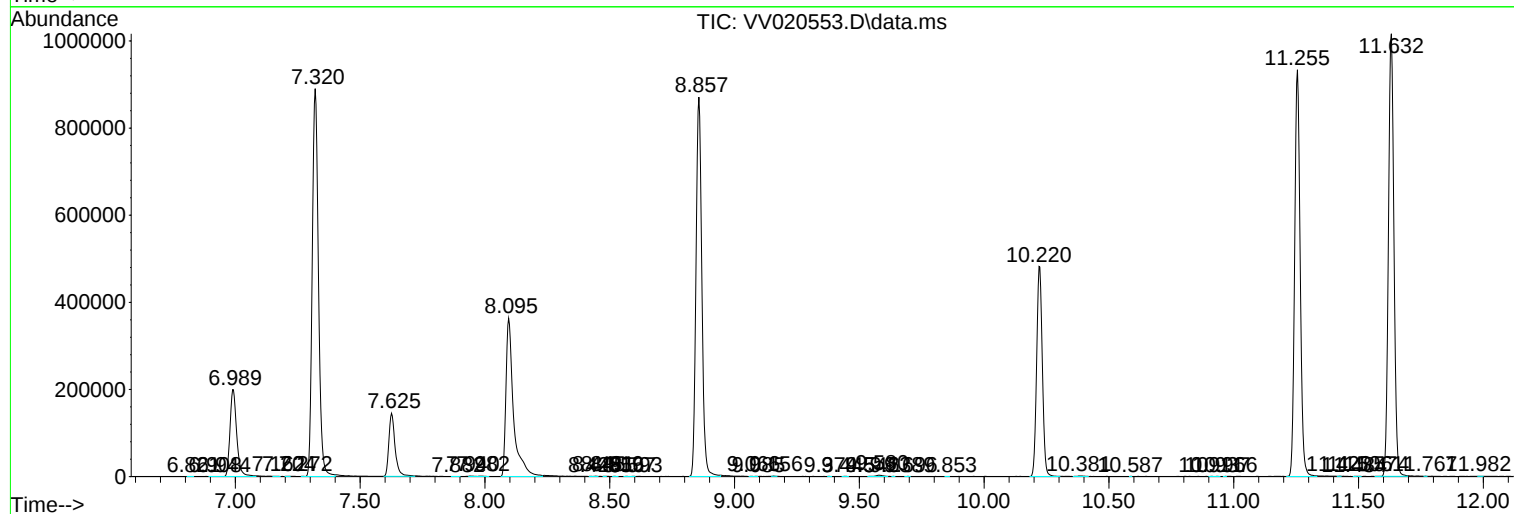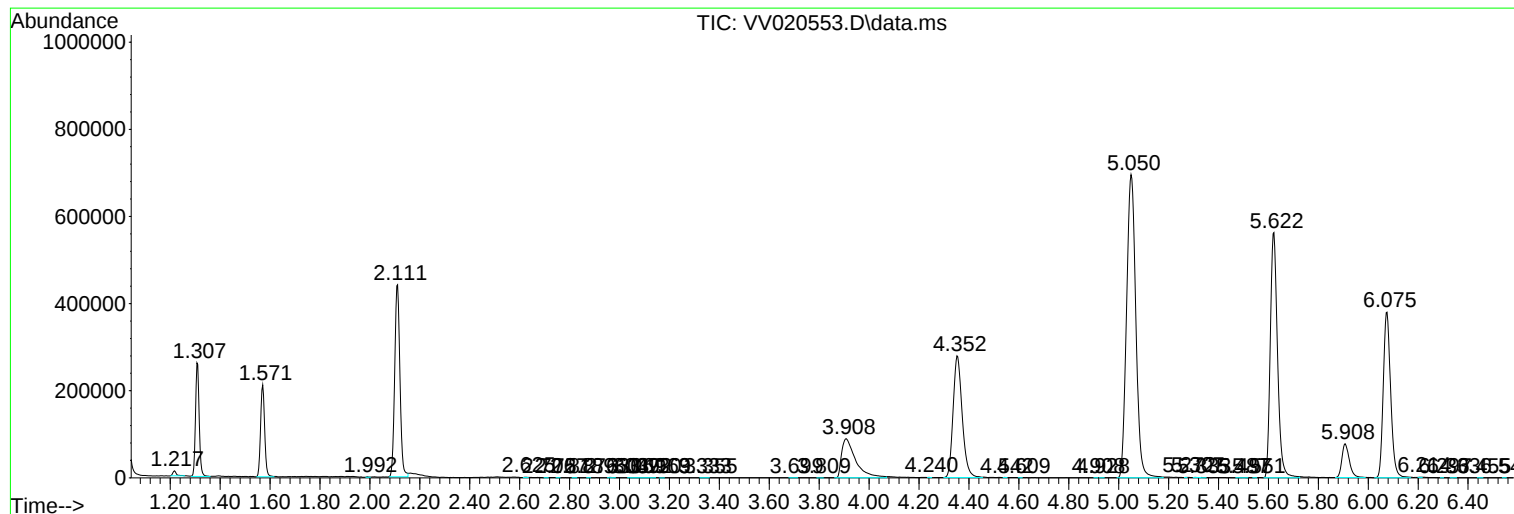

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
Data File : VV020553.D
Acq On : 11 Mar 2021 22:27
Operator : SY/MD
Sample : M1633-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B72

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
Data File : VV020553.D
Acq On : 11 Mar 2021 22:27
Operator : SY/MD
Sample : M1633-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B72

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
