

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
 Data File : VV020554.D
 Acq On : 11 Mar 2021 22:50
 Operator : SY/MD
 Sample : M1633-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B75

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M

Title : VOC Analysis

Signal : TIC: VV020554.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	99	rVB	258385	260035	14.80%	1.857%
2	1.571	157	165	182	rBV	203472	235610	13.41%	1.683%
3	2.108	321	332	373	rVB	434206	657643	37.44%	4.697%
4	2.320	395	398	401	rBV	310	185	0.01%	0.001%
5	2.388	417	419	424	rBV	311	231	0.01%	0.002%
6	2.426	428	431	433	rBV2	278	215	0.01%	0.002%
7	2.513	451	458	464	rBV6	883	1224	0.07%	0.009%
8	2.548	464	469	472	rVV3	270	229	0.01%	0.002%
9	2.735	523	527	532	rVB2	190	176	0.01%	0.001%
10	2.825	552	555	557	rBV	281	197	0.01%	0.001%
11	2.841	558	560	563	rVB	356	227	0.01%	0.002%
12	2.860	563	566	567	rBV	329	164	0.01%	0.001%
13	2.953	590	595	597	rBV2	164	192	0.01%	0.001%
14	3.191	666	669	672	rVB2	297	191	0.01%	0.001%
15	3.217	672	677	679	rBV	257	260	0.01%	0.002%
16	3.291	698	700	703	rVB	271	159	0.01%	0.001%
17	3.445	743	748	750	rBV2	246	195	0.01%	0.001%
18	3.593	789	794	798	rVB2	293	311	0.02%	0.002%
19	3.616	798	801	802	rBV2	244	155	0.01%	0.001%
20	3.902	879	890	932	rBV	93020	324260	18.46%	2.316%
21	4.352	1011	1030	1058	rBV	274582	701494	39.94%	5.010%
22	4.568	1093	1097	1100	rBV2	270	249	0.01%	0.002%
23	4.722	1141	1145	1148	rVB2	261	181	0.01%	0.001%
24	4.748	1149	1153	1155	rBV2	257	163	0.01%	0.001%
25	4.896	1193	1199	1201	rBV2	159	174	0.01%	0.001%
26	5.050	1229	1247	1282	rBV2	694400	1756444	100.00%	12.544%
27	5.320	1327	1331	1333	rBV3	337	288	0.02%	0.002%
28	5.452	1370	1372	1376	rBV3	268	181	0.01%	0.001%
29	5.510	1387	1390	1395	rVB3	243	181	0.01%	0.001%
30	5.542	1396	1400	1404	rVB3	279	261	0.01%	0.002%
31	5.574	1404	1410	1412	rBV3	387	357	0.02%	0.003%
32	5.622	1412	1425	1456	rBV	556680	1122080	63.88%	8.013%
33	5.908	1502	1514	1535	rVV2	58339	120051	6.83%	0.857%
34	6.072	1552	1565	1590	rBV	375775	755301	43.00%	5.394%
35	6.268	1623	1626	1630	rVB3	513	327	0.02%	0.002%
36	6.291	1631	1633	1637	rVB3	380	308	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW031221\
 Data File : VW020554.D
 Acq On : 11 Mar 2021 22:50
 Operator : SY/MD
 Sample : M1633-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B75

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
 Title : VOC Analysis

37	6.320	1640	1642	1645	rVB	333	184	0.01%	0.001%
38	6.358	1652	1654	1660	rVB2	244	151	0.01%	0.001%
39	6.770	1775	1782	1785	rBV2	204	232	0.01%	0.002%
40	6.905	1821	1824	1825	rBV2	349	153	0.01%	0.001%
41	6.989	1839	1850	1883	rBV	196298	362265	20.62%	2.587%
42	7.133	1893	1895	1898	rVB	416	221	0.01%	0.002%
43	7.149	1898	1900	1903	rVB2	337	165	0.01%	0.001%
44	7.236	1924	1927	1932	rVB2	433	365	0.02%	0.003%
45	7.320	1940	1953	1979	rBV	880342	1510459	86.00%	10.787%
46	7.625	2038	2048	2077	rBV	140822	245699	13.99%	1.755%
47	7.899	2130	2133	2136	rBV2	229	172	0.01%	0.001%
48	7.940	2144	2146	2147	rBV	498	223	0.01%	0.002%
49	7.985	2155	2160	2162	rBV4	752	544	0.03%	0.004%
50	8.014	2167	2169	2174	rVB2	173	152	0.01%	0.001%
51	8.095	2184	2194	2228	rBV2	362244	743441	42.33%	5.309%
52	8.394	2283	2287	2289	rVB2	332	200	0.01%	0.001%
53	8.471	2303	2311	2314	rBV3	310	280	0.02%	0.002%
54	8.487	2314	2316	2319	rBV2	251	157	0.01%	0.001%
55	8.522	2324	2327	2329	rBV	344	233	0.01%	0.002%
56	8.625	2354	2359	2362	rVB3	226	202	0.01%	0.001%
57	8.693	2377	2380	2385	rVB	224	172	0.01%	0.001%
58	8.735	2391	2393	2397	rVB	310	174	0.01%	0.001%
59	8.857	2419	2431	2456	rBV	875725	1400340	79.73%	10.001%
60	9.297	2564	2568	2571	rBV2	225	191	0.01%	0.001%
61	9.329	2574	2578	2583	rVB3	288	285	0.02%	0.002%
62	9.558	2647	2649	2652	rBV	348	226	0.01%	0.002%
63	9.596	2657	2661	2665	rVB2	222	187	0.01%	0.001%
64	9.632	2665	2672	2673	rBV2	132	160	0.01%	0.001%
65	9.648	2676	2677	2686	rVB3	281	263	0.01%	0.002%
66	9.783	2715	2719	2722	rVB2	214	172	0.01%	0.001%
67	9.940	2765	2768	2770	rBV	266	191	0.01%	0.001%
68	9.992	2779	2784	2790	rVB2	211	285	0.02%	0.002%
69	10.223	2843	2856	2880	rBV	505819	794532	45.24%	5.674%
70	10.336	2889	2891	2895	rVB2	580	333	0.02%	0.002%
71	10.390	2901	2908	2917	rBV2	1155	1576	0.09%	0.011%
72	10.516	2939	2947	2950	rBV2	249	388	0.02%	0.003%
73	10.619	2975	2979	2984	rVB2	182	187	0.01%	0.001%
74	10.670	2992	2995	3001	rVB2	185	156	0.01%	0.001%
75	10.825	3038	3043	3047	rBV2	247	339	0.02%	0.002%
76	10.847	3047	3050	3055	rVV2	215	254	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
 Data File : VV020554.D
 Acq On : 11 Mar 2021 22:50
 Operator : SY/MD
 Sample : M1633-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B75

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
 Title : VOC Analysis

77	10.976	3087	3090	3094	rBV	264	223	0.01%	0.002%
78	11.117	3130	3134	3137	rBV	239	220	0.01%	0.002%
79	11.255	3164	3177	3206	rBV	936624	1424576	81.11%	10.174%
80	11.545	3257	3267	3281	rBV3	11401	21894	1.25%	0.156%
81	11.632	3282	3294	3322	rVB	993573	1544459	87.93%	11.030%
82	11.837	3356	3358	3361	rVB	361	163	0.01%	0.001%
83	11.963	3393	3397	3403	rBV	427	265	0.02%	0.002%
84	12.062	3424	3428	3433	rBV3	414	373	0.02%	0.003%
85	12.104	3438	3441	3445	rBV2	296	222	0.01%	0.002%
86	12.259	3485	3489	3490	rBV2	455	265	0.02%	0.002%
87	12.323	3506	3509	3510	rBV	481	196	0.01%	0.001%
88	12.464	3548	3553	3556	rBV2	323	344	0.02%	0.002%
89	12.615	3596	3600	3608	rVB3	255	287	0.02%	0.002%
90	12.660	3610	3614	3617	rBV3	313	271	0.02%	0.002%
91	12.699	3623	3626	3628	rBV2	276	154	0.01%	0.001%
92	12.905	3687	3690	3693	rBV	259	170	0.01%	0.001%
93	13.043	3731	3733	3737	rVB	397	218	0.01%	0.002%
94	13.249	3794	3797	3799	rBV	339	210	0.01%	0.001%
95	13.323	3816	3820	3822	rBV2	357	291	0.02%	0.002%
96	13.625	3911	3914	3920	rBV2	346	333	0.02%	0.002%
97	13.757	3953	3955	3961	rVB3	468	344	0.02%	0.002%
98	14.062	4047	4050	4052	rBV	480	272	0.02%	0.002%
99	14.837	4289	4291	4293	rVB	549	225	0.01%	0.002%
100	15.033	4349	4352	4358	rBV3	636	715	0.04%	0.005%


Sum of corrected areas: 14002498

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
Data File : VV020554.D
Acq On : 11 Mar 2021 22:50
Operator : SY/MD
Sample : M1633-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B75

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

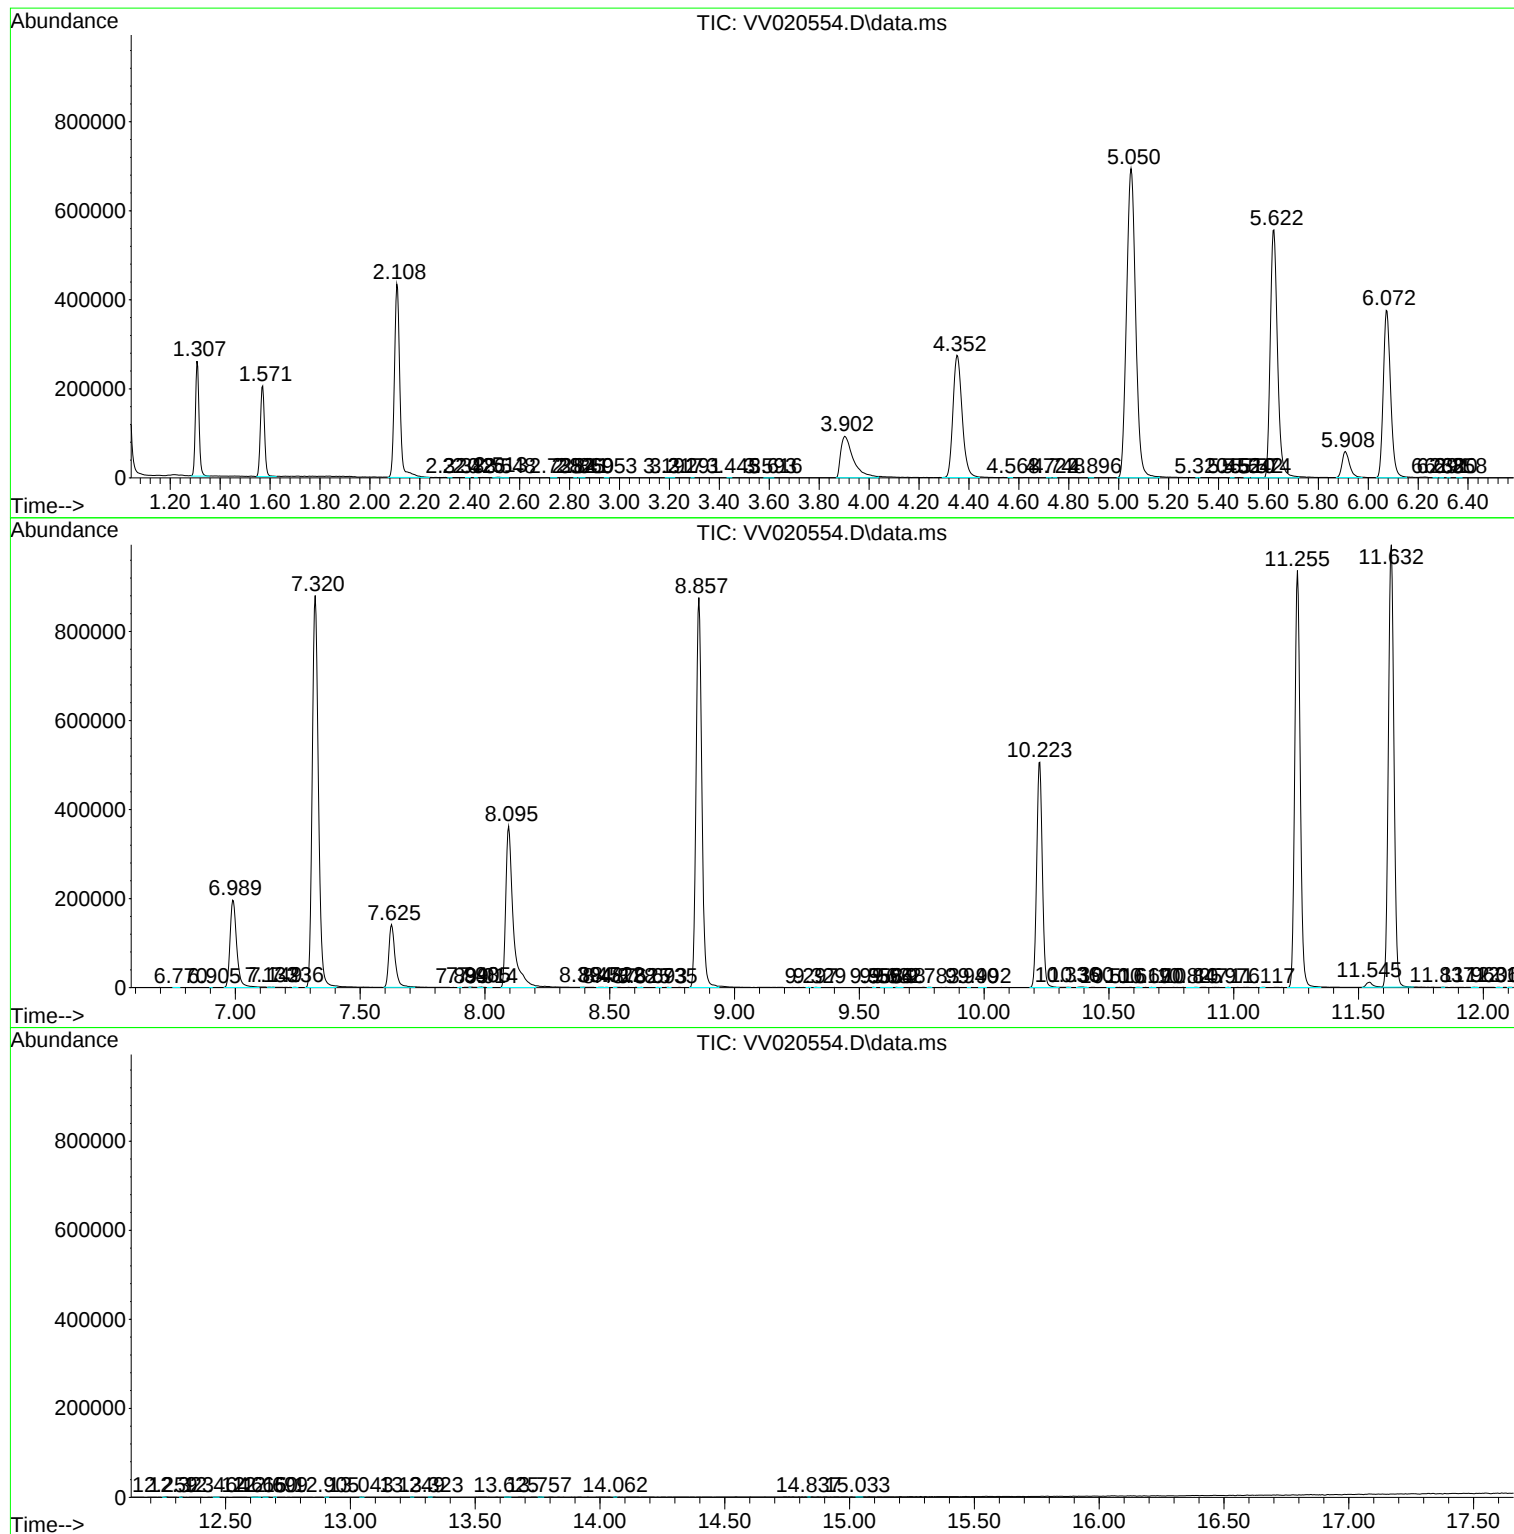

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
Data File : VV020554.D
Acq On : 11 Mar 2021 22:50
Operator : SY/MD
Sample : M1633-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B75

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
Data File : VV020554.D
Acq On : 11 Mar 2021 22:50
Operator : SY/MD
Sample : M1633-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B75

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
