

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
 Data File : VV020555.D
 Acq On : 11 Mar 2021 23:14
 Operator : SY/MD
 Sample : M1633-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B76

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M

Title : VOC Analysis

Signal : TIC: VV020555.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	96	rVB	259636	260352	14.71%	1.868%
2	1.571	157	165	180	rVB	201416	232332	13.13%	1.667%
3	1.973	288	290	293	rBV5	617	318	0.02%	0.002%
4	2.108	321	332	344	rBV	439568	632662	35.75%	4.539%
5	2.339	401	404	406	rBV2	271	179	0.01%	0.001%
6	2.420	427	429	432	rVV3	373	225	0.01%	0.002%
7	2.487	447	450	453	rBV	375	269	0.02%	0.002%
8	2.513	453	458	465	rVB3	1025	1225	0.07%	0.009%
9	2.625	489	493	497	rBV3	433	333	0.02%	0.002%
10	2.648	498	500	506	rVB2	254	159	0.01%	0.001%
11	2.696	511	515	519	rVB2	316	253	0.01%	0.002%
12	2.722	520	523	526	rBV2	238	167	0.01%	0.001%
13	3.137	649	652	657	rVB2	186	147	0.01%	0.001%
14	3.207	672	674	680	rVB2	175	148	0.01%	0.001%
15	3.252	684	688	690	rBV2	209	148	0.01%	0.001%
16	3.391	727	731	739	rBV	181	310	0.02%	0.002%
17	3.629	801	805	807	rBV2	221	207	0.01%	0.001%
18	3.712	827	831	834	rBV	333	161	0.01%	0.001%
19	3.821	863	865	871	rVB2	344	365	0.02%	0.003%
20	3.854	871	875	879	rBV2	247	299	0.02%	0.002%
21	3.905	879	891	925	rBV2	88769	317728	17.95%	2.280%
22	4.211	982	986	988	rBV3	349	299	0.02%	0.002%
23	4.352	1013	1030	1065	rBV	277004	703154	39.73%	5.045%
24	4.558	1090	1094	1097	rBV3	388	351	0.02%	0.003%
25	4.577	1097	1100	1107	rVB3	435	436	0.02%	0.003%
26	4.786	1162	1165	1172	rVB2	289	261	0.01%	0.002%
27	4.828	1172	1178	1181	rBV	187	210	0.01%	0.002%
28	4.860	1185	1188	1195	rVB2	184	223	0.01%	0.002%
29	4.982	1224	1226	1229	rBV	263	199	0.01%	0.001%
30	5.050	1230	1247	1274	rBV2	697832	1769734	100.00%	12.698%
31	5.288	1319	1321	1326	rVB3	515	243	0.01%	0.002%
32	5.310	1326	1328	1333	rVB2	242	139	0.01%	0.001%
33	5.487	1378	1383	1387	rVB3	418	391	0.02%	0.003%
34	5.561	1400	1406	1410	rVB2	291	348	0.02%	0.002%
35	5.622	1411	1425	1457	rBV	549871	1109545	62.70%	7.961%
36	5.841	1491	1493	1499	rVB3	464	374	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW031221\
 Data File : VW020555.D
 Acq On : 11 Mar 2021 23:14
 Operator : SY/MD
 Sample : M1633-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B76

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
 Title : VOC Analysis

37	5.908	1502	1514	1539	rBV	58255	123036	6.95%	0.883%
38	6.027	1548	1551	1552	rBV2	301	174	0.01%	0.001%
39	6.072	1552	1565	1590	rVV	371780	766591	43.32%	5.500%
40	6.220	1604	1611	1612	rBV4	860	921	0.05%	0.007%
41	6.307	1637	1638	1641	rVB	353	162	0.01%	0.001%
42	6.673	1749	1752	1755	rVV2	241	166	0.01%	0.001%
43	6.702	1758	1761	1765	rBV2	216	174	0.01%	0.001%
44	6.950	1833	1838	1839	rBV	265	215	0.01%	0.002%
45	6.989	1839	1850	1876	rVV	200284	362097	20.46%	2.598%
46	7.146	1897	1899	1902	rBV2	290	161	0.01%	0.001%
47	7.236	1924	1927	1933	rVB3	276	288	0.02%	0.002%
48	7.320	1940	1953	1985	rBV	873073	1520583	85.92%	10.910%
49	7.625	2038	2048	2069	rBV	139710	245247	13.86%	1.760%
50	7.857	2116	2120	2123	rBV2	414	275	0.02%	0.002%
51	7.940	2142	2146	2153	rBV2	505	585	0.03%	0.004%
52	7.989	2155	2161	2166	rVB5	1026	1105	0.06%	0.008%
53	8.059	2178	2183	2184	rBV2	178	132	0.01%	0.001%
54	8.095	2184	2194	2228	rBV2	366163	746492	42.18%	5.356%
55	8.390	2284	2286	2290	rVB	348	215	0.01%	0.002%
56	8.722	2386	2389	2393	rBV2	169	147	0.01%	0.001%
57	8.857	2418	2431	2458	rBV	872921	1386006	78.32%	9.944%
58	9.046	2486	2490	2497	rVB4	337	409	0.02%	0.003%
59	9.127	2512	2515	2519	rBV2	337	238	0.01%	0.002%
60	9.246	2549	2552	2555	rBV	242	138	0.01%	0.001%
61	9.316	2571	2574	2578	rVB2	172	133	0.01%	0.001%
62	9.477	2620	2624	2627	rBV	312	286	0.02%	0.002%
63	9.757	2709	2711	2714	rVB	255	147	0.01%	0.001%
64	9.844	2734	2738	2745	rBV2	270	342	0.02%	0.002%
65	9.931	2761	2765	2768	rBV2	250	190	0.01%	0.001%
66	10.223	2843	2856	2881	rBV	514177	803376	45.40%	5.764%
67	10.387	2901	2907	2919	rVB3	1264	1867	0.11%	0.013%
68	10.561	2959	2961	2964	rBV2	164	132	0.01%	0.001%
69	10.676	2993	2997	3000	rBV2	181	189	0.01%	0.001%
70	10.718	3007	3010	3015	rVB2	338	256	0.01%	0.002%
71	10.792	3027	3033	3036	rBV	195	237	0.01%	0.002%
72	10.847	3047	3050	3056	rBV	171	154	0.01%	0.001%
73	10.924	3071	3074	3076	rBV2	230	148	0.01%	0.001%
74	10.956	3079	3084	3087	rBV2	257	241	0.01%	0.002%
75	11.021	3100	3104	3105	rBV	196	136	0.01%	0.001%
76	11.104	3126	3130	3137	rBV2	216	316	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
 Data File : VV020555.D
 Acq On : 11 Mar 2021 23:14
 Operator : SY/MD
 Sample : M1633-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B76

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M

Title : VOC Analysis

77	11.255	3165	3177	3198	rBV	902603	1393627	78.75%	9.999%
78	11.631	3280	3294	3315	rBV	989869	1540862	87.07%	11.055%
79	11.892	3372	3375	3379	rVB2	252	181	0.01%	0.001%
80	11.966	3396	3398	3402	rBV2	215	170	0.01%	0.001%
81	12.258	3487	3489	3494	rVB2	283	178	0.01%	0.001%
82	12.287	3495	3498	3501	rBV2	399	244	0.01%	0.002%
83	12.445	3544	3547	3549	rVB2	325	177	0.01%	0.001%
84	12.500	3561	3564	3569	rBV2	289	230	0.01%	0.002%
85	12.647	3608	3610	3615	rBV3	256	239	0.01%	0.002%
86	12.766	3645	3647	3652	rVB3	314	256	0.01%	0.002%
87	12.811	3659	3661	3665	rVB	310	179	0.01%	0.001%
88	12.837	3665	3669	3672	rBV2	250	275	0.02%	0.002%
89	12.879	3679	3682	3684	rBV2	215	147	0.01%	0.001%
90	12.914	3691	3693	3701	rVB3	319	392	0.02%	0.003%
91	13.274	3802	3805	3808	rVB2	400	259	0.01%	0.002%
92	13.291	3808	3810	3813	rBV	337	260	0.01%	0.002%
93	13.387	3837	3840	3844	rBV2	355	225	0.01%	0.002%
94	13.410	3844	3847	3849	rBV2	304	201	0.01%	0.001%
95	13.493	3871	3873	3877	rBV2	266	186	0.01%	0.001%
96	13.516	3877	3880	3882	rVV4	289	170	0.01%	0.001%
97	13.628	3911	3915	3918	rBV2	368	375	0.02%	0.003%
98	14.152	4073	4078	4079	rBV2	436	381	0.02%	0.003%
99	15.249	4416	4419	4421	rBV	517	317	0.02%	0.002%
100	15.493	4492	4495	4497	rBV3	734	523	0.03%	0.004%


Sum of corrected areas: 13937655

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
Data File : VV020555.D
Acq On : 11 Mar 2021 23:14
Operator : SY/MD
Sample : M1633-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B76

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

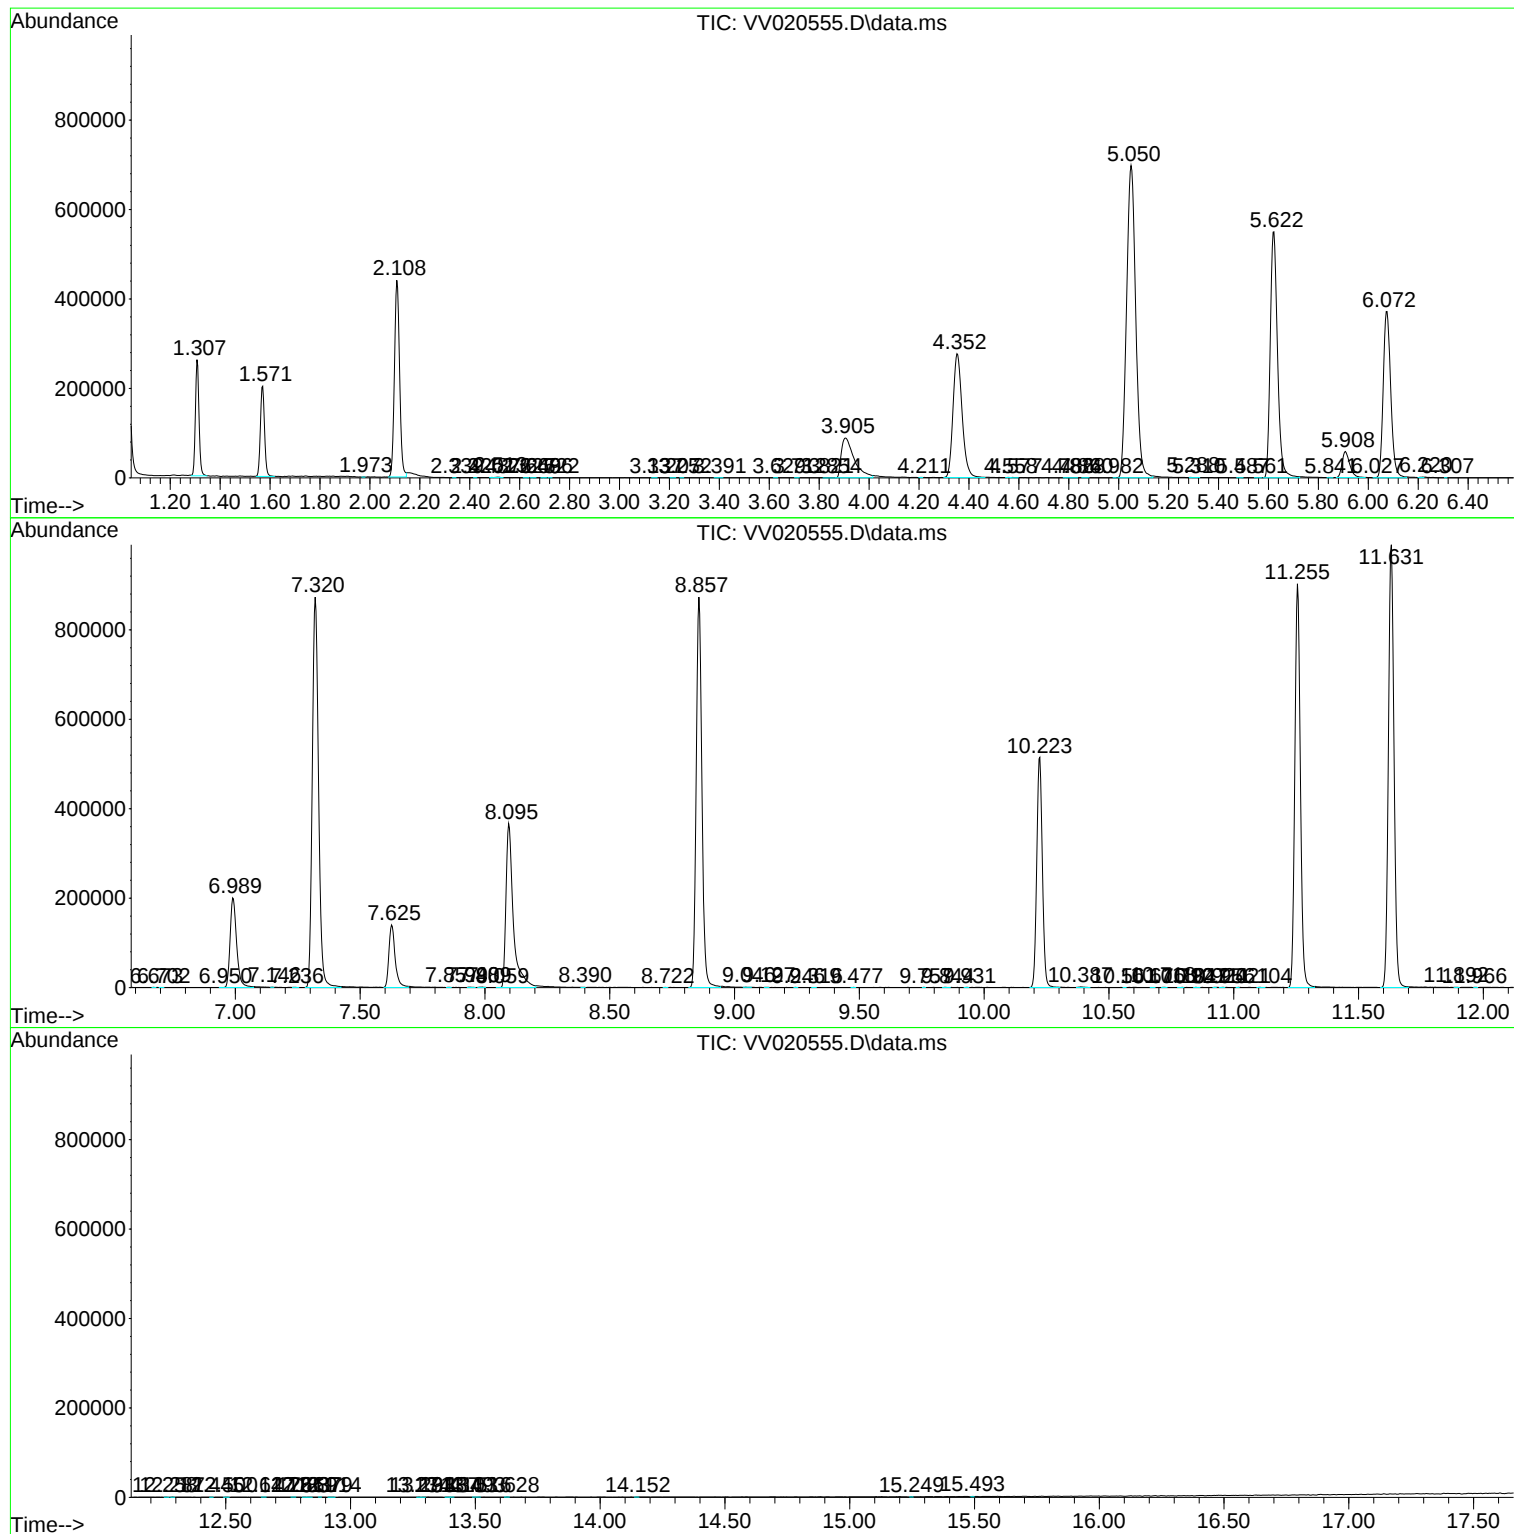

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
Data File : VV020555.D
Acq On : 11 Mar 2021 23:14
Operator : SY/MD
Sample : M1633-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B76

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
Data File : VV020555.D
Acq On : 11 Mar 2021 23:14
Operator : SY/MD
Sample : M1633-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B76

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
