

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
 Data File : VV020556.D
 Acq On : 11 Mar 2021 23:38
 Operator : SY/MD
 Sample : M1633-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B78

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M

Title : VOC Analysis

Signal : TIC: VV020556.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	99	rVB	265089	260531	14.82%	1.868%
2	1.568	157	164	184	rVB	202061	233082	13.25%	1.671%
3	2.108	321	332	367	rVB	436950	654938	37.24%	4.696%
4	2.436	431	434	438	rBV2	313	270	0.02%	0.002%
5	2.494	447	452	453	rBV2	514	337	0.02%	0.002%
6	2.510	455	457	461	rVB2	670	474	0.03%	0.003%
7	2.596	479	484	485	rBV	245	229	0.01%	0.002%
8	2.754	527	533	535	rBV2	235	254	0.01%	0.002%
9	2.767	535	537	541	rVB	205	148	0.01%	0.001%
10	2.950	587	594	597	rBV2	202	243	0.01%	0.002%
11	3.069	626	631	635	rVB2	320	376	0.02%	0.003%
12	3.098	635	640	642	rBV	254	301	0.02%	0.002%
13	3.191	665	669	673	rBV2	203	221	0.01%	0.002%
14	3.320	705	709	712	rVB2	239	178	0.01%	0.001%
15	3.346	712	717	718	rBV2	257	202	0.01%	0.001%
16	3.590	786	793	799	rVB2	245	332	0.02%	0.002%
17	3.635	803	807	810	rBV2	221	185	0.01%	0.001%
18	3.754	840	844	849	rBV2	160	155	0.01%	0.001%
19	3.902	878	890	937	rBV	92224	328685	18.69%	2.357%
20	4.133	959	962	966	rBV2	382	417	0.02%	0.003%
21	4.275	1004	1006	1009	rBV	226	153	0.01%	0.001%
22	4.352	1013	1030	1060	rVV	273381	700968	39.86%	5.026%
23	4.600	1103	1107	1109	rBV2	366	291	0.02%	0.002%
24	4.645	1118	1121	1123	rBV2	403	295	0.02%	0.002%
25	4.709	1138	1141	1144	rVB	390	200	0.01%	0.001%
26	4.738	1147	1150	1155	rVV3	297	203	0.01%	0.001%
27	4.780	1160	1163	1167	rVV3	332	242	0.01%	0.002%
28	4.870	1188	1191	1195	rVB2	213	153	0.01%	0.001%
29	4.908	1199	1203	1209	rVB3	232	205	0.01%	0.001%
30	5.050	1230	1247	1280	rBV2	690694	1758543	100.00%	12.609%
31	5.500	1384	1387	1390	rVB2	192	157	0.01%	0.001%
32	5.622	1411	1425	1455	rBV	554089	1117918	63.57%	8.016%
33	5.860	1497	1499	1502	rVB3	408	152	0.01%	0.001%
34	5.908	1502	1514	1539	rBV	58370	121218	6.89%	0.869%
35	6.072	1551	1565	1592	rBV	369467	753371	42.84%	5.402%
36	6.374	1652	1659	1661	rBV	148	163	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW031221\
 Data File : VW020556.D
 Acq On : 11 Mar 2021 23:38
 Operator : SY/MD
 Sample : M1633-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B78

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
 Title : VOC Analysis

37	6.432	1671	1677	1680	rBV2	264	275	0.02%	0.002%
38	6.458	1683	1685	1691	rVB2	170	157	0.01%	0.001%
39	6.519	1702	1704	1708	rVB	236	171	0.01%	0.001%
40	6.545	1708	1712	1716	rBV	408	379	0.02%	0.003%
41	6.886	1814	1818	1820	rBV	196	157	0.01%	0.001%
42	6.989	1839	1850	1872	rBV	195250	360577	20.50%	2.585%
43	7.204	1913	1917	1919	rBV3	303	233	0.01%	0.002%
44	7.223	1919	1923	1928	rBV3	403	419	0.02%	0.003%
45	7.320	1940	1953	1981	rBV	877782	1511107	85.93%	10.835%
46	7.625	2037	2048	2070	rBV	140634	244669	13.91%	1.754%
47	7.886	2124	2129	2133	rBV2	213	211	0.01%	0.002%
48	7.911	2133	2137	2140	rBV	324	206	0.01%	0.001%
49	7.931	2140	2143	2144	rBV	282	154	0.01%	0.001%
50	7.979	2154	2158	2159	rBV	671	424	0.02%	0.003%
51	8.095	2183	2194	2246	rBV2	363708	751185	42.72%	5.386%
52	8.329	2264	2267	2270	rVB3	711	432	0.02%	0.003%
53	8.355	2270	2275	2277	rVB3	611	433	0.02%	0.003%
54	8.390	2282	2286	2290	rBV2	336	283	0.02%	0.002%
55	8.644	2362	2365	2372	rVB2	227	210	0.01%	0.002%
56	8.857	2418	2431	2457	rBV	867213	1386282	78.83%	9.940%
57	9.111	2507	2510	2516	rVB2	344	319	0.02%	0.002%
58	9.143	2516	2520	2522	rBV	357	250	0.01%	0.002%
59	9.419	2601	2606	2614	rBV2	260	411	0.02%	0.003%
60	9.532	2636	2641	2645	rBV	252	281	0.02%	0.002%
61	9.898	2750	2755	2759	rBV2	305	364	0.02%	0.003%
62	10.001	2781	2787	2789	rBV	388	398	0.02%	0.003%
63	10.223	2843	2856	2874	rBV	509864	798826	45.43%	5.728%
64	10.384	2901	2906	2907	rBV2	803	545	0.03%	0.004%
65	10.435	2918	2922	2925	rBV	362	348	0.02%	0.002%
66	10.464	2928	2931	2936	rVV2	243	227	0.01%	0.002%
67	10.818	3036	3041	3043	rVV	174	158	0.01%	0.001%
68	11.040	3105	3110	3116	rBV2	171	230	0.01%	0.002%
69	11.152	3141	3145	3149	rVB2	278	206	0.01%	0.001%
70	11.178	3149	3153	3156	rVB3	566	439	0.02%	0.003%
71	11.197	3156	3159	3163	rVB3	270	171	0.01%	0.001%
72	11.255	3163	3177	3200	rBV	920070	1403988	79.84%	10.067%
73	11.445	3234	3236	3243	rVV2	255	303	0.02%	0.002%
74	11.474	3243	3245	3248	rVB3	437	242	0.01%	0.002%
75	11.493	3248	3251	3254	rBV	328	253	0.01%	0.002%
76	11.509	3254	3256	3260	rVB3	379	204	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
 Data File : VV020556.D
 Acq On : 11 Mar 2021 23:38
 Operator : SY/MD
 Sample : M1633-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B78

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M

Title : VOC Analysis

77	11.631	3281	3294	3313	rBV	992949	1536822	87.39%	11.019%
78	11.811	3343	3350	3352	rBV2	271	377	0.02%	0.003%
79	11.908	3377	3380	3384	rBV4	270	194	0.01%	0.001%
80	11.963	3392	3397	3403	rVB	331	408	0.02%	0.003%
81	12.204	3463	3472	3480	rBV2	319	637	0.04%	0.005%
82	12.381	3524	3527	3531	rBV2	178	172	0.01%	0.001%
83	12.596	3590	3594	3596	rBV	242	212	0.01%	0.002%
84	12.654	3610	3612	3620	rVB2	555	570	0.03%	0.004%
85	12.692	3620	3624	3629	rBV2	272	186	0.01%	0.001%
86	12.824	3662	3665	3672	rVB2	524	510	0.03%	0.004%
87	12.860	3672	3676	3678	rBV	406	317	0.02%	0.002%
88	12.975	3708	3712	3714	rBV3	367	303	0.02%	0.002%
89	13.020	3724	3726	3732	rBV3	222	190	0.01%	0.001%
90	13.345	3824	3827	3830	rBV2	435	337	0.02%	0.002%
91	13.397	3839	3843	3845	rBV3	316	231	0.01%	0.002%
92	13.461	3858	3863	3868	rBV2	325	392	0.02%	0.003%
93	13.500	3871	3875	3878	rVV2	300	326	0.02%	0.002%
94	13.522	3881	3882	3891	rVB3	610	650	0.04%	0.005%
95	13.744	3948	3951	3956	rBV2	285	376	0.02%	0.003%
96	13.834	3976	3979	3981	rBV2	354	232	0.01%	0.002%
97	14.557	4202	4204	4207	rVB	359	164	0.01%	0.001%
98	14.895	4307	4309	4313	rBV	459	244	0.01%	0.002%
99	15.085	4365	4368	4373	rVB4	790	629	0.04%	0.005%
100	15.364	4453	4455	4457	rBV	480	254	0.01%	0.002%




Sum of corrected areas: 13946650

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
Data File : VV020556.D
Acq On : 11 Mar 2021 23:38
Operator : SY/MD
Sample : M1633-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B78

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

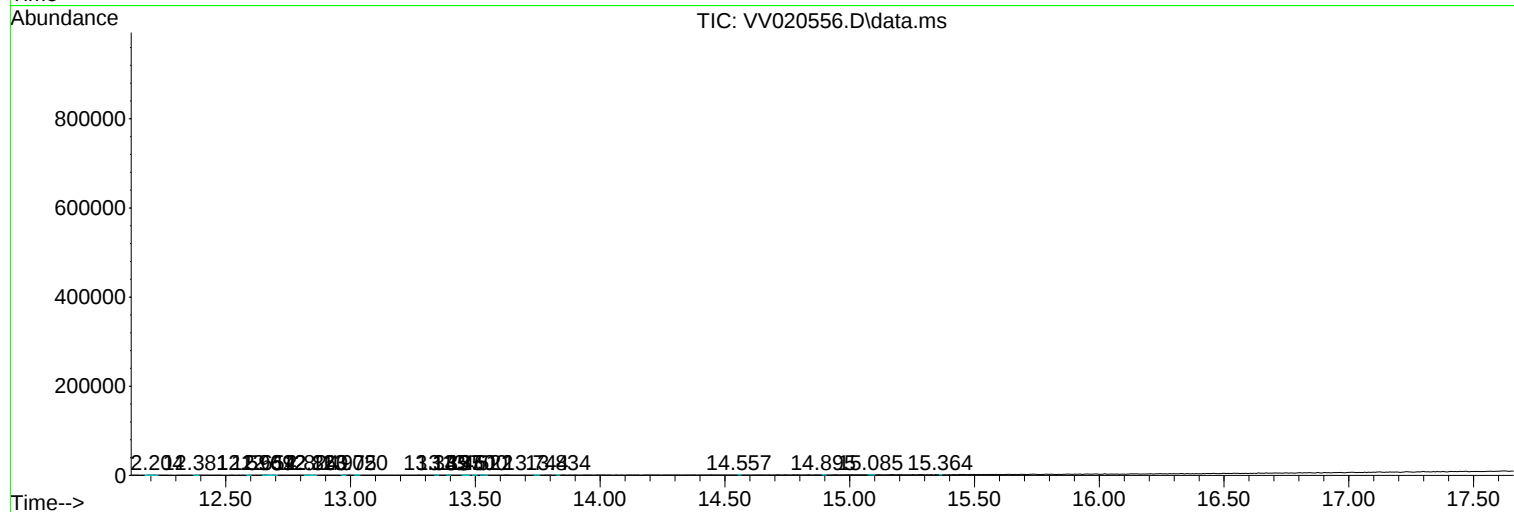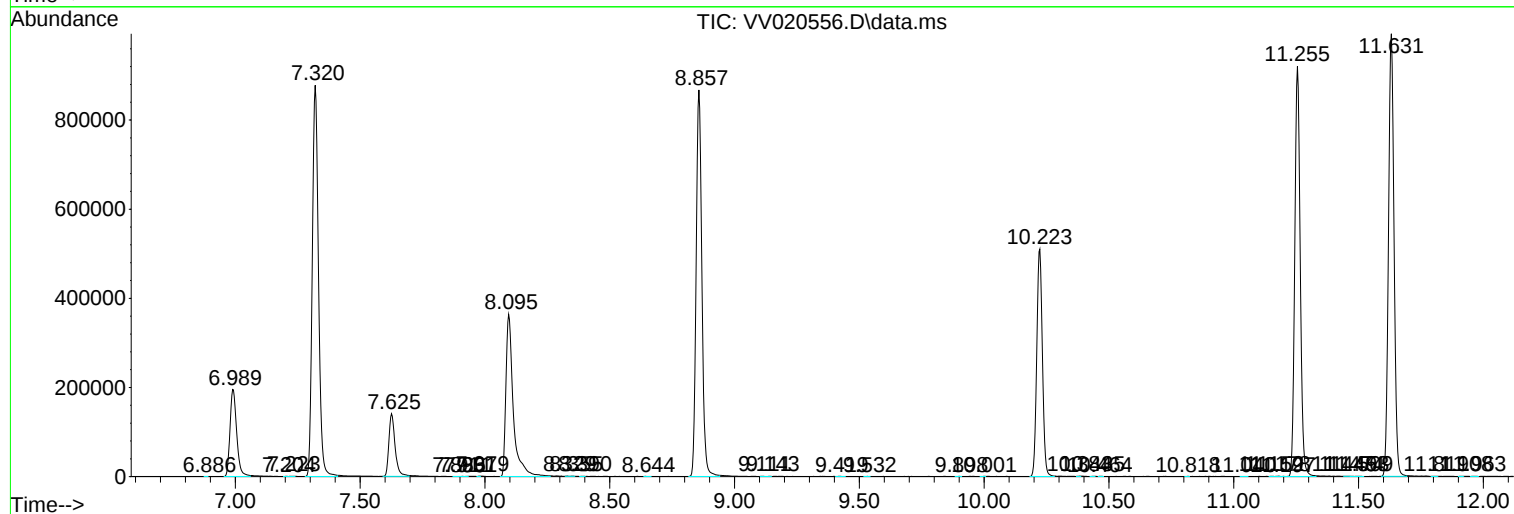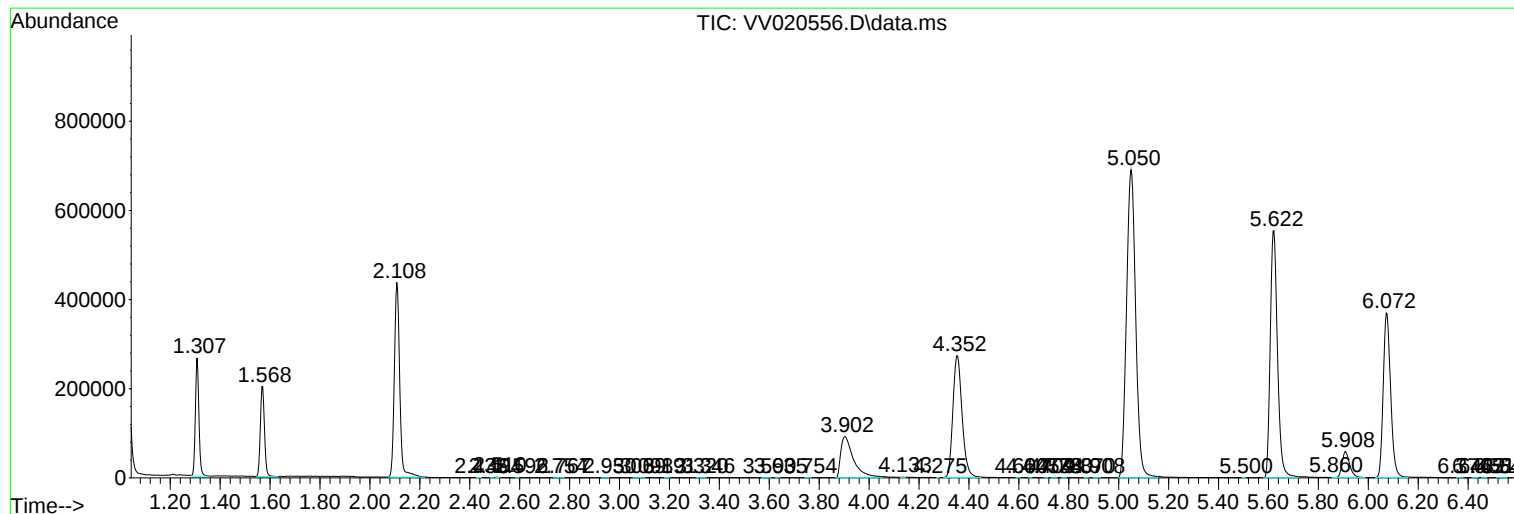

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
Data File : VV020556.D
Acq On : 11 Mar 2021 23:38
Operator : SY/MD
Sample : M1633-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B78

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
Data File : VV020556.D
Acq On : 11 Mar 2021 23:38
Operator : SY/MD
Sample : M1633-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B78

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
