

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
 Data File : VV020558.D
 Acq On : 12 Mar 2021 00:25
 Operator : SY/MD
 Sample : M1633-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B83

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M

Title : VOC Analysis

Signal : TIC: VV020558.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	96	rVB	255496	255929	14.82%	1.861%
2	1.568	156	164	178	rBV	199869	228058	13.21%	1.659%
3	2.108	321	332	365	rBV	425269	643137	37.25%	4.678%
4	2.282	382	386	387	rBV	442	285	0.02%	0.002%
5	2.330	398	401	404	rBV3	464	351	0.02%	0.003%
6	2.507	452	456	465	rVB6	1260	1823	0.11%	0.013%
7	2.619	484	491	494	rBV3	506	585	0.03%	0.004%
8	2.700	514	516	519	rVB2	256	136	0.01%	0.001%
9	2.719	519	522	524	rBV2	205	153	0.01%	0.001%
10	2.835	555	558	562	rBV	211	228	0.01%	0.002%
11	3.118	643	646	650	rBV	194	155	0.01%	0.001%
12	3.195	667	670	678	rVV	283	380	0.02%	0.003%
13	3.381	722	728	733	rBV2	172	249	0.01%	0.002%
14	3.654	806	813	817	rBV	206	285	0.02%	0.002%
15	3.687	821	823	827	rBV2	245	240	0.01%	0.002%
16	3.767	846	848	854	rVB2	162	149	0.01%	0.001%
17	3.809	854	861	866	rVB2	174	248	0.01%	0.002%
18	3.899	877	889	923	rBV	103870	344670	19.96%	2.507%
19	4.272	1003	1005	1008	rVB3	275	159	0.01%	0.001%
20	4.352	1014	1030	1064	rVV	273130	693694	40.18%	5.045%
21	4.542	1086	1089	1092	rVB2	315	181	0.01%	0.001%
22	4.584	1100	1102	1105	rVB2	264	161	0.01%	0.001%
23	4.616	1109	1112	1114	rVB3	337	200	0.01%	0.001%
24	4.642	1114	1120	1121	rBV3	201	182	0.01%	0.001%
25	4.671	1124	1129	1131	rBV4	262	254	0.01%	0.002%
26	4.841	1179	1182	1184	rBV2	422	216	0.01%	0.002%
27	4.863	1188	1189	1196	rVV2	259	206	0.01%	0.001%
28	5.050	1229	1247	1274	rBV2	681133	1726561	100.00%	12.557%
29	5.256	1309	1311	1315	rBV2	284	202	0.01%	0.001%
30	5.426	1361	1364	1366	rBV3	240	161	0.01%	0.001%
31	5.497	1380	1386	1389	rBV4	419	461	0.03%	0.003%
32	5.568	1406	1408	1411	rBV	244	163	0.01%	0.001%
33	5.622	1411	1425	1462	rBV	545580	1096030	63.48%	7.972%
34	5.908	1503	1514	1535	rBV2	51746	105790	6.13%	0.769%
35	6.072	1551	1565	1589	rBV	365937	745808	43.20%	5.424%
36	6.429	1669	1676	1677	rBV	235	173	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW031221\
 Data File : VW020558.D
 Acq On : 12 Mar 2021 00:25
 Operator : SY/MD
 Sample : M1633-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B83

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
 Title : VOC Analysis

37	6.471	1685	1689	1692	rBV2	144	147	0.01%	0.001%
38	6.667	1748	1750	1754	rVB	344	223	0.01%	0.002%
39	6.693	1754	1758	1760	rBV2	247	213	0.01%	0.002%
40	6.818	1791	1797	1800	rBV2	239	260	0.02%	0.002%
41	6.992	1839	1851	1874	rBV	195744	355621	20.60%	2.586%
42	7.127	1891	1893	1897	rVB3	586	350	0.02%	0.003%
43	7.188	1909	1912	1917	rVB2	318	240	0.01%	0.002%
44	7.256	1930	1933	1936	rVB	322	225	0.01%	0.002%
45	7.320	1939	1953	1988	rBV	852785	1482040	85.84%	10.779%
46	7.625	2035	2048	2077	rBV	139273	244209	14.14%	1.776%
47	7.783	2095	2097	2101	rVB3	425	205	0.01%	0.001%
48	7.841	2112	2115	2118	rBV	329	194	0.01%	0.001%
49	7.947	2142	2148	2156	rVB3	739	875	0.05%	0.006%
50	7.985	2156	2160	2167	rVB2	725	667	0.04%	0.005%
51	8.095	2183	2194	2235	rBV2	375974	756487	43.81%	5.502%
52	8.474	2310	2312	2319	rBV2	132	150	0.01%	0.001%
53	8.548	2329	2335	2340	rBV3	267	360	0.02%	0.003%
54	8.619	2354	2357	2358	rBV	328	139	0.01%	0.001%
55	8.857	2419	2431	2454	rBV	851250	1357669	78.63%	9.874%
56	9.066	2493	2496	2499	rBV2	522	274	0.02%	0.002%
57	9.127	2510	2515	2517	rVV3	217	213	0.01%	0.002%
58	9.201	2535	2538	2540	rVV	314	147	0.01%	0.001%
59	9.230	2543	2547	2551	rBV2	249	231	0.01%	0.002%
60	9.249	2551	2553	2558	rVB2	349	207	0.01%	0.002%
61	9.297	2563	2568	2570	rBV	148	141	0.01%	0.001%
62	9.484	2623	2626	2628	rBV	188	138	0.01%	0.001%
63	9.625	2667	2670	2672	rBV	195	136	0.01%	0.001%
64	9.870	2743	2746	2750	rVB2	206	166	0.01%	0.001%
65	9.895	2750	2754	2758	rBV2	261	229	0.01%	0.002%
66	10.223	2843	2856	2876	rBV	512600	804207	46.58%	5.849%
67	10.320	2885	2886	2892	rVB2	476	286	0.02%	0.002%
68	10.387	2900	2907	2916	rBV2	954	1574	0.09%	0.011%
69	10.587	2965	2969	2974	rVB2	254	241	0.01%	0.002%
70	10.612	2974	2977	2980	rBV2	192	141	0.01%	0.001%
71	10.815	3037	3040	3044	rVB2	306	242	0.01%	0.002%
72	11.075	3117	3121	3126	rVB2	227	206	0.01%	0.001%
73	11.162	3142	3148	3149	rBV	235	236	0.01%	0.002%
74	11.255	3165	3177	3199	rBV	906445	1377399	79.78%	10.018%
75	11.436	3231	3233	3237	rVB2	305	145	0.01%	0.001%
76	11.455	3237	3239	3242	rBV2	201	157	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
 Data File : VV020558.D
 Acq On : 12 Mar 2021 00:25
 Operator : SY/MD
 Sample : M1633-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B83

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M

Title : VOC Analysis

77	11.632	3281	3294	3325	rBV	979949	1508538	87.37%	10.972%
78	12.030	3415	3418	3422	rVV2	323	252	0.01%	0.002%
79	12.111	3440	3443	3447	rBV2	179	148	0.01%	0.001%
80	12.230	3478	3480	3484	rVB2	291	159	0.01%	0.001%
81	12.281	3492	3496	3499	rBV2	207	191	0.01%	0.001%
82	12.567	3581	3585	3588	rBV	302	228	0.01%	0.002%
83	12.580	3588	3589	3594	rVB2	199	138	0.01%	0.001%
84	12.667	3612	3616	3618	rBV2	361	238	0.01%	0.002%
85	12.789	3650	3654	3658	rBV2	254	226	0.01%	0.002%
86	12.960	3704	3707	3708	rBV2	331	158	0.01%	0.001%
87	13.159	3763	3769	3771	rBV3	370	426	0.02%	0.003%
88	13.284	3806	3808	3813	rVB4	486	301	0.02%	0.002%
89	13.329	3820	3822	3826	rBV2	240	207	0.01%	0.002%
90	13.455	3857	3861	3866	rBV3	378	369	0.02%	0.003%
91	13.522	3872	3882	3883	rBV	397	545	0.03%	0.004%
92	13.548	3887	3890	3893	rVB2	356	222	0.01%	0.002%
93	13.689	3932	3934	3938	rBV2	337	270	0.02%	0.002%
94	13.760	3953	3956	3959	rVB	353	236	0.01%	0.002%
95	13.783	3959	3963	3967	rBV2	219	222	0.01%	0.002%
96	14.053	4045	4047	4050	rBV	280	193	0.01%	0.001%
97	14.583	4209	4212	4215	rBV	425	251	0.01%	0.002%
98	14.866	4298	4300	4304	rBV2	544	336	0.02%	0.002%
99	15.046	4354	4356	4360	rBV3	423	237	0.01%	0.002%
100	15.310	4435	4438	4441	rBV3	657	530	0.03%	0.004%




Sum of corrected areas: 13749274

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
Data File : VV020558.D
Acq On : 12 Mar 2021 00:25
Operator : SY/MD
Sample : M1633-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B83

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

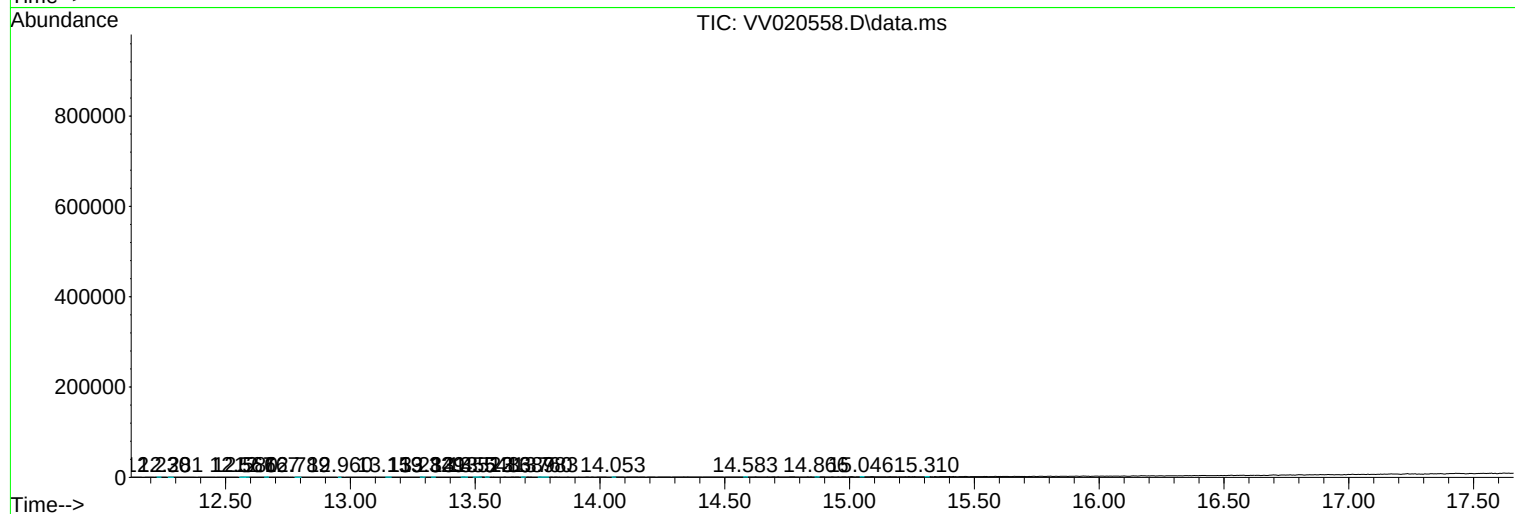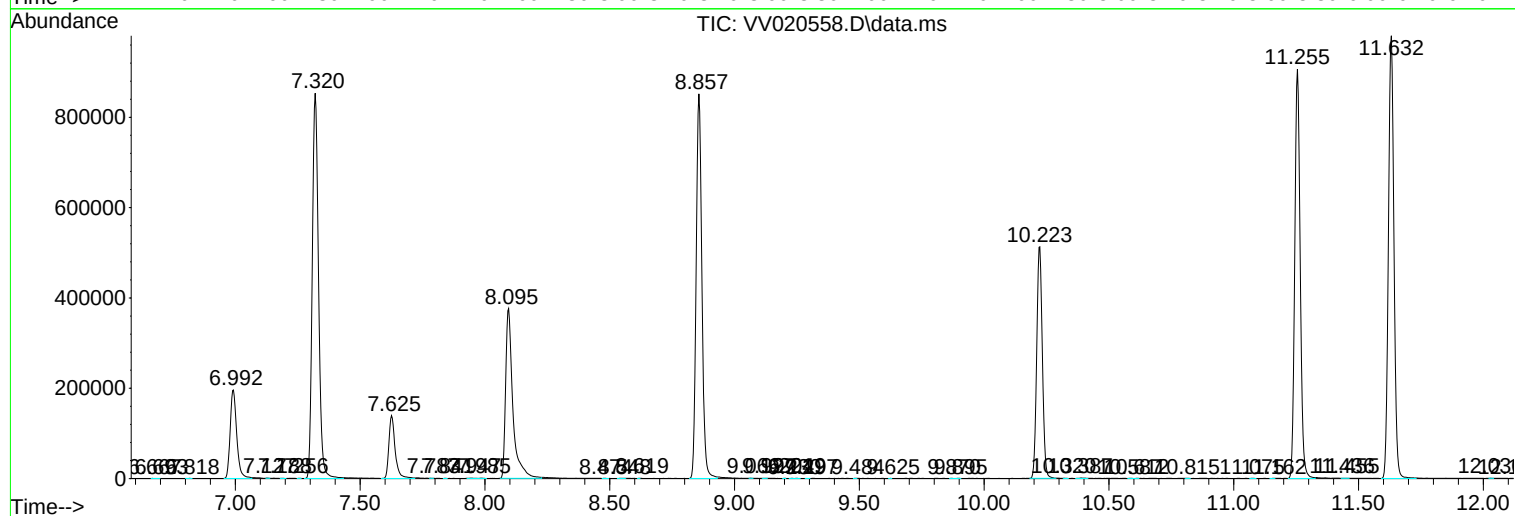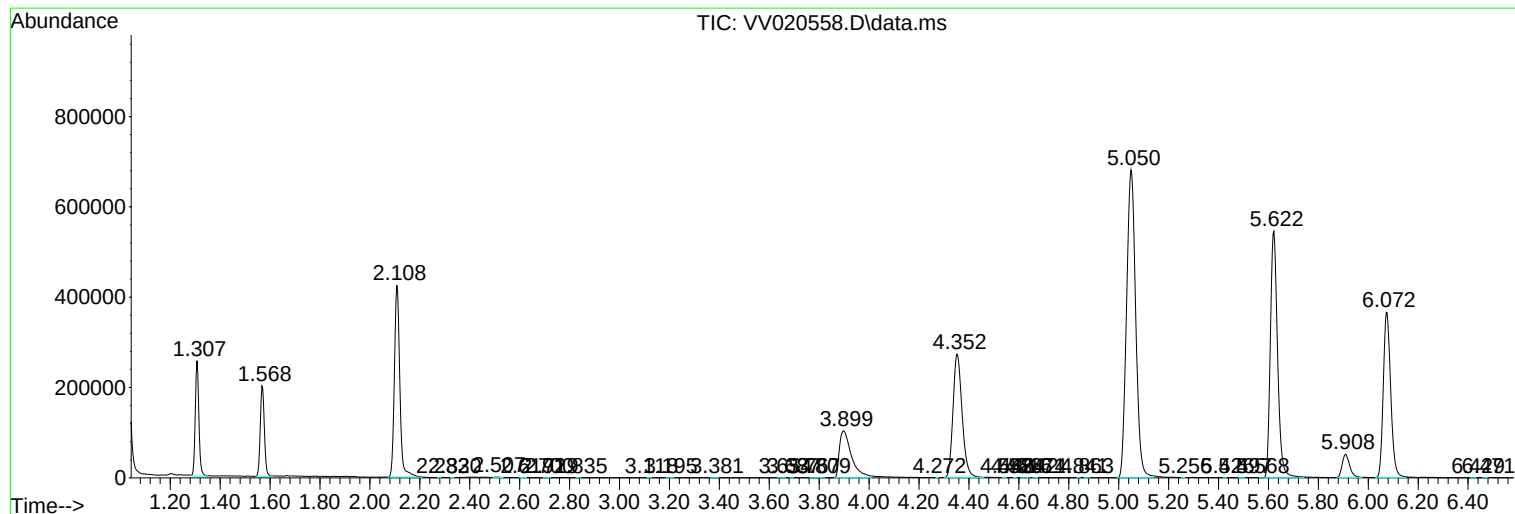

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
Data File : VV020558.D
Acq On : 12 Mar 2021 00:25
Operator : SY/MD
Sample : M1633-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B83

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
Data File : VV020558.D
Acq On : 12 Mar 2021 00:25
Operator : SY/MD
Sample : M1633-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B83

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
