
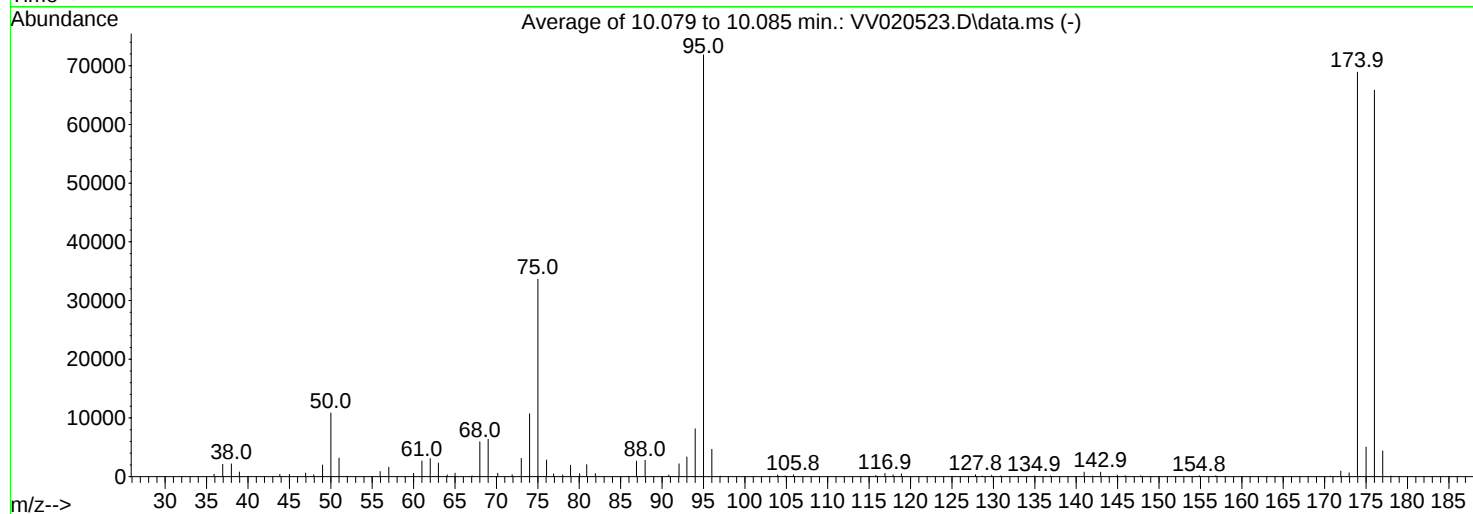


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031221\
Data File : VV020523.D
Acq On : 11 Mar 2021 09:09
Operator : SY/MD
Sample : BFB98
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB98

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
Title : VOC Analysis
Last Update : Fri Mar 12 07:54:21 2021

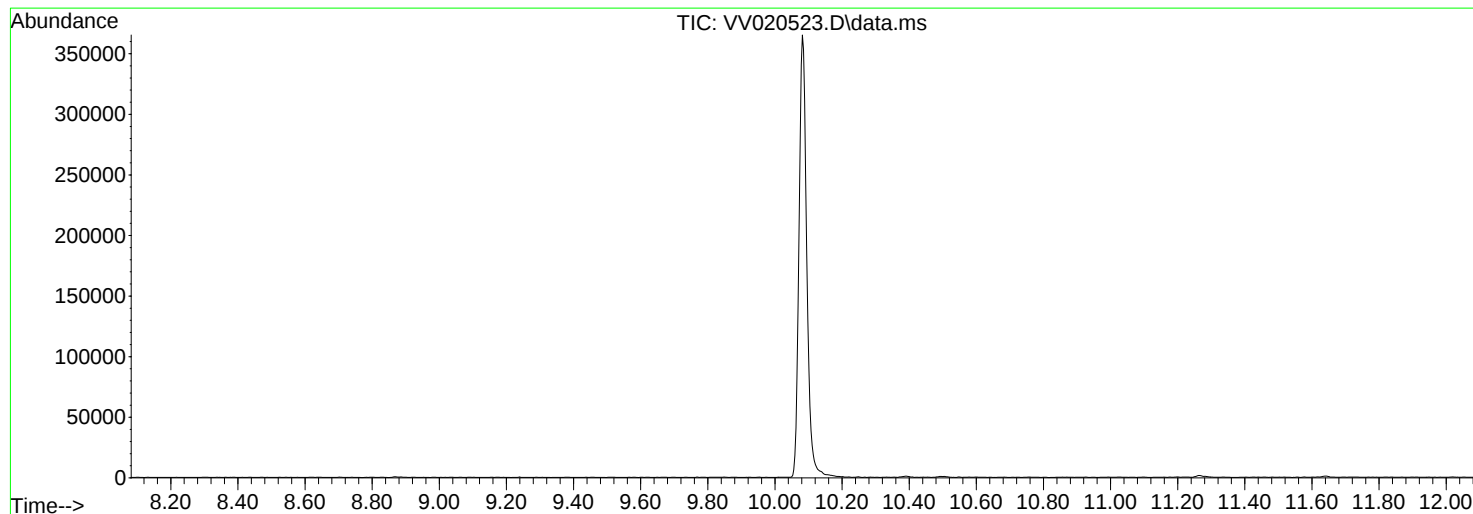

AutoFind: Scans 2811, 2812, 2813; Background Corrected with Scan 2800

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.1	10846	PASS
75	95	30	80	46.8	33635	PASS
95	95	100	100	100.0	71851	PASS
96	95	5	9	6.5	4663	PASS
173	174	0.00	2	1.0	661	PASS
174	95	50	120	95.9	68896	PASS
175	174	5	9	7.3	5045	PASS
176	174	95	101	95.5	65824	PASS
177	176	5	9	6.7	4381	PASS

m/z	Abundance
35.90	358.0
36.90	2112.0
38.00	2170.0
38.90	823.0
39.90	241.0
43.90	693.0
45.00	392.0
47.00	653.0
48.00	340.0
49.00	1869.0
50.00	10470.0
51.00	3205.0
52.00	139.0
54.90	101.0
55.90	825.0
57.00	1685.0
60.00	543.0
61.00	2780.0
62.00	3012.0
63.00	2319.0
64.00	299.0
65.00	614.0
67.00	120.0
68.00	5992.0
69.00	6473.0
70.20	419.0
71.90	327.0
73.00	2939.0
74.00	10298.0
75.00	32616.0
76.10	2755.0
76.90	411.0
78.10	287.0
78.90	1870.0
80.00	573.0
80.90	2020.0
82.00	538.0
86.90	2702.0
87.90	2858.0
90.80	266.0
92.10	2119.0
93.00	3432.0
94.00	7822.0
95.00	69776.0
96.00	4572.0
97.10	122.0
103.90	260.0
104.90	135.0
105.80	282.0
115.80	222.0
116.90	510.0
117.90	318.0
118.90	431.0
127.80	304.0
128.70	130.0
129.80	234.0
130.90	164.0
134.90	146.0
137.00	135.0
141.00	755.0
142.10	104.0
143.00	779.0
144.90	300.0
145.90	120.0
147.80	194.0
154.80	150.0
156.90	161.0
170.70	134.0
172.00	912.0
173.00	659.0
174.00	64856.0
175.00	4840.0
176.00	62408.0
177.00	4207.0
178.00	157.0

Instrument :
MSVOA_V
ClientSampleId :
BFB98

m/z	Abundance
35.90	414.0
36.90	2148.0
38.00	2280.0
38.90	821.0
39.90	190.0
43.90	703.0
45.00	419.0
47.00	615.0
47.90	323.0
49.00	2038.0
50.00	11299.0
51.00	3243.0
51.90	115.0
56.00	918.0
57.00	1667.0
60.00	599.0
61.00	2735.0
62.00	3206.0
63.00	2398.0
64.10	324.0
65.00	674.0
67.10	131.0
68.00	6129.0
69.00	6552.0
70.10	590.0
71.90	328.0
73.00	3308.0
74.00	11047.0
75.00	34792.0
76.00	2921.0
76.90	486.0
78.00	307.0
78.90	1990.0
80.00	530.0
80.90	2071.0
81.90	533.0
85.90	118.0
86.90	2730.0
88.00	2849.0
90.80	277.0
92.00	2263.0
93.00	3467.0
94.00	8392.0
95.00	74408.0
96.00	4774.0
97.00	109.0
104.00	274.0
104.90	135.0
105.80	331.0
115.80	226.0
116.90	548.0
117.90	318.0
118.90	482.0
127.80	329.0
128.60	140.0
129.80	248.0
130.90	163.0
135.00	144.0
136.90	140.0
141.00	767.0
142.00	123.0
142.90	778.0
144.90	287.0
145.90	159.0
147.80	181.0
154.90	184.0
156.90	172.0
170.70	109.0
172.00	979.0
173.00	691.0
174.00	71400.0
175.00	5213.0
176.00	68048.0
177.00	4493.0
178.00	148.0

Instrument :
MSVOA_V
ClientSampleId :
BFB98

m/z	Abundance
35.00	444.0
37.00	2011.0
38.00	2126.0
39.00	740.0
39.00	169.0
43.00	647.0
45.00	385.0
46.00	537.0
47.00	311.0
49.00	2079.0
50.00	10768.0
51.00	3048.0
56.00	884.0
57.00	1510.0
60.00	612.0
61.00	2501.0
62.00	3064.0
63.00	2225.0
64.10	299.0
65.00	553.0
67.10	177.0
68.00	5701.0
69.00	6087.0
70.10	699.0
71.90	321.0
73.00	3114.0
74.00	10756.0
75.00	33496.0
76.00	2875.0
76.90	530.0
77.90	292.0
79.00	1923.0
80.10	479.0
80.90	2034.0
81.90	515.0
85.90	113.0
86.90	2503.0
88.00	2612.0
90.80	310.0
92.00	2127.0
93.00	3203.0
94.00	8239.0
95.00	71368.0
96.00	4643.0
104.00	270.0
104.80	115.0
105.90	343.0
115.80	200.0
116.90	556.0
117.90	257.0
118.90	483.0
127.90	364.0
128.60	120.0
129.80	255.0
130.90	104.0
135.00	134.0
136.80	119.0
140.90	738.0
141.90	123.0
143.00	739.0
145.00	271.0
145.90	176.0
147.80	158.0
154.90	229.0
156.80	171.0
171.90	941.0
172.90	632.0
173.90	70432.0
175.00	5082.0
176.00	67016.0
177.00	4443.0

Instrument :
MSVOA_V
ClientSampleId :
BFB98

m/z	Abundance
39.90	194.0
43.80	306.0

Instrument :
MSVOA_V
ClientSampleId :
BFB98