

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031224\
 Data File : VV034551.D
 Acq On : 12 Mar 2024 10:00
 Operator : SY/MD
 Sample : P1715-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Mar 13 04:57:11 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM030524.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Mar 06 04:17:25 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	11157	0.500	ug/L	-0.02
5) Chlorobenzene-d5	8.800	117	10440	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.191	152	5507	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.280	65	6806	0.569	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	114.000%
4) 1,2-Dichloroethane-d4	4.946	65	4059	0.548	ug/L	-0.02
Spiked Amount	0.500	Range	70 - 130	Recovery	=	110.000%
7) 1,2-Dichloropropane-d6	5.995	67	4596	0.566	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	114.000%
8) Toluene-d8	7.253	98	12927	0.538	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	108.000%
10) 1,1,2,2-Tetrachloroeth...	10.146	84	2985	0.513	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	102.000%
Target Compounds						
13) 1,2-Dibromo-3-chloropr...	12.185	75	44	0.044	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031224\
Data File : VV034551.D
Acq On : 12 Mar 2024 10:00
Operator : SY/MD
Sample : P1715-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Mar 13 04:57:11 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM030524.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Mar 06 04:17:25 2024
Response via : Initial Calibration

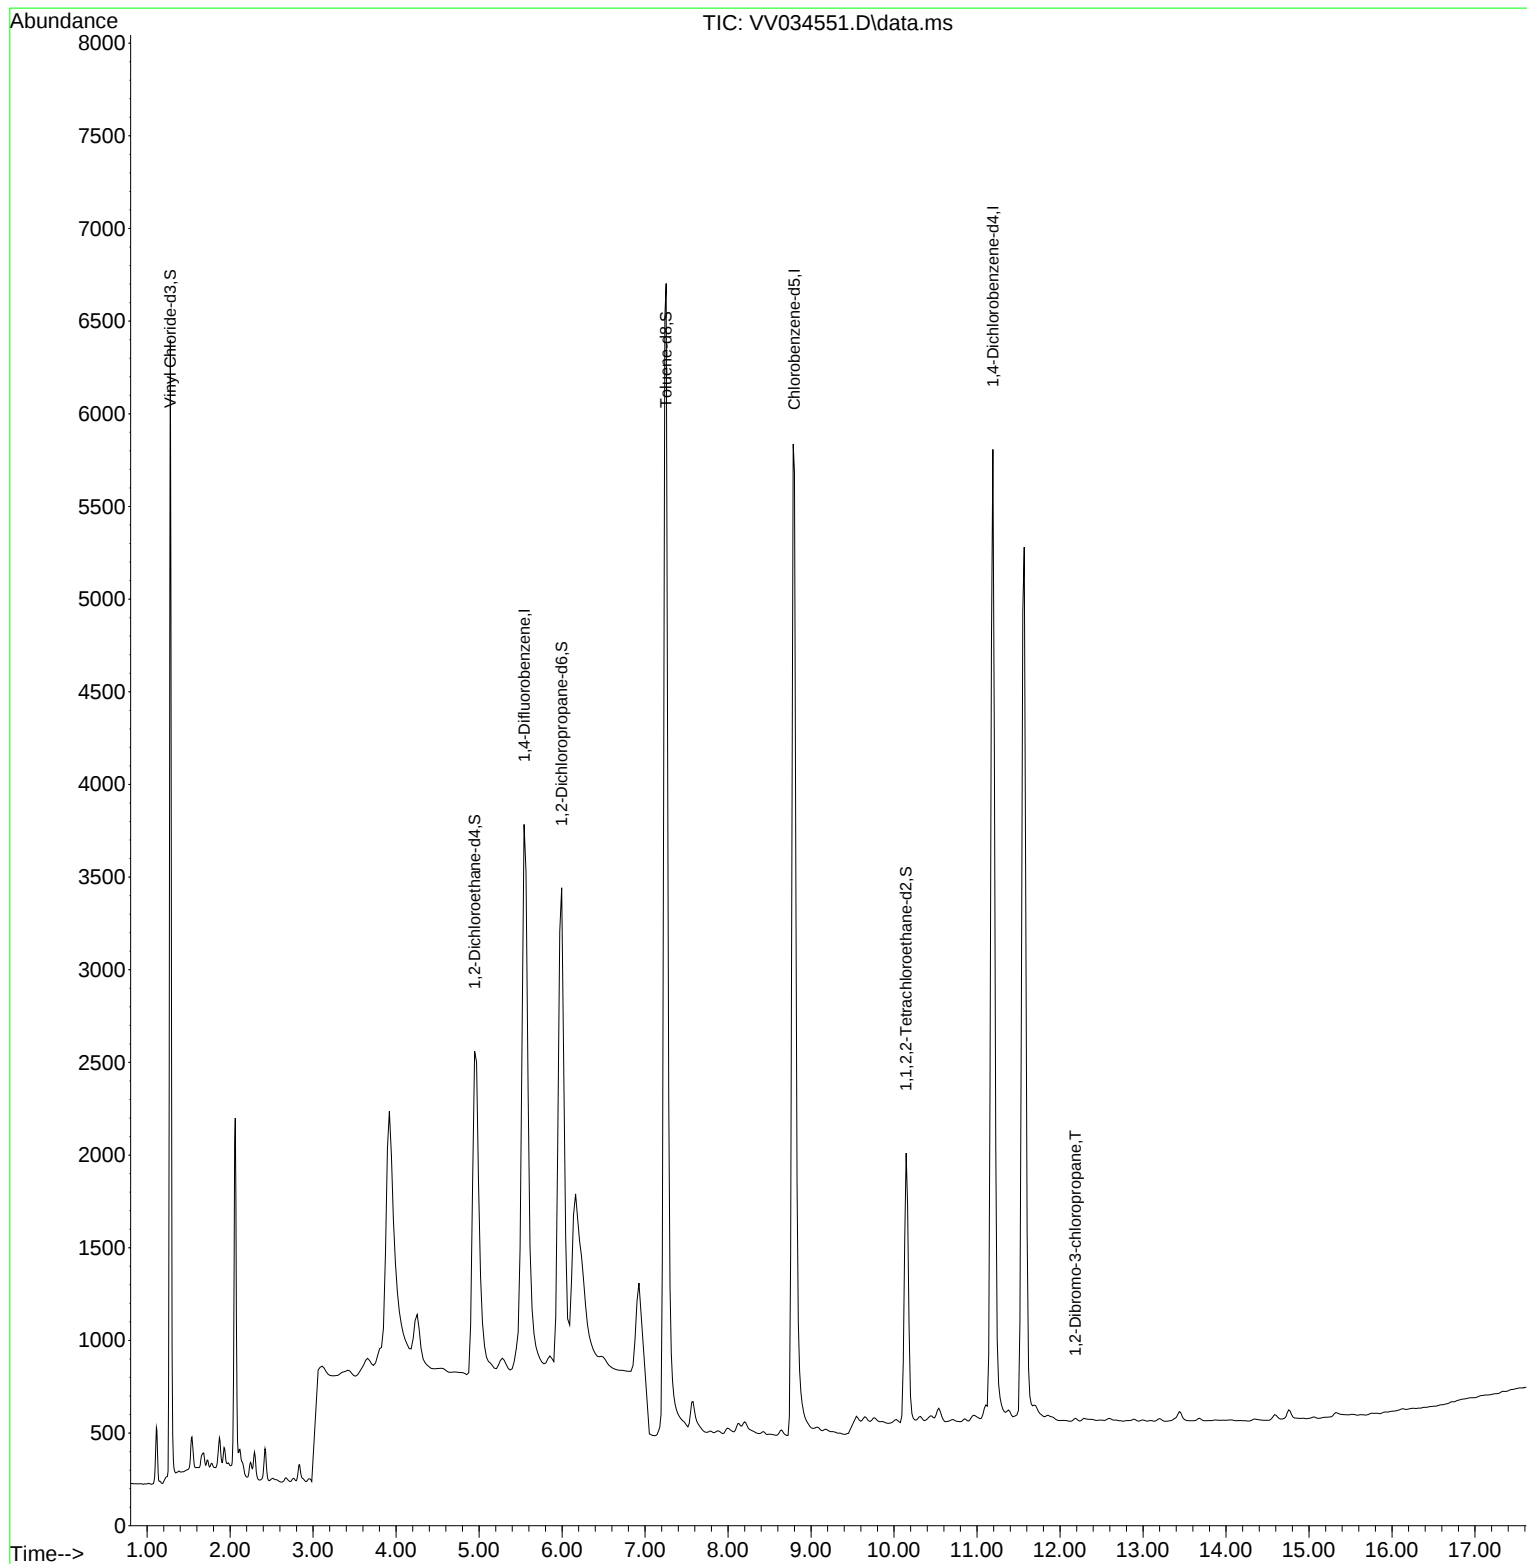

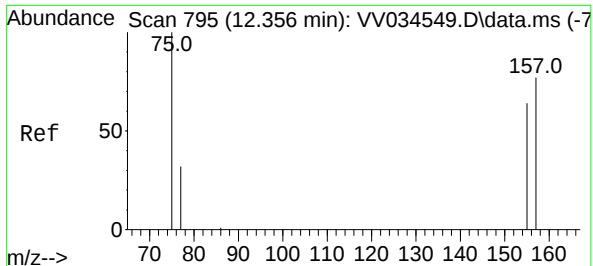

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.044 ug/L
 RT: 12.185 min Scan# 785
 Delta R.T. -0.171 min
 Lab File: VV034551.D
 Acq: 12 Mar 2024 10:00

Instrument :
 MSVOA_V
 ClientSampleId :

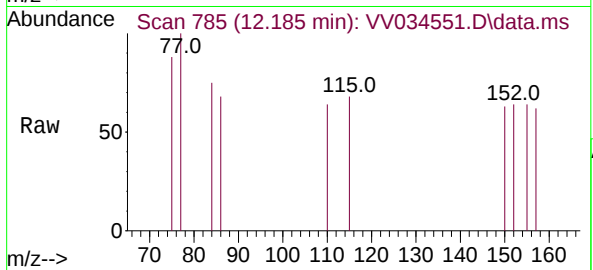

Tgt Ion: 75 Resp: 44

Ion	Ratio	Lower	Upper
75	100		
157	70.4	62.9	94.3
155	73.2	56.2	84.4

