

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031224\
 Data File : VV034553.D
 Acq On : 12 Mar 2024 10:48
 Operator : SY/MD
 Sample : P1715-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Mar 13 04:57:26 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM030524.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Mar 06 04:17:25 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	11014	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.800	117	10288	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.191	152	5414	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.280	65	5897	0.499	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	100.000%
4) 1,2-Dichloroethane-d4	4.969	65	3751	0.513	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	102.000%
7) 1,2-Dichloropropane-d6	5.995	67	3914	0.489	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	98.000%
8) Toluene-d8	7.253	98	11215	0.473	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	94.000%
10) 1,1,2,2-Tetrachloroeth...	10.146	84	2680	0.467	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	94.000%
Target Compounds						
					Qvalue	
12) 1,2,3-Trichloropropane	10.300	75	60	0.013	ug/L #	71
13) 1,2-Dibromo-3-chloropr...	12.185	75	47	0.048	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031224\
Data File : VV034553.D
Acq On : 12 Mar 2024 10:48
Operator : SY/MD
Sample : P1715-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Mar 13 04:57:26 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM030524.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Mar 06 04:17:25 2024
Response via : Initial Calibration

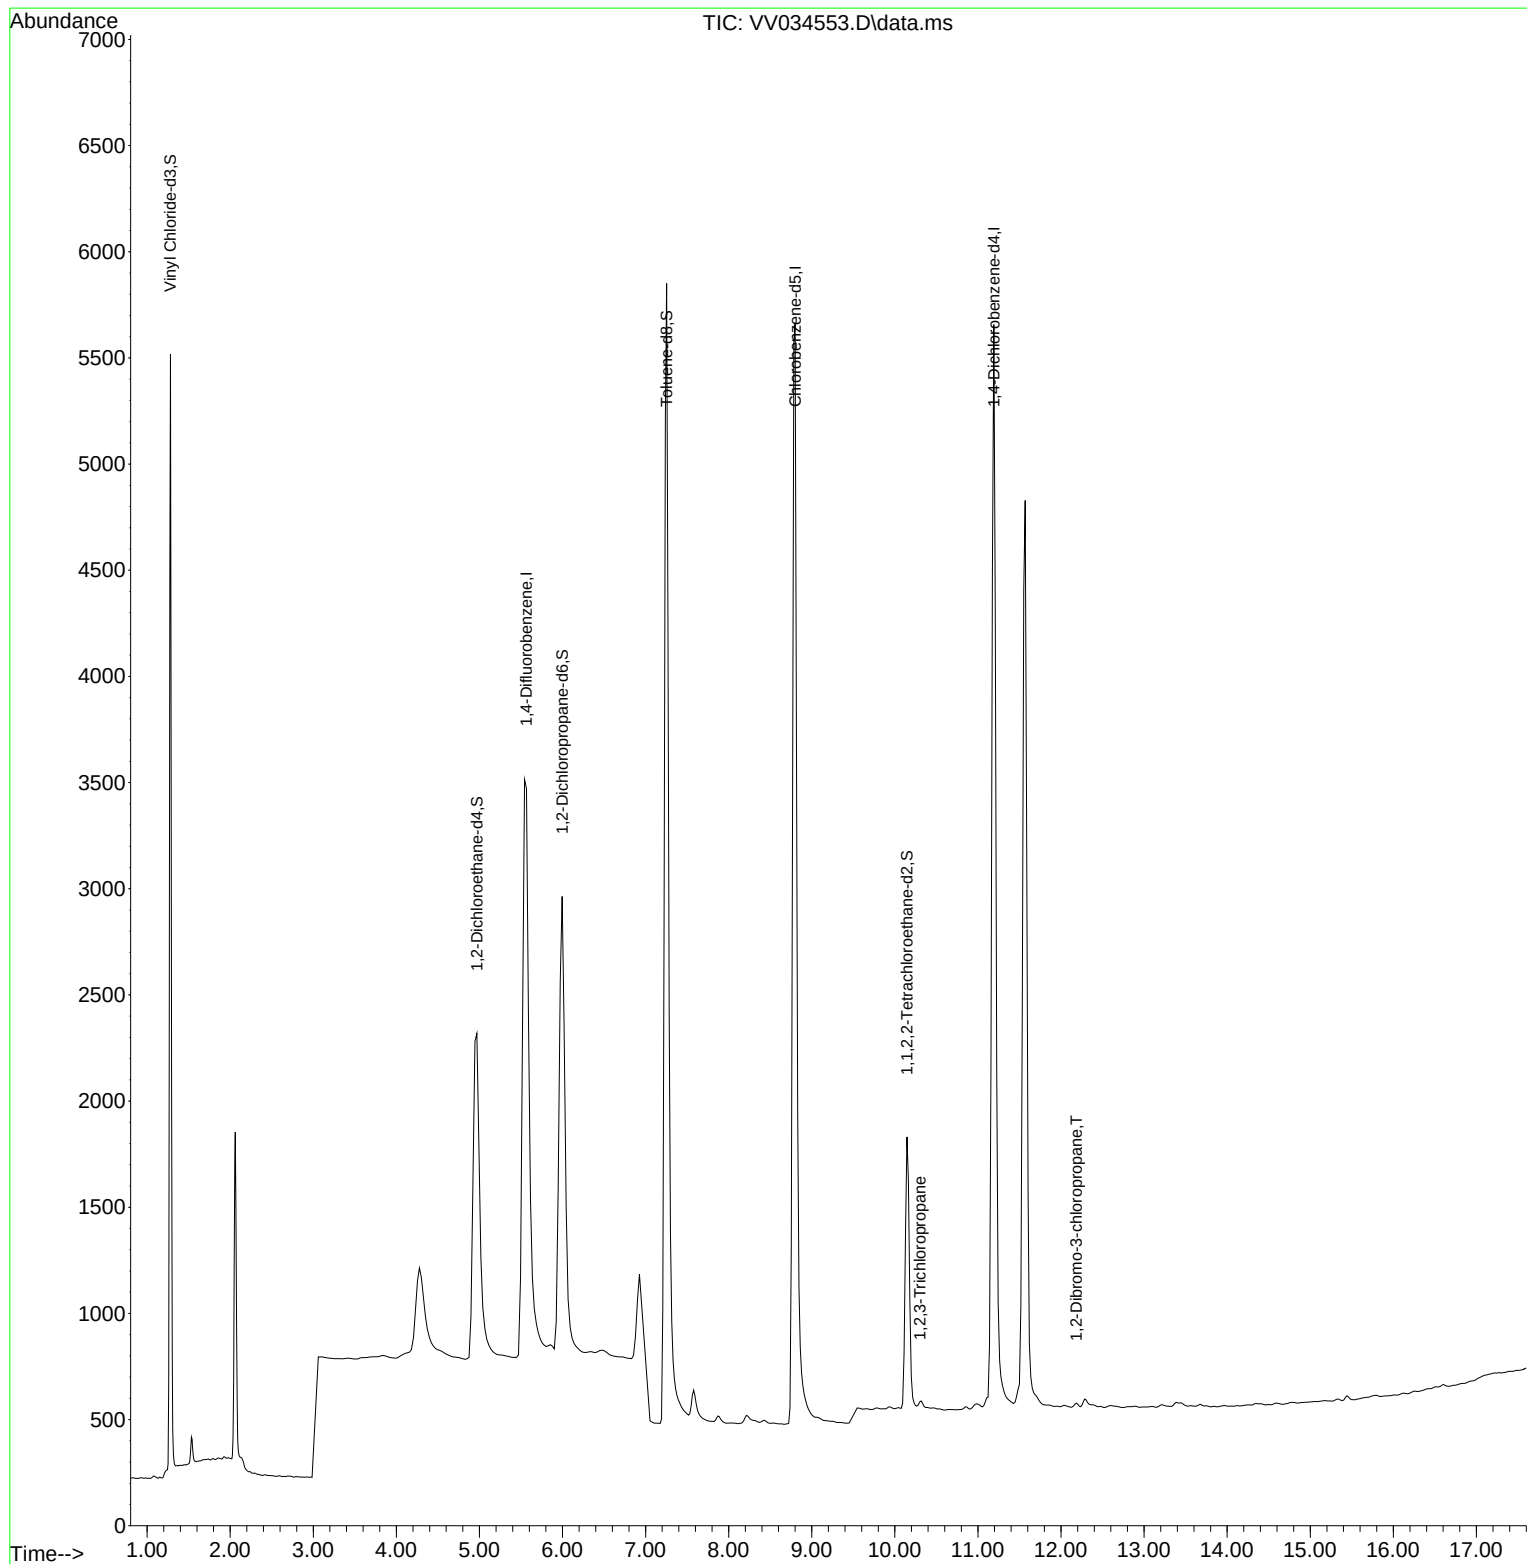



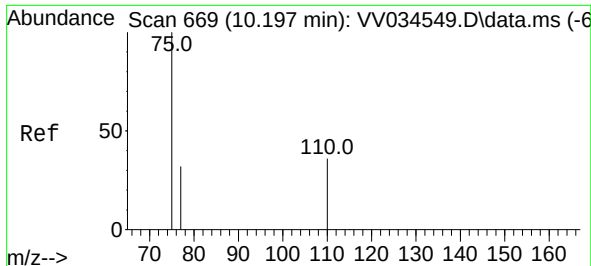


#12
1,2,3-Trichloropropane
Concen: 0.013 ug/L
RT: 10.300 min Scan# 61
Delta R.T. 0.086 min
Lab File: VV034553.D
Acq: 12 Mar 2024 10:48

Instrument :
MSVOA_V
ClientSampleId :

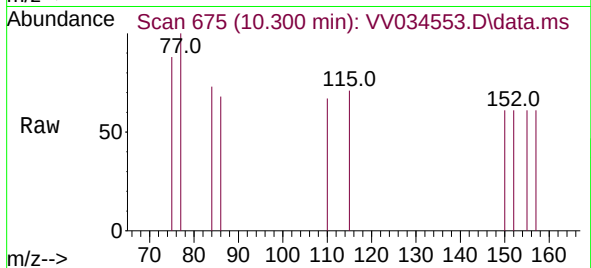

Tgt Ion: 75 Resp: 60
Ion Ratio Lower Upper
75 100
110 31.7 33.1 49.7#
77 6.7 26.2 39.4#

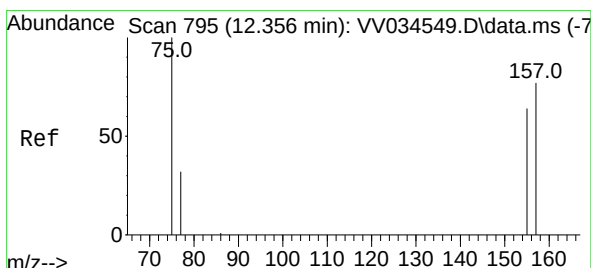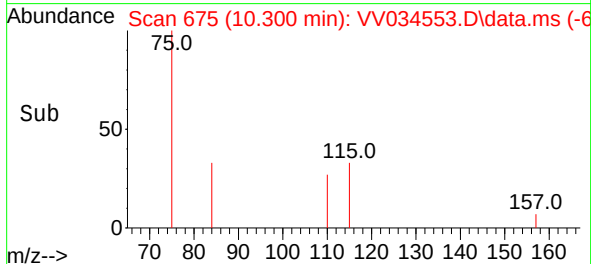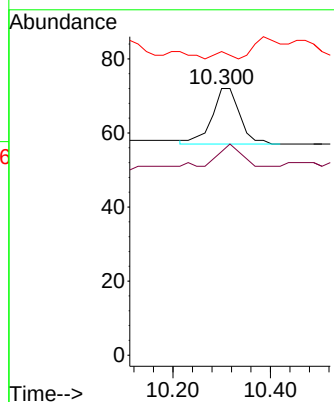

#13
1,2-Dibromo-3-chloropropane
Concen: 0.048 ug/L
RT: 12.185 min Scan# 785
Delta R.T. -0.171 min
Lab File: VV034553.D
Acq: 12 Mar 2024 10:48

Tgt Ion: 75 Resp: 47
Ion Ratio Lower Upper
75 100
157 68.5 62.9 94.3
155 72.6 56.2 84.4

