

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031224\
 Data File : VV034558.D
 Acq On : 12 Mar 2024 15:24
 Operator : SY/MD
 Sample : P1715-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Mar 13 04:58:07 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM030524.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Mar 06 04:17:25 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	11521	0.500	ug/L	-0.02
5) Chlorobenzene-d5	8.800	117	10765	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.191	152	5786	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.280	65	6413	0.519	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	104.000%
4) 1,2-Dichloroethane-d4	4.946	65	4148	0.542	ug/L	-0.02
Spiked Amount	0.500	Range	70 - 130	Recovery	=	108.000%
7) 1,2-Dichloropropane-d6	5.995	67	4378	0.523	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	104.000%
8) Toluene-d8	7.253	98	12229	0.493	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	98.000%
10) 1,1,2,2-Tetrachloroeth...	10.146	84	3204	0.534	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	106.000%
Target Compounds						
					Qvalue	
3) Vinyl chloride	1.280	62	372	0.029	ug/L #	42
6) Trichloroethene	5.852	95	1207	0.143	ug/L	95
12) 1,2,3-Trichloropropane	10.317	75	64	0.013	ug/L #	76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031224\
Data File : VV034558.D
Acq On : 12 Mar 2024 15:24
Operator : SY/MD
Sample : P1715-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Mar 13 04:58:07 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM030524.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Mar 06 04:17:25 2024
Response via : Initial Calibration

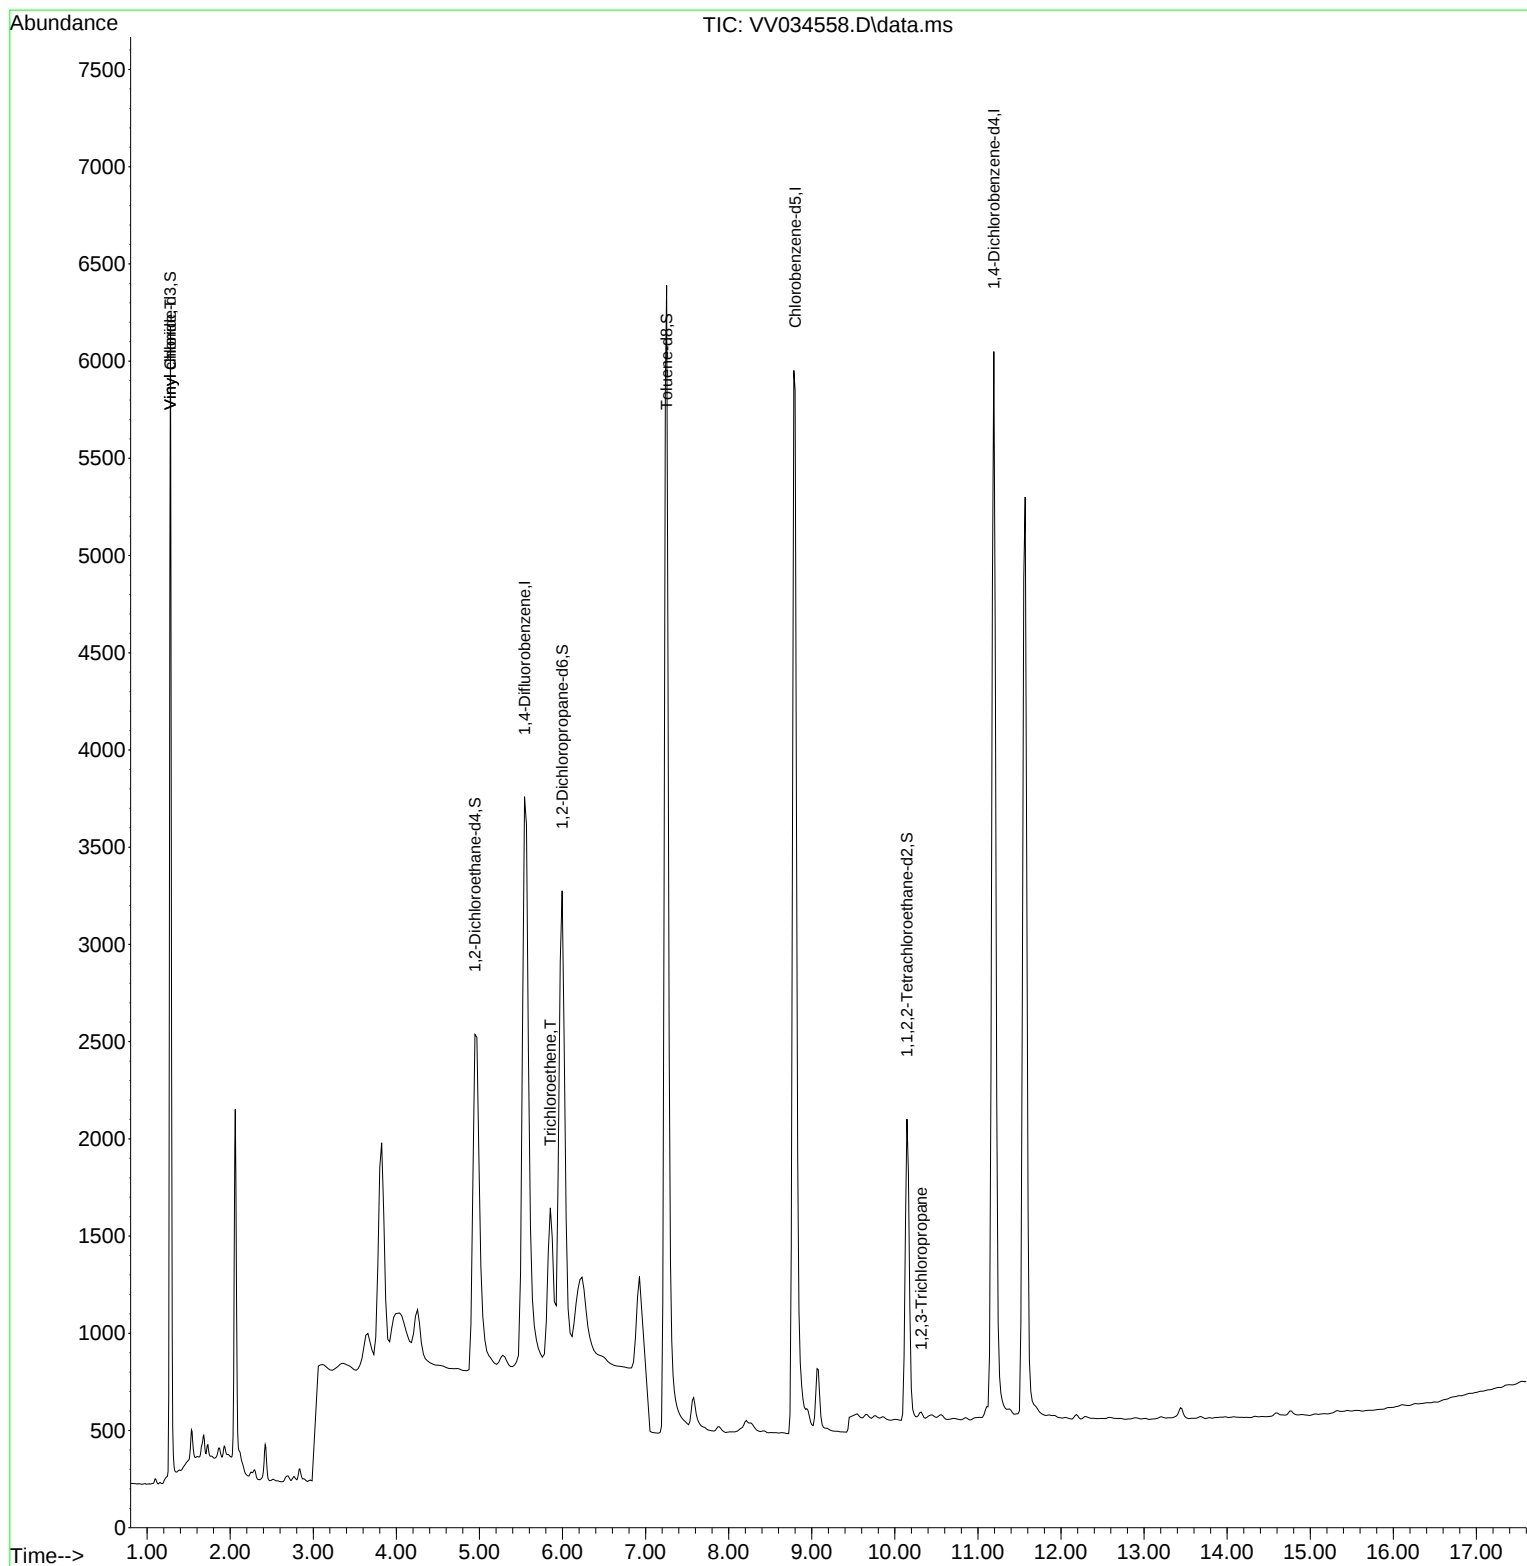

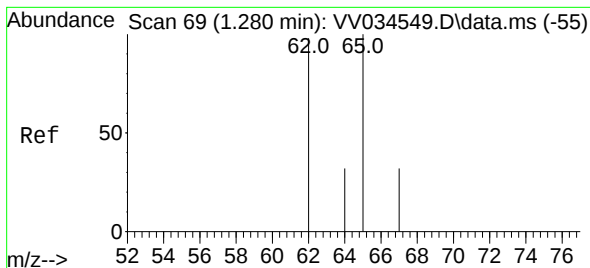

#3

Vinyl chloride

Concen: 0.029 ug/L

RT: 1.280 min Scan# 69

Delta R.T. 0.000 min

Lab File: VV034558.D

Acq: 12 Mar 2024 15:24

Instrument :

MSVOA_V





ClientSampleId :

Tgt Ion: 62 Resp: 372

Ion Ratio Lower Upper

62 100

64 67.3 23.7 44.1#

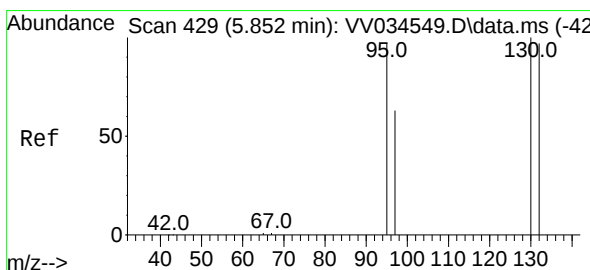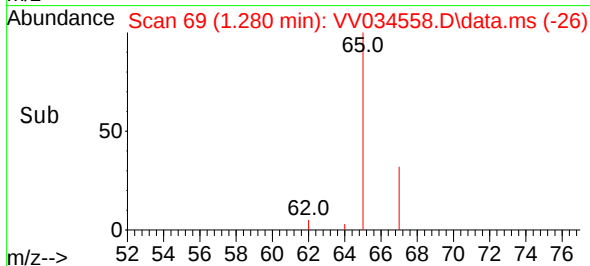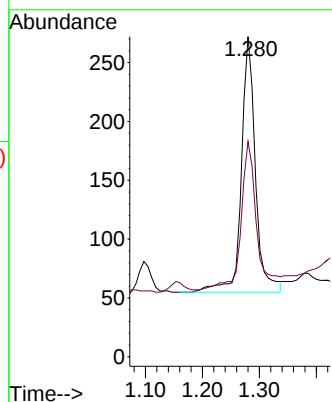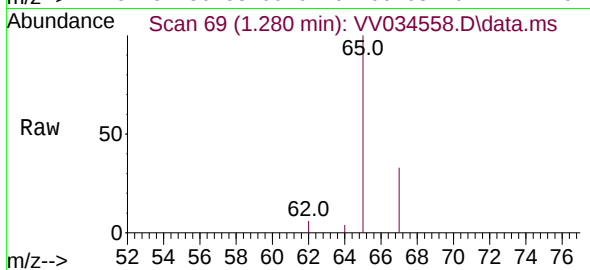

#6

Trichloroethene

Concen: 0.143 ug/L

RT: 5.852 min Scan# 429

Delta R.T. 0.000 min

Lab File: VV034558.D

Acq: 12 Mar 2024 15:24

Tgt Ion: 95 Resp: 1207




Ion Ratio Lower Upper


95 100

97 71.0 47.0 87.2

132 94.6 70.0 130.0


130 97.5 72.4 134.4

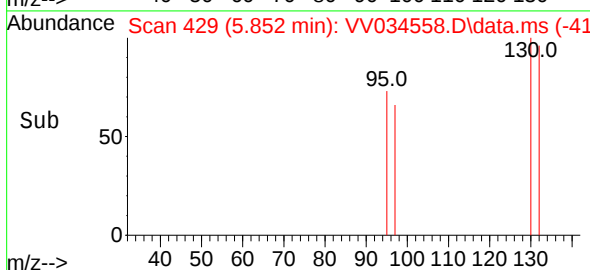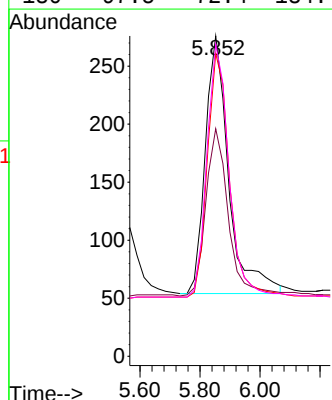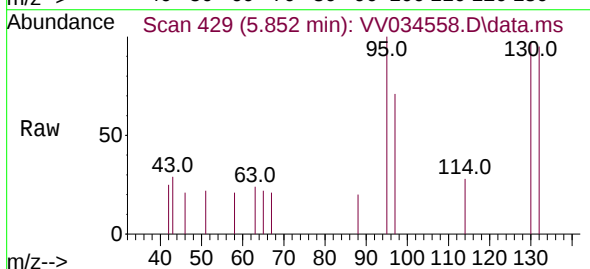

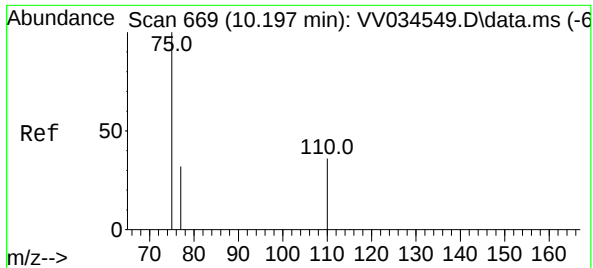

#12
 1,2,3-Trichloropropane
 Concen: 0.013 ug/L
 RT: 10.317 min Scan# 61
 Delta R.T. 0.103 min
 Lab File: VV034558.D
 Acq: 12 Mar 2024 15:24

Instrument :
 MSVOA_V
 ClientSampleId :

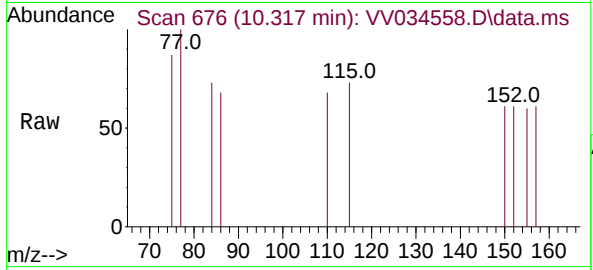

Tgt Ion: 75 Resp: 64

Ion	Ratio	Lower	Upper
75	100		
110	35.9	33.1	49.7
77	7.8	26.2	39.4#

