

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031224\
 Data File : VV034559.D
 Acq On : 12 Mar 2024 15:48
 Operator : SY/MD
 Sample : P1715-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Mar 13 04:58:15 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM030524.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Mar 06 04:17:25 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	11168	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.800	117	10421	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.191	152	5452	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.280	65	5974	0.499	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	100.000%
4) 1,2-Dichloroethane-d4	4.970	65	3820	0.515	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	102.000%
7) 1,2-Dichloropropane-d6	5.996	67	3970	0.490	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	98.000%
8) Toluene-d8	7.254	98	11202	0.467	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	94.000%
10) 1,1,2,2-Tetrachloroeth...	10.146	84	2952	0.508	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	102.000%
Target Compounds						
6) Trichloroethene	5.852	95	3635	0.445	ug/L	99
13) 1,2-Dibromo-3-chloropr...	12.185	75	42	0.043	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031224\
Data File : VV034559.D
Acq On : 12 Mar 2024 15:48
Operator : SY/MD
Sample : P1715-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Mar 13 04:58:15 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM030524.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Mar 06 04:17:25 2024
Response via : Initial Calibration

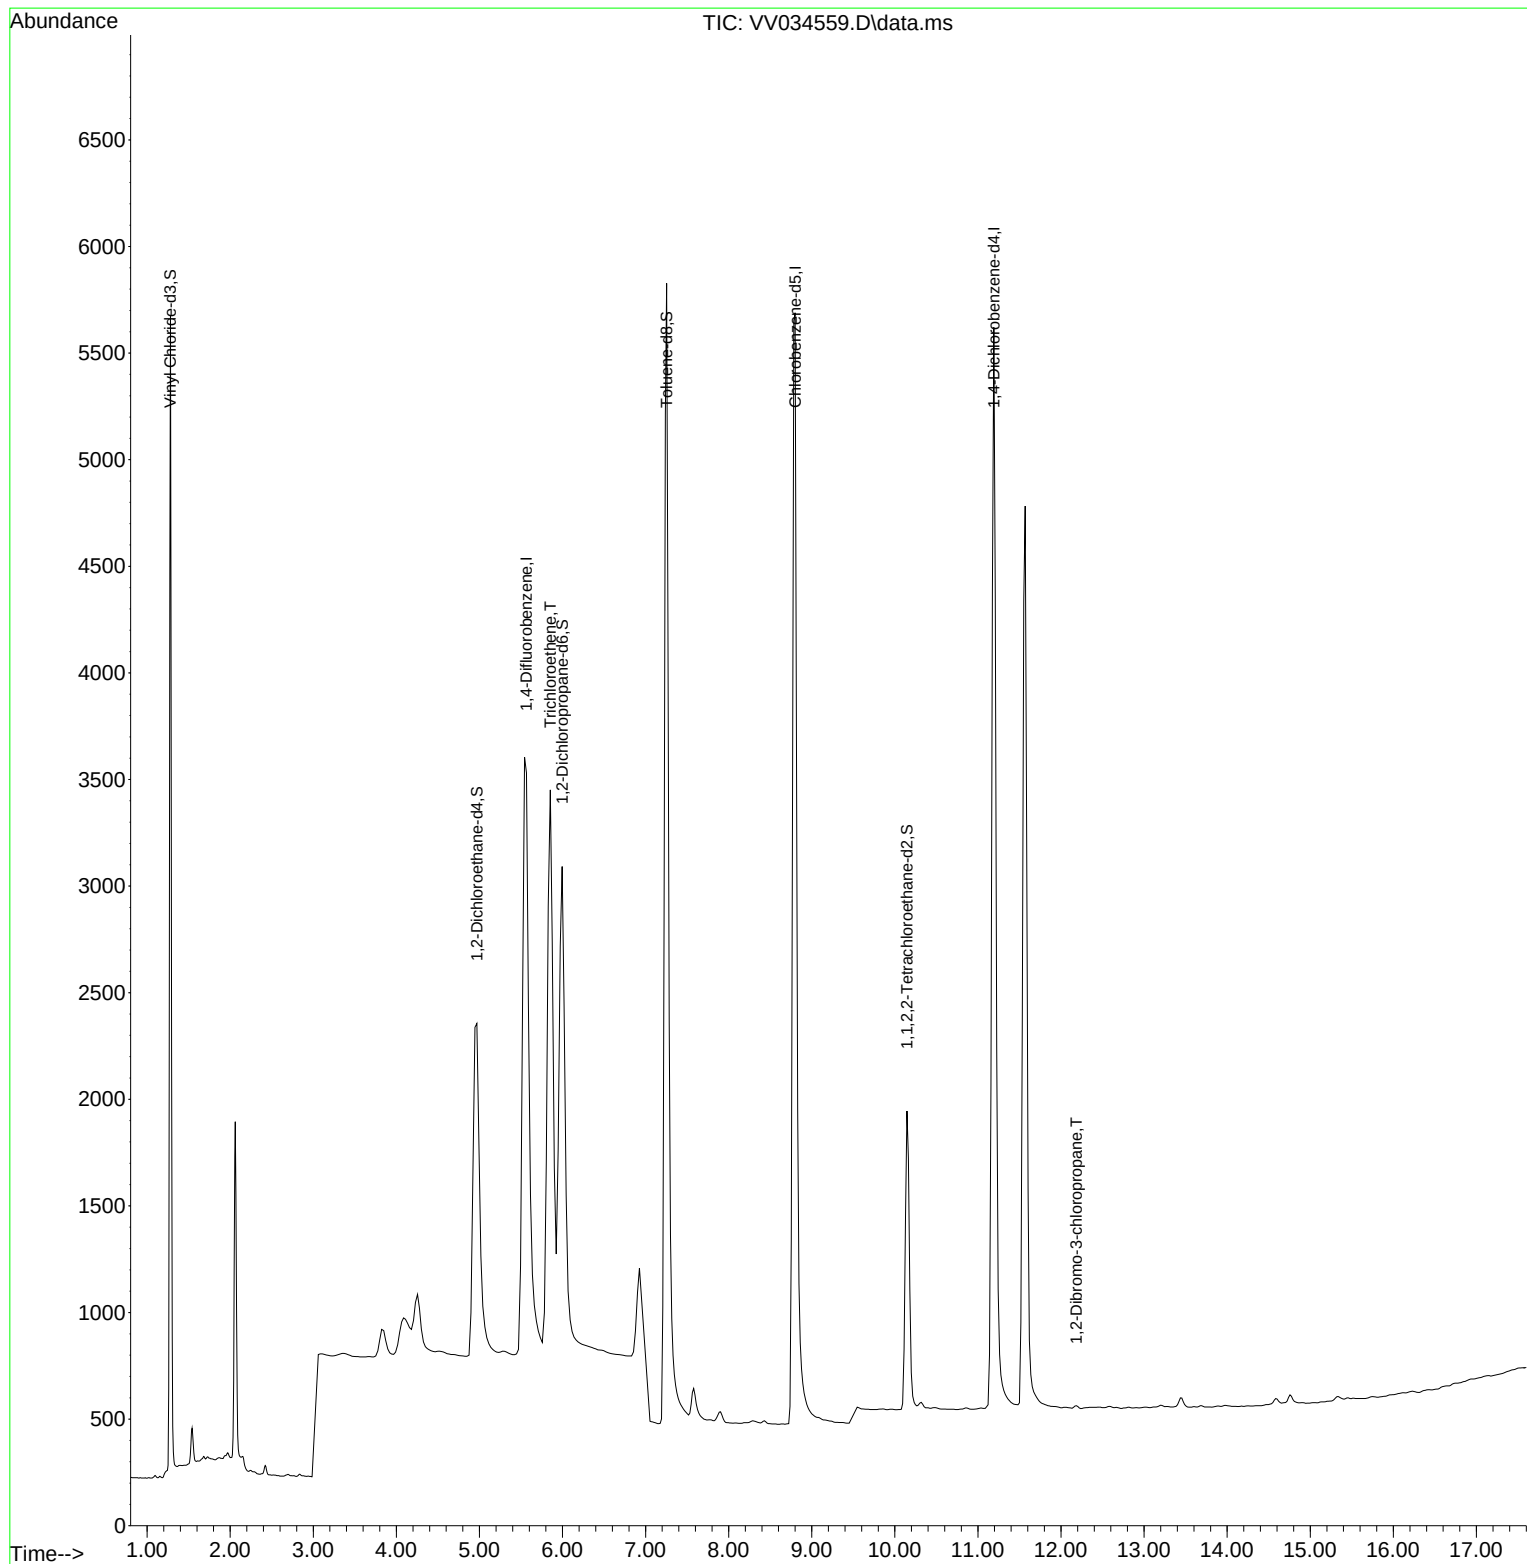

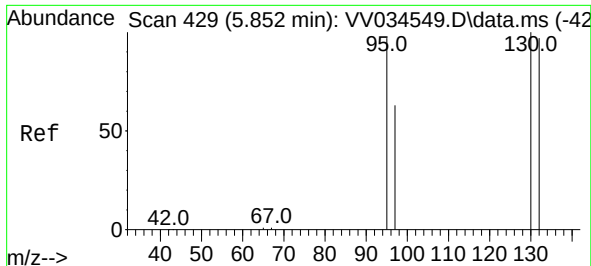

#6

Trichloroethene

Concen: 0.445 ug/L

RT: 5.852 min Scan# 41

Delta R.T. 0.000 min


Lab File: VV034559.D

Acq: 12 Mar 2024 15:48

Instrument :

MSVOA_V

ClientSampleId :

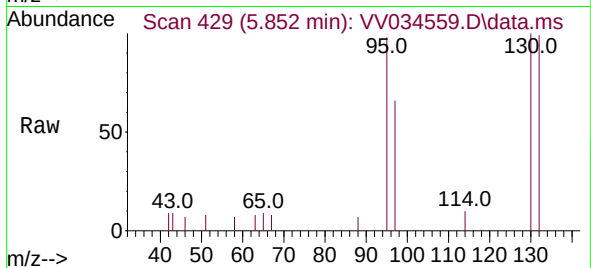

Tgt Ion: 95 Resp: 3635




Ion Ratio Lower Upper

95 100

97 67.5 47.0 87.2

132 100.7 70.0 130.0

130 101.6 72.4 134.4

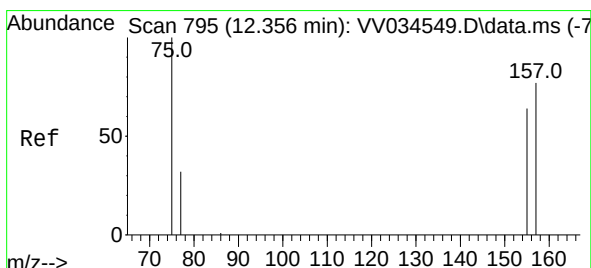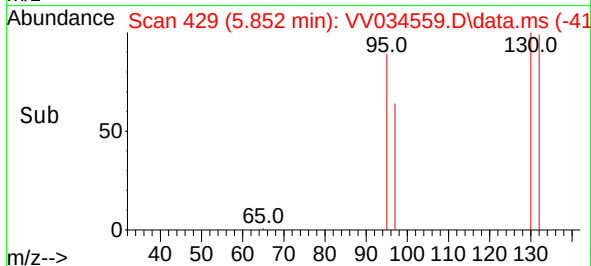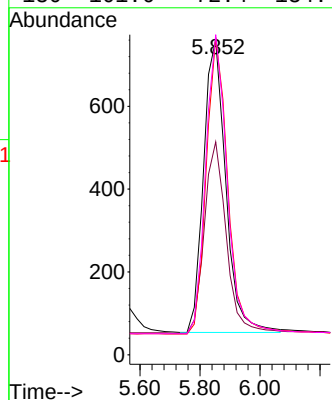

#13

1,2-Dibromo-3-chloropropane

Concen: 0.043 ug/L

RT: 12.185 min Scan# 785

Delta R.T. -0.171 min

Lab File: VV034559.D

Acq: 12 Mar 2024 15:48

Tgt Ion: 75 Resp: 42

Ion Ratio Lower Upper

75 100

157 72.5 62.9 94.3

155 73.9 56.2 84.4

