

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW031224\
 Data File : VW034557.D
 Acq On : 12 Mar 2024 15:00
 Operator : SY/MD
 Sample : P1715-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGQM0

Quant Time: Mar 13 04:57:59 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM030524.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Mar 06 04:17:25 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	12425	0.500	ug/L	-0.02
5) Chlorobenzene-d5	8.785	117	11783	0.500	ug/L	-0.02
11) 1,4-Dichlorobenzene-d4	11.191	152	6301	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.280	65	6554	0.492	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	98.000%
4) 1,2-Dichloroethane-d4	4.946	65	3844	0.466	ug/L	-0.02
Spiked Amount	0.500	Range	70 - 130	Recovery	=	94.000%
7) 1,2-Dichloropropane-d6	5.995	67	4261	0.465	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	94.000%
8) Toluene-d8	7.238	98	12018	0.443	ug/L	-0.02
Spiked Amount	0.500	Range	70 - 130	Recovery	=	88.000%
10) 1,1,2,2-Tetrachloroeth...	10.146	84	2807	0.427	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	86.000%
Target Compounds						
					Qvalue	
3) Vinyl chloride	1.280	62	617	0.044	ug/L	# 28
6) Trichloroethene	5.852	95	1958	0.212	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031224\
Data File : VV034557.D
Acq On : 12 Mar 2024 15:00
Operator : SY/MD
Sample : P1715-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGQM0

Quant Time: Mar 13 04:57:59 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM030524.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Mar 06 04:17:25 2024
Response via : Initial Calibration

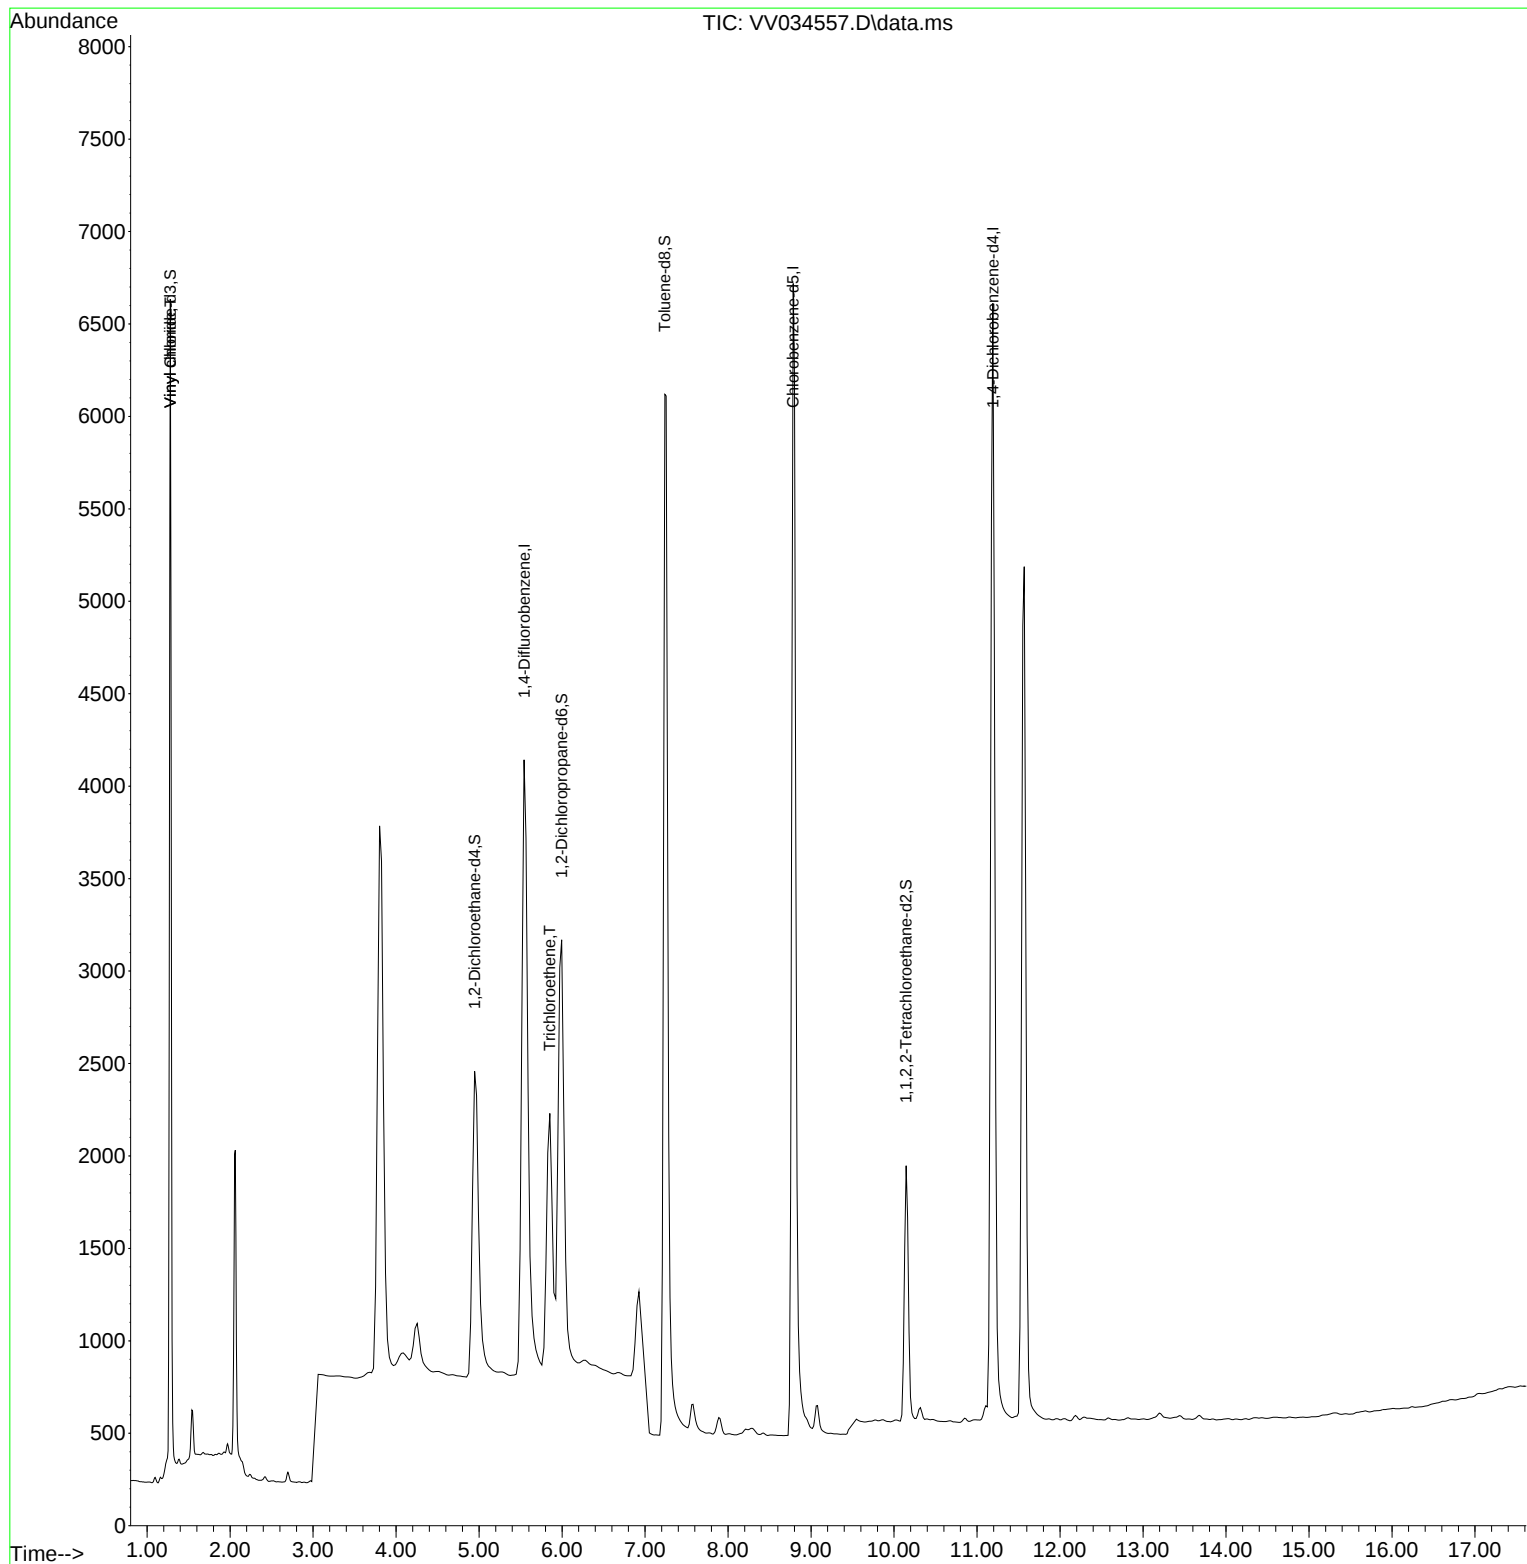

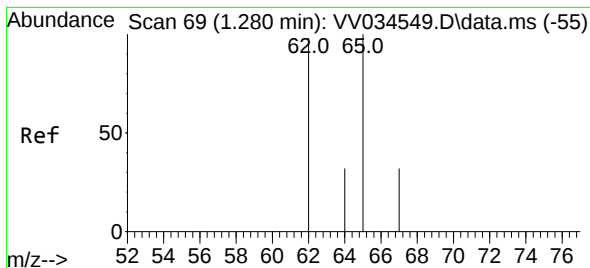

#3

Vinyl chloride

Concen: 0.044 ug/L

RT: 1.280 min Scan# 69

Delta R.T. 0.000 min

Lab File: VV034557.D

Acq: 12 Mar 2024 15:00

Instrument :

MSVOA_V

ClientSampleId :





BGQM0

Tgt Ion: 62 Resp: 617

Ion Ratio Lower Upper

62 100

64 75.1 23.7 44.1#

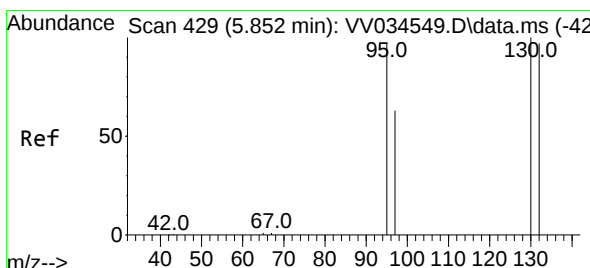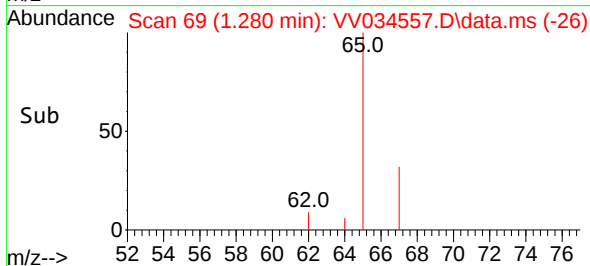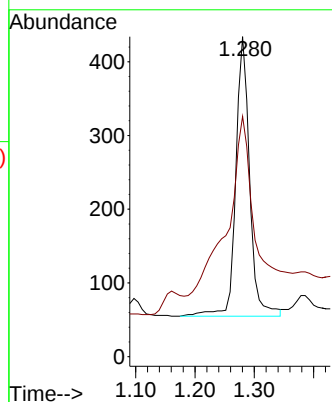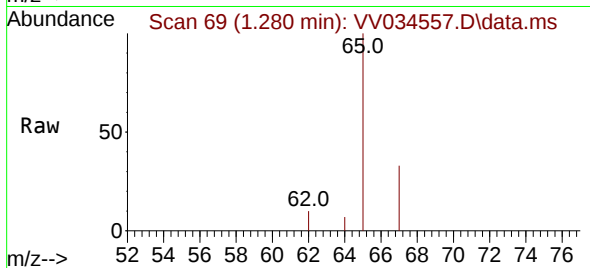

#6

Trichloroethene

Concen: 0.212 ug/L

RT: 5.852 min Scan# 429

Delta R.T. 0.000 min

Lab File: VV034557.D

Acq: 12 Mar 2024 15:00

Tgt Ion: 95 Resp: 1958

Ion Ratio Lower Upper

95 100

97 69.1 47.0 87.2

132 98.8 70.0 130.0

130 101.4 72.4 134.4

