

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031319\
 Data File : VV009655.D
 Acq On : 14 Mar 2019 00:01
 Operator : SY/MD
 Sample : K1794-18
 Misc : 5.14G/10ML/MSVOA V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BF5P5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM031319S.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.126	314	322	337	rVB	51098	74607	25.68%	4.790%
2	2.360	392	395	402	rBV2	352	375	0.13%	0.024%
3	2.444	419	421	422	rBV	214	71	0.02%	0.005%
4	2.534	440	449	465	rVB4	13239	21718	7.48%	1.394%
5	2.650	475	485	501	rBV2	4931	10422	3.59%	0.669%
6	2.801	529	532	541	rBV2	261	276	0.10%	0.018%
7	2.974	582	586	587	rBV2	232	135	0.05%	0.009%
8	3.023	597	601	603	rBV2	309	198	0.07%	0.013%
9	3.068	609	615	619	rBV6	1010	1433	0.49%	0.092%
10	3.228	662	665	666	rBV	252	153	0.05%	0.010%
11	3.328	694	696	697	rBV	156	37	0.01%	0.002%
12	3.389	712	715	718	rBV2	218	135	0.05%	0.009%
13	3.785	835	838	840	rBV2	269	178	0.06%	0.011%
14	3.926	878	882	883	rBV	326	207	0.07%	0.013%
15	4.399	1014	1029	1050	rBV2	56726	136708	47.06%	8.777%
16	4.569	1080	1082	1086	rBV2	281	168	0.06%	0.011%
17	4.614	1092	1096	1098	rBV	384	272	0.09%	0.017%
18	4.679	1113	1116	1120	rBV	214	132	0.05%	0.008%
19	4.791	1149	1151	1153	rBV	234	149	0.05%	0.010%
20	4.871	1173	1176	1177	rBV	130	76	0.03%	0.005%
21	4.958	1196	1203	1210	rBV2	319	637	0.22%	0.041%
22	5.010	1216	1219	1224	rVB2	193	163	0.06%	0.010%
23	5.035	1224	1227	1228	rBV2	145	91	0.03%	0.006%
24	5.093	1228	1245	1263	rBV3	113485	290500	100.00%	18.650%
25	5.389	1332	1337	1340	rBV2	279	338	0.12%	0.022%
26	5.453	1355	1357	1358	rBV	138	66	0.02%	0.004%
27	5.482	1363	1366	1372	rBV2	202	180	0.06%	0.012%
28	5.662	1410	1422	1447	rBV	80963	162522	55.95%	10.434%
29	5.849	1479	1480	1482	rVB	110	39	0.01%	0.003%
30	5.862	1482	1484	1487	rBV2	119	84	0.03%	0.005%
31	5.923	1497	1503	1505	rBV2	427	330	0.11%	0.021%
32	5.942	1505	1509	1512	rBV2	1296	1392	0.48%	0.089%
33	6.023	1532	1534	1538	rBB2	168	78	0.03%	0.005%
34	6.119	1551	1564	1584	rBV	78101	160448	55.23%	10.301%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031319\
 Data File : VV009655.D
 Acq On : 14 Mar 2019 00:01
 Operator : SY/MD
 Sample : K1794-18
 Misc : 5.14G/10ML/MSVOA V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BF5P5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM031319S.M
 Title : VOC Analysis

35	6.331	1627	1630	1632	rBV2	174	116	0.04%	0.007%
36	6.553	1696	1699	1701	rBV	142	70	0.02%	0.004%
37	6.592	1708	1711	1714	rVB	1563	852	0.29%	0.055%
38	6.929	1813	1816	1818	rBV	228	159	0.05%	0.010%
39	7.035	1836	1849	1858	rBV7	2823	5431	1.87%	0.349%
40	7.132	1872	1879	1893	rVB4	2466	4734	1.63%	0.304%
41	7.289	1924	1928	1929	rBV2	537	389	0.13%	0.025%
42	7.360	1938	1950	1968	rBV	103046	182597	62.86%	11.723%
43	7.521	1998	2000	2001	rBV	175	66	0.02%	0.004%
44	7.569	2014	2015	2016	rBV	142	37	0.01%	0.002%
45	7.582	2016	2019	2023	rVV	318	252	0.09%	0.016%
46	7.669	2038	2046	2054	rBV3	2627	4020	1.38%	0.258%
47	7.727	2059	2064	2066	rBV2	423	305	0.10%	0.020%
48	7.945	2130	2132	2133	rBV2	159	72	0.02%	0.005%
49	7.984	2136	2144	2151	rVV5	2417	3675	1.27%	0.236%
50	8.055	2163	2166	2168	rBV2	224	148	0.05%	0.010%
51	8.167	2199	2201	2202	rBV	540	239	0.08%	0.015%
52	8.280	2234	2236	2238	rBV	204	126	0.04%	0.008%
53	8.395	2268	2272	2276	rVB2	362	320	0.11%	0.021%
54	8.418	2276	2279	2282	rBV	207	133	0.05%	0.009%
55	8.440	2282	2286	2288	rBV2	147	121	0.04%	0.008%
56	8.466	2290	2294	2297	rBV2	1050	1099	0.38%	0.071%
57	8.553	2318	2321	2325	rBV	239	158	0.05%	0.010%
58	8.662	2352	2355	2356	rBV2	155	98	0.03%	0.006%
59	8.897	2415	2428	2443	rBV	105292	180620	62.18%	11.596%
60	9.260	2537	2541	2544	rVB2	315	199	0.07%	0.013%
61	9.289	2544	2550	2552	rBV2	137	168	0.06%	0.011%
62	9.511	2616	2619	2623	rBV2	268	182	0.06%	0.012%
63	9.884	2730	2735	2739	rBV2	179	212	0.07%	0.014%
64	10.164	2819	2822	2823	rBV	128	63	0.02%	0.004%
65	10.190	2827	2830	2833	rBV	328	206	0.07%	0.013%
66	10.264	2842	2853	2869	rBV	65589	105023	36.15%	6.743%
67	10.428	2895	2904	2914	rBV4	5369	8273	2.85%	0.531%
68	10.518	2929	2932	2933	rBV	250	153	0.05%	0.010%
69	10.710	2989	2992	2996	rBV2	205	169	0.06%	0.011%
70	10.958	3065	3069	3072	rVB3	324	229	0.08%	0.015%
71	10.993	3077	3080	3084	rBV	158	98	0.03%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031319\
 Data File : VV009655.D
 Acq On : 14 Mar 2019 00:01
 Operator : SY/MD
 Sample : K1794-18
 Misc : 5.14G/10ML/MSVOA V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BF5P5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM031319S.M
 Title : VOC Analysis

72	11.296	3164	3174	3195	rVB	55289	92582	31.87%	5.944%
73	11.444	3217	3220	3225	rVB2	381	239	0.08%	0.015%
74	11.469	3225	3228	3231	rBV2	247	209	0.07%	0.013%
75	11.495	3234	3236	3239	rBV2	153	59	0.02%	0.004%
76	11.601	3261	3269	3271	rBV2	323	369	0.13%	0.024%
77	11.675	3281	3292	3308	rVV	57048	95597	32.91%	6.137%
78	11.733	3308	3310	3313	rVB2	222	76	0.03%	0.005%
79	11.881	3354	3356	3360	rBV2	224	101	0.03%	0.006%
80	12.106	3424	3426	3429	rBV	116	45	0.02%	0.003%
81	12.125	3429	3432	3434	rBV	209	152	0.05%	0.010%
82	12.157	3439	3442	3445	rBV	178	146	0.05%	0.009%
83	12.366	3501	3507	3509	rBV2	225	256	0.09%	0.016%
84	12.424	3523	3525	3528	rBV	218	157	0.05%	0.010%
85	12.479	3540	3542	3543	rBV	235	54	0.02%	0.003%
86	12.524	3554	3556	3559	rBV	148	100	0.03%	0.006%
87	12.614	3581	3584	3585	rBV	200	116	0.04%	0.007%
88	12.926	3676	3681	3684	rBV2	300	328	0.11%	0.021%
89	12.980	3695	3698	3699	rBV2	267	155	0.05%	0.010%
90	13.305	3796	3799	3803	rBV	249	216	0.07%	0.014%
91	13.350	3809	3813	3816	rBV2	400	326	0.11%	0.021%
92	13.836	3963	3964	3970	rBV2	290	222	0.08%	0.014%
93	13.952	3997	4000	4001	rBV2	155	83	0.03%	0.005%
94	14.025	4021	4023	4025	rBV	210	128	0.04%	0.008%
95	14.495	4167	4169	4173	rVB3	322	200	0.07%	0.013%
96	14.681	4223	4227	4230	rBV2	640	572	0.20%	0.037%


Sum of corrected areas: 1557618

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV031319\
Data File : VV009655.D
Acq On : 14 Mar 2019 00:01
Operator : SY/MD
Sample : K1794-18
Misc : 5.14G/10ML/MSVOA V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BF5P5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM031319S.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

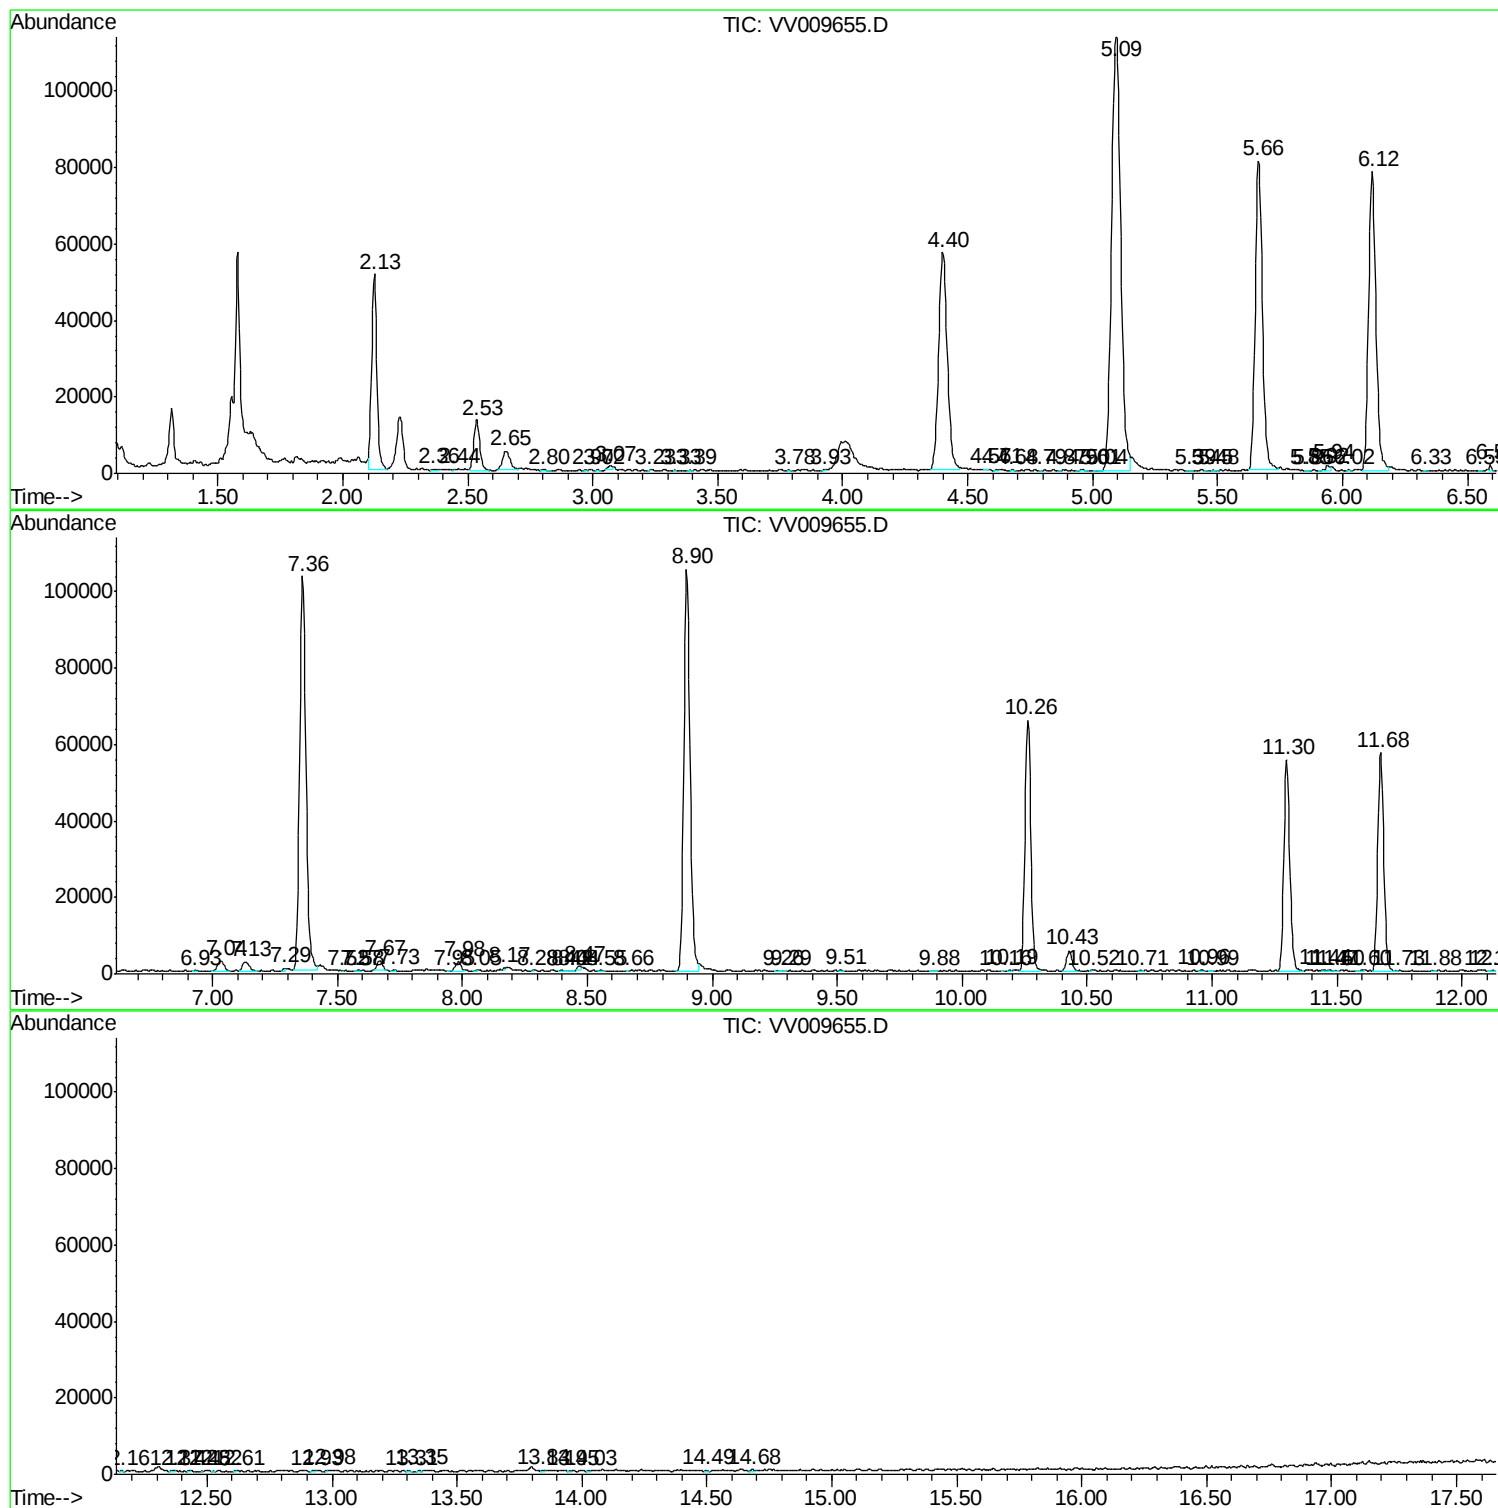

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV031319\
Data File : VV009655.D
Acq On : 14 Mar 2019 00:01
Operator : SY/MD
Sample : K1794-18
Misc : 5.14G/10ML/MSV0A_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BF5P5

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOM2VLM031319S.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV031319\
Data File : VV009655.D
Acq On : 14 Mar 2019 00:01
Operator : SY/MD
Sample : K1794-18
Misc : 5.14G/10ML/MSV0A_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BF5P5

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOM2VLM031319S.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc