


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV031319\
 Data File : VV009630.D
 Acq On : 13 Mar 2019 09:18
 Operator : SY/MD
 Sample : BFB75
 Misc : 5.00G/10mL/MSVOA V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB75

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM031319S.M
 Title : VOC Analysis
 Last Update : Fri Mar 15 04:30:02 2019

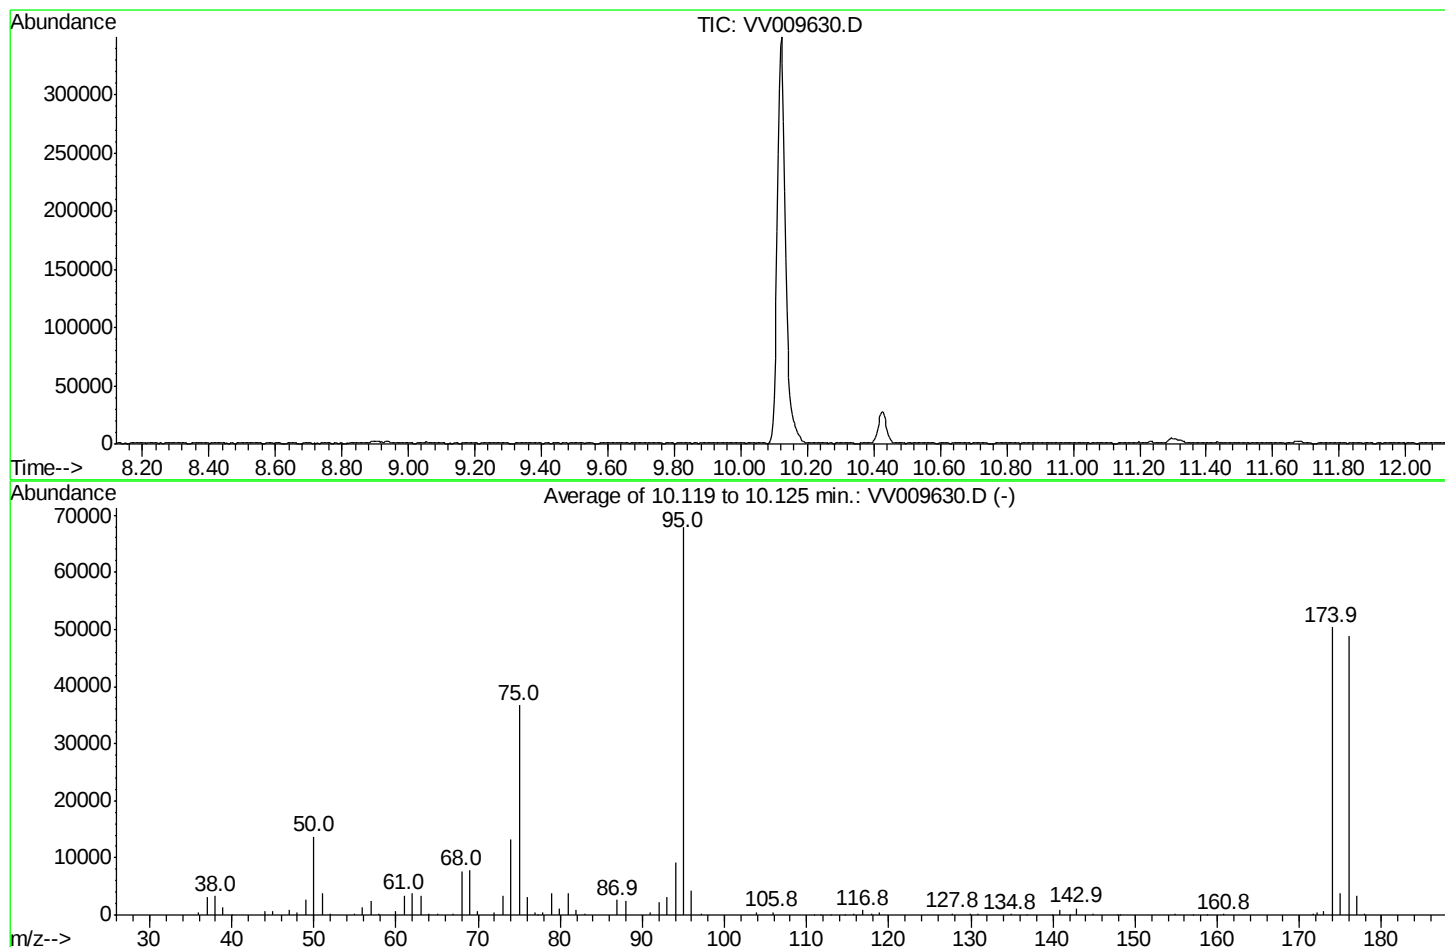

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	13708	PASS
75	95	30	80	54.1	36706	PASS
95	95	100	100	100.0	67866	PASS
96	95	5	9	6.4	4369	PASS
173	174	0.00	2	1.3	632	PASS
174	95	50	120	74.2	50378	PASS
175	174	5	9	7.6	3844	PASS
176	174	95	101	97.1	48912	PASS
177	176	5	9	6.9	3397	PASS

Scan 2796 (10.080 min): VV009630.D
BFB75

m/z	Abundance
39.90	428.0
43.90	144.0

Instrument :
MSVOA_V
ClientSampleId :
BFB75

m/z	Abundance
35.90	584.0
37.00	3200.0
38.00	3395.0
38.90	1304.0
39.90	521.0
44.00	763.0
45.00	788.0
46.90	741.0
47.90	354.0
49.00	2562.0
50.00	13953.0
51.00	3926.0
51.90	171.0
54.90	205.0
55.90	1343.0
57.00	2469.0
57.90	193.0
60.00	669.0
61.00	3461.0
62.00	3828.0
63.00	3398.0
64.00	299.0
65.10	208.0
67.00	214.0
68.00	7881.0
69.00	8149.0
70.00	736.0
72.00	438.0
73.00	3524.0
74.00	13198.0
75.00	38144.0
76.00	3282.0
76.90	414.0
77.90	338.0
78.90	4091.0
79.90	1119.0
80.90	3912.0
82.00	786.0
83.00	135.0
86.90	2723.0
87.90	2395.0
90.90	378.0
92.00	2272.0
92.90	3292.0
94.00	9130.0
95.00	69088.0
96.00	4329.0
97.10	172.0
103.90	427.0
105.80	540.0
111.70	106.0
112.90	127.0
115.80	321.0
116.90	745.0
117.90	256.0
118.80	539.0
127.80	342.0
130.00	293.0
130.80	115.0
134.80	201.0
136.70	176.0
140.90	921.0
142.00	119.0
142.90	1206.0
145.00	225.0
147.90	123.0
154.80	163.0
157.00	133.0
158.80	147.0
160.80	158.0
172.10	432.0
174.00	49624.0
175.00	3886.0
176.00	48184.0
177.00	3490.0
177.90	165.0

Instrument :
MSVOA_V
ClientSampleId :
BFB75

m/z	Abundance
35.90	590.0
37.00	3260.0
38.00	3340.0
38.90	1371.0
39.90	534.0
44.00	724.0
44.90	771.0
47.00	864.0
47.90	413.0
49.00	2707.0
50.00	14093.0
51.00	4004.0
51.90	164.0
54.90	231.0
55.90	1329.0
57.00	2496.0
57.90	168.0
60.00	681.0
61.00	3531.0
62.00	3923.0
63.00	3378.0
63.90	309.0
65.10	220.0
67.00	231.0
68.00	7848.0
69.00	8092.0
70.00	752.0
71.90	368.0
73.00	3415.0
74.00	13450.0
75.00	37704.0
76.00	3180.0
76.90	444.0
77.90	372.0
78.90	4040.0
79.80	1116.0
80.90	3988.0
81.90	813.0
83.10	136.0
86.90	2641.0
87.90	2443.0
90.90	413.0
92.00	2278.0
92.90	3275.0
94.00	9315.0
95.00	70232.0
96.00	4537.0
97.10	178.0
103.90	466.0
105.80	542.0
110.90	115.0
111.70	106.0
112.90	128.0
114.70	122.0
115.80	328.0
116.80	856.0
117.80	299.0
118.90	507.0
127.80	326.0
129.90	277.0
130.80	148.0
134.90	199.0
136.70	134.0
140.80	923.0
142.90	1252.0
145.00	167.0
148.10	129.0
154.80	172.0
157.00	111.0
158.80	126.0
160.80	202.0
171.70	353.0
172.10	476.0
172.90	936.0
173.90	51864.0
175.00	3909.0
176.00	50504.0
177.00	3504.0
177.90	176.0

Instrument :
MSVOA_V
ClientSampleId :
BFB75

m/z	Abundance
36.00	519.0
37.00	3068.0
38.00	3185.0
39.00	1283.0
39.90	525.0
44.10	656.0
44.90	690.0
47.00	859.0
47.80	427.0
49.00	2764.0
50.00	13079.0
51.00	3816.0
52.00	135.0
55.00	222.0
55.90	1224.0
57.00	2291.0
57.90	118.0
60.00	629.0
61.00	3320.0
62.00	3713.0
63.00	3057.0
63.90	267.0
65.10	198.0
67.00	233.0
68.00	7178.0
69.00	7304.0
69.90	697.0
71.80	303.0
73.00	3168.0
74.00	12995.0
75.00	34272.0
76.00	2681.0
76.80	379.0
77.20	359.0
77.90	349.0
78.90	3619.0
79.90	958.0
80.90	3677.0
81.90	810.0
83.10	135.0
86.90	2419.0
88.00	2301.0
90.90	372.0
92.00	2133.0
92.90	2925.0
94.00	8887.0
95.00	64280.0
96.00	4241.0
97.20	160.0
103.90	481.0
105.90	472.0
110.90	120.0
111.70	106.0
112.80	103.0
114.70	136.0
115.70	317.0
116.80	796.0
117.80	327.0
118.90	484.0
127.80	278.0
129.90	288.0
130.80	172.0
134.90	180.0
139.90	107.0
140.80	828.0
142.90	1217.0
144.90	132.0
147.70	109.0
148.20	150.0
154.80	172.0
160.90	204.0
171.70	316.0
172.10	447.0
172.90	961.0
173.90	49648.0
175.00	3738.0
176.00	48048.0
177.00	3197.0
177.90	143.0

Instrument :
MSVOA_V
ClientSampleId :
BFB75